

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006869.D
 Acq On : 25 Aug 2021 03:55
 Operator : CG/JU
 Sample : M3468-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SAMPLE-5-(184.50)

Quant Time: Aug 25 04:55:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 13:40:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	172020	20.000	ng	0.00
21) Naphthalene-d8	10.463	136	703334	20.000	ng	#-0.01
39) Acenaphthene-d10	14.328	164	391465	20.000	ng	-0.01
64) Phenanthrene-d10	17.086	188	787194	20.000	ng	#-0.01
76) Chrysene-d12	21.186	240	777825	20.000	ng	#-0.02
86) Perylene-d12	23.492	264	838588	20.000	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.293	112	1444753	129.000	ng	0.00
7) Phenol-d6	6.875	99	1582142	99.448	ng	0.00
23) Nitrobenzene-d5	8.846	82	1384246	90.843	ng	0.00
42) 2,4,6-Tribromophenol	15.828	330	665965	162.778	ng	-0.02
45) 2-Fluorobiphenyl	12.951	172	2490786	95.195	ng	0.00
79) Terphenyl-d14	19.669	244	3870790	99.717	ng	-0.02


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006869.D
Acq On : 25 Aug 2021 03:55
Operator : CG/JU
Sample : M3468-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SAMPLE-5-(184.50)

Quant Time: Aug 25 04:55:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 13:40:38 2021
Response via : Initial Calibration




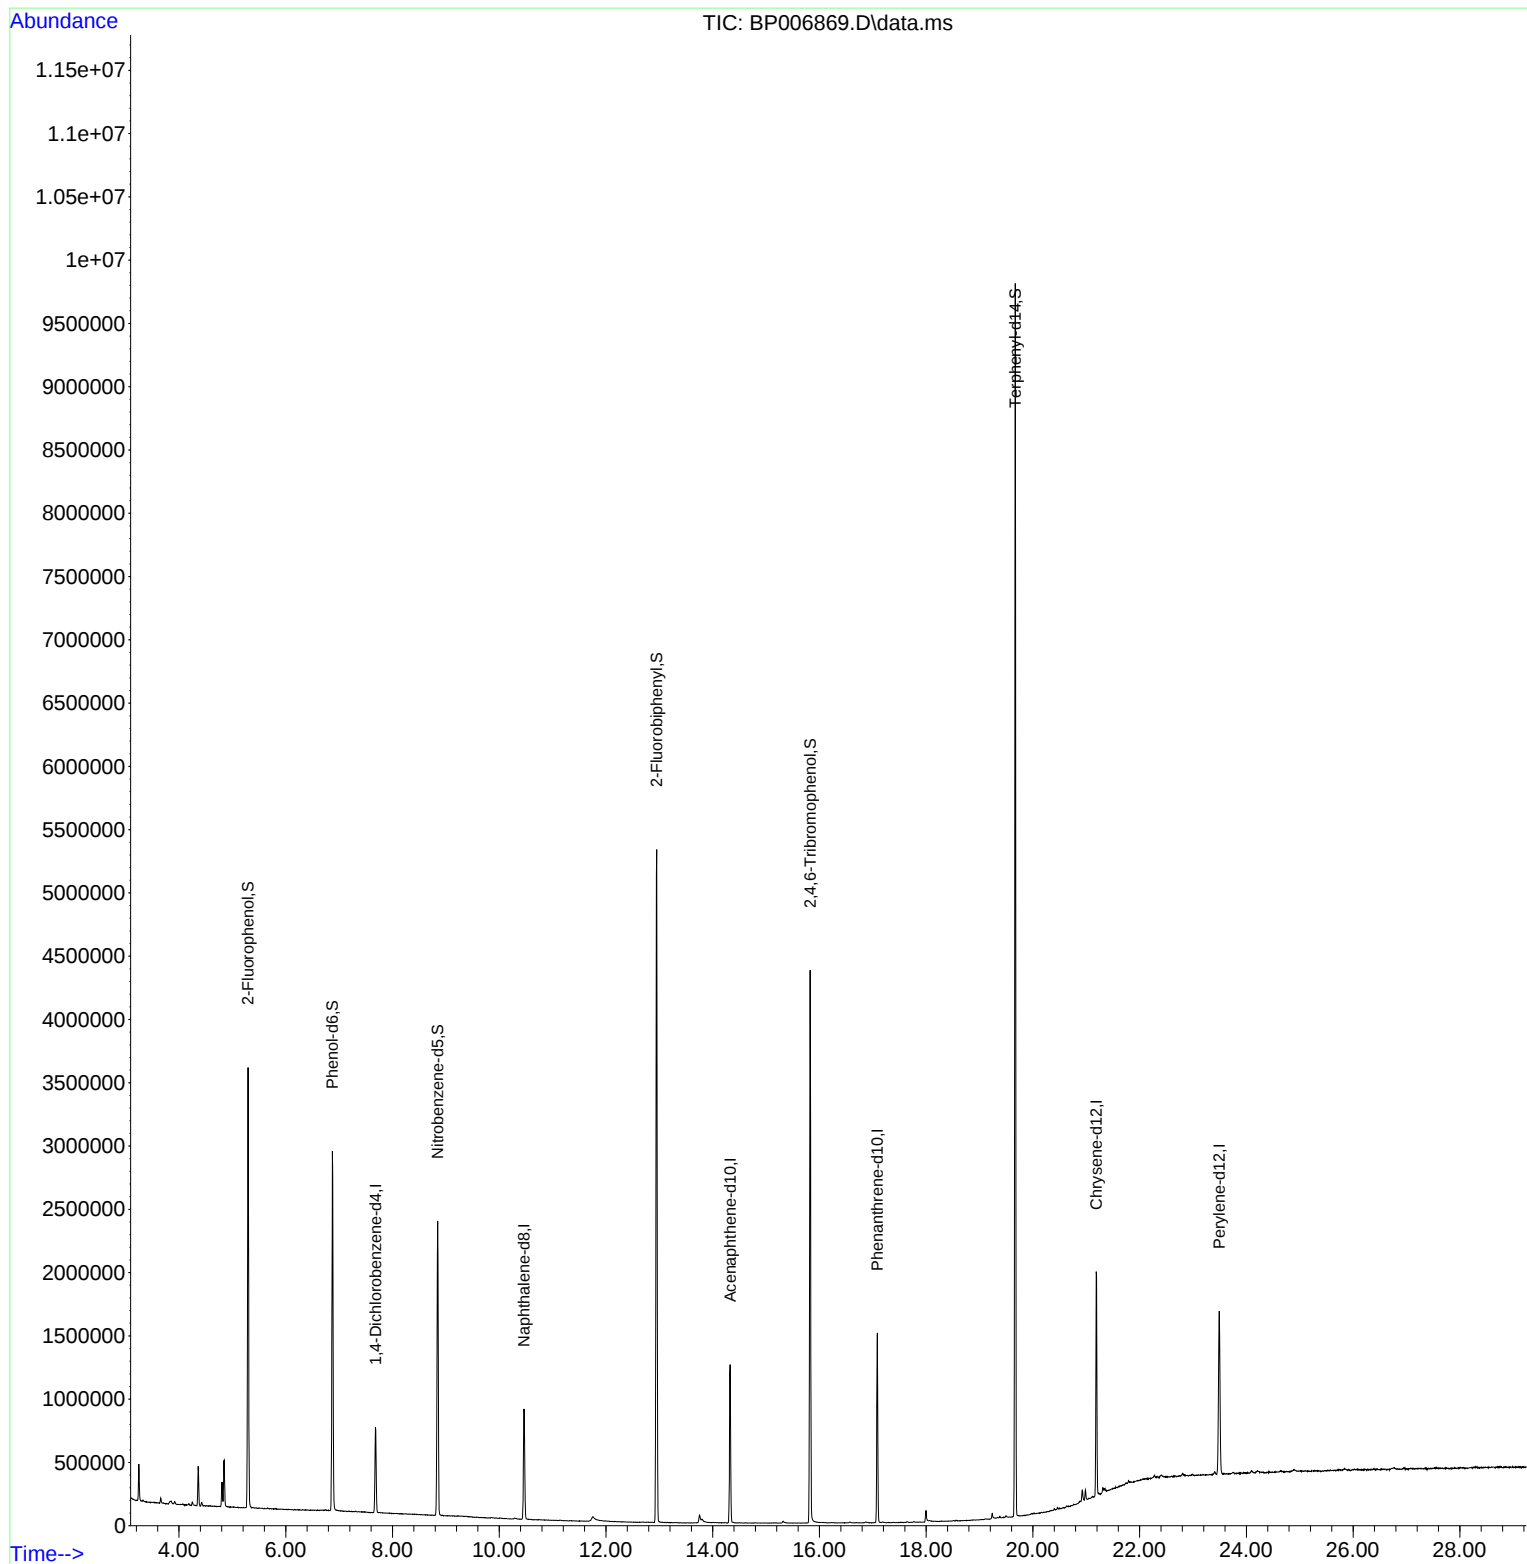


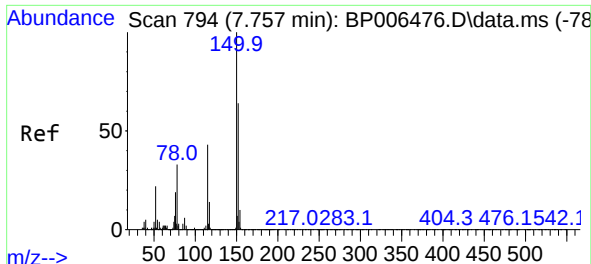

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.681 min Scan# 781
Delta R.T. -0.006 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55




Instrument :
BNA_P
ClientSampleId :
SAMPLE-5-(184.50)

Tgt Ion:152 Resp: 172020
Ion Ratio Lower Upper
152 100
150 156.8 125.6 188.4
115 67.6 48.5 72.7

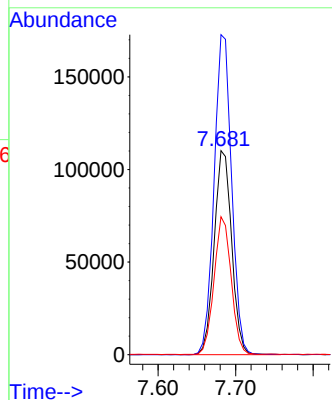

#5
2-Fluorophenol
Concen: 129.000 ng
RT: 5.293 min Scan# 375
Delta R.T. -0.000 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55

Tgt Ion:112 Resp: 1444753
Ion Ratio Lower Upper
112 100
64 55.3 41.4 62.2
63 29.4 23.8 35.8


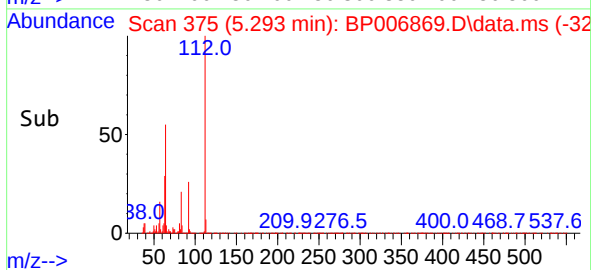
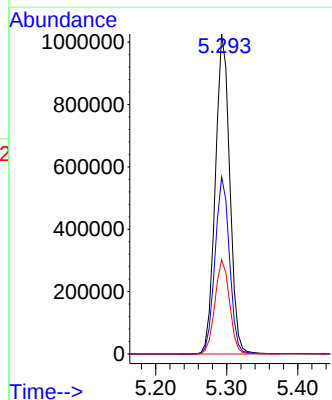
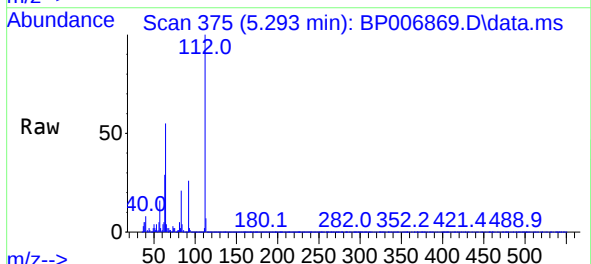




#7
Phenol-d6
Concen: 99.448 ng
RT: 6.875 min Scan# 644
Delta R.T. -0.006 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55




Instrument :
BNA_P
ClientSampleId :
SAMPLE-5-(184.50)


Tgt Ion: 99 Resp: 1582142
Ion Ratio Lower Upper
99 100
42 15.8 13.4 20.0
71 38.3 30.6 46.0

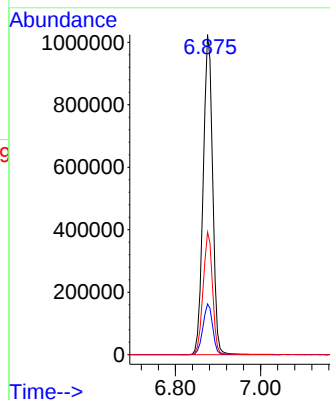

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.463 min Scan# 1254
Delta R.T. -0.012 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55

Tgt Ion: 136 Resp: 703334
Ion Ratio Lower Upper
136 100
137 10.9 8.6 12.8
54 7.4 4.6 6.8#
68 6.5 3.6 5.4#

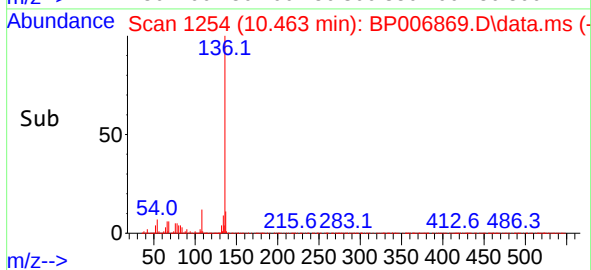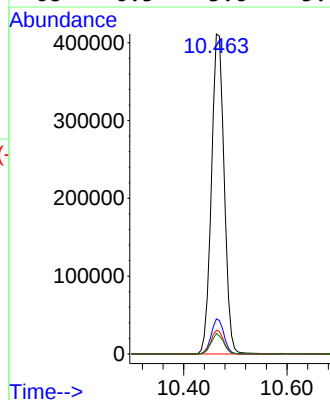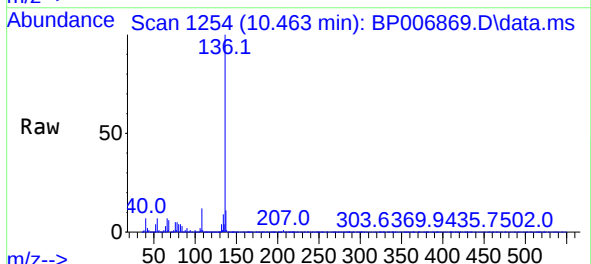




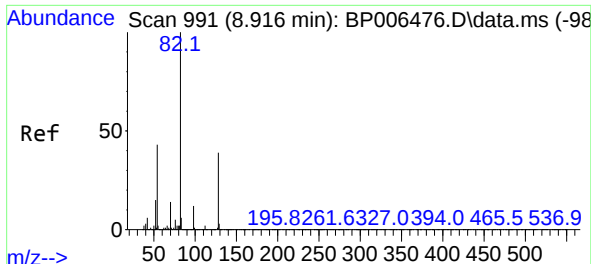


#23
Nitrobenzene-d5
Concen: 90.843 ng
RT: 8.846 min Scan# 979
Delta R.T. -0.006 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55

Instrument :
BNA_P
ClientSampleId :
SAMPLE-5-(184.50)

Tgt Ion: 82 Resp: 1384246




Ion	Ratio	Lower	Upper
82	100		
128	39.7	35.7	53.5
54	42.8	35.0	52.4

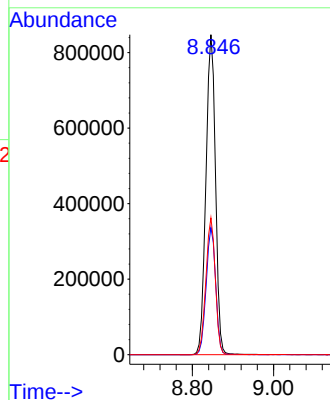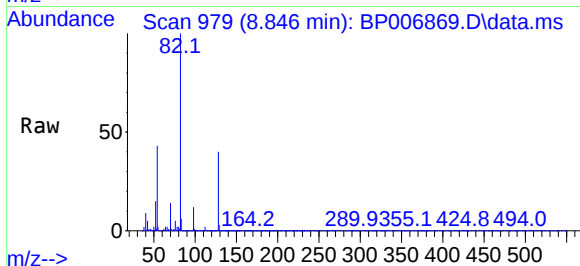


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.328 min Scan# 1911
Delta R.T. -0.012 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55

Tgt Ion: 164 Resp: 391465

Ion	Ratio	Lower	Upper
164	100		
162	103.5	80.2	120.2
160	47.6	34.5	51.7


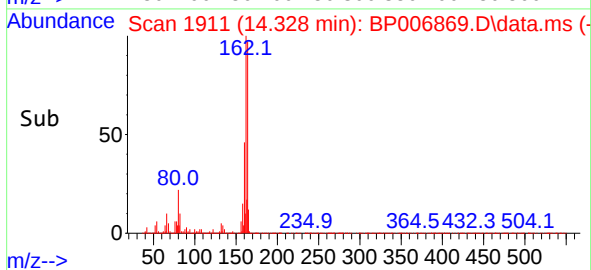
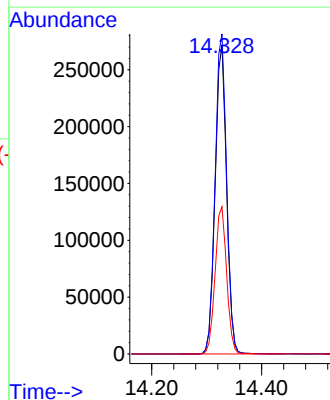
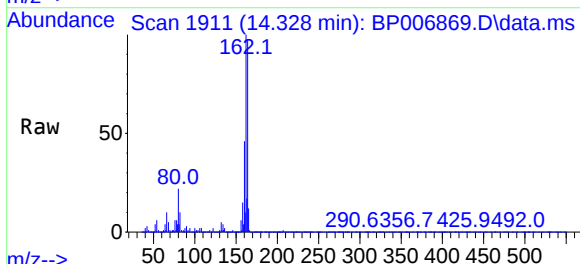


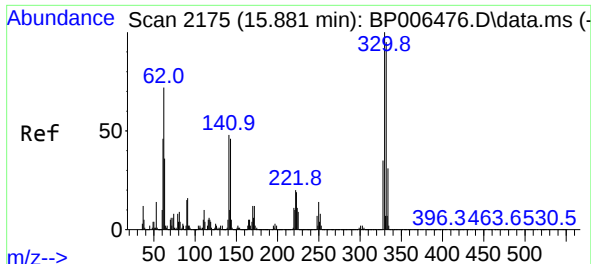

#42
2,4,6-Tribromophenol
Concen: 162.778 ng
RT: 15.828 min Scan# 2166
Delta R.T. -0.018 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55




Instrument :
BNA_P
ClientSampleId :
SAMPLE-5-(184.50)

Tgt Ion:330 Resp: 665965
Ion Ratio Lower Upper
330 100
332 96.1 77.8 116.8
141 48.2 25.4 38.2#

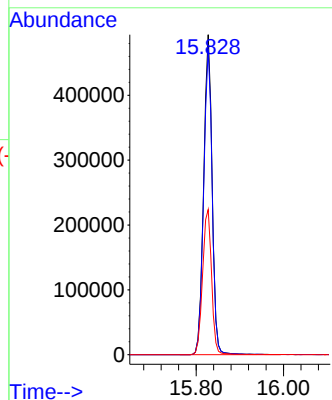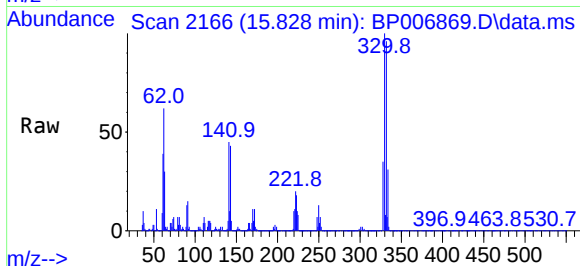

#45
2-Fluorobiphenyl
Concen: 95.195 ng
RT: 12.951 min Scan# 1677
Delta R.T. -0.006 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55

Tgt Ion:172 Resp: 2490786
Ion Ratio Lower Upper
172 100
171 35.3 27.9 41.9
170 23.6 18.6 27.8


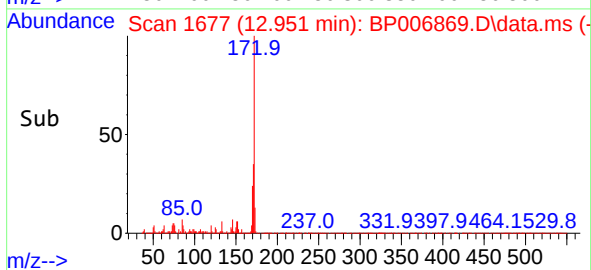
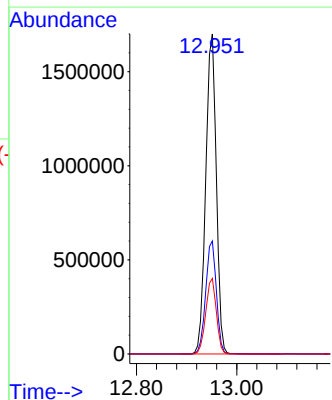
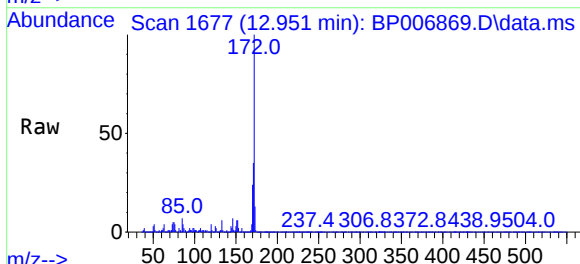




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.086 min Scan# 2380
Delta R.T. -0.012 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55




Instrument :
BNA_P
ClientSampleId :
SAMPLE-5-(184.50)

Tgt Ion:188 Resp: 787194
Ion Ratio Lower Upper
188 100
94 10.6 5.6 8.4#
80 12.1 6.3 9.5#

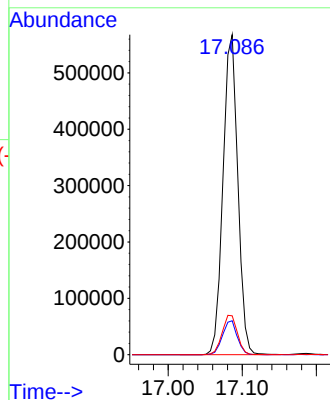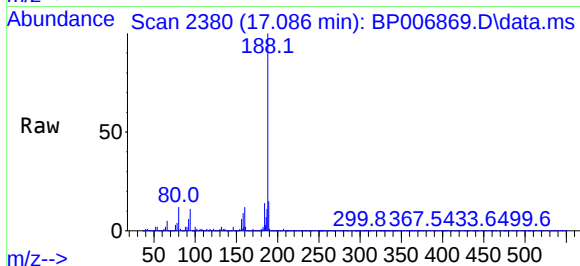

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.186 min Scan# 3077
Delta R.T. -0.024 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55

Tgt Ion:240 Resp: 777825
Ion Ratio Lower Upper
240 100
120 13.0 6.5 9.7#
236 25.0 20.6 31.0


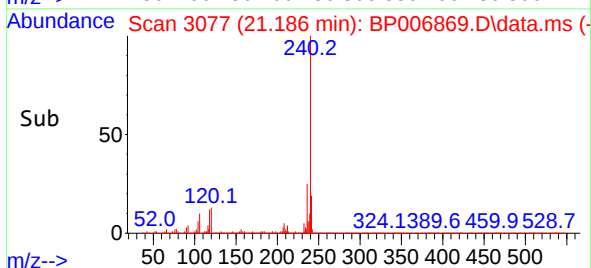
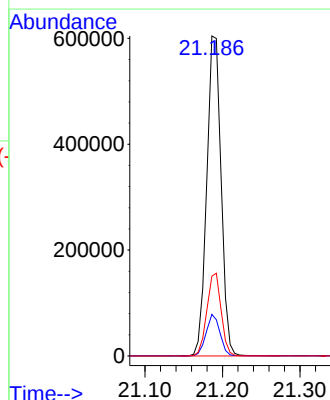
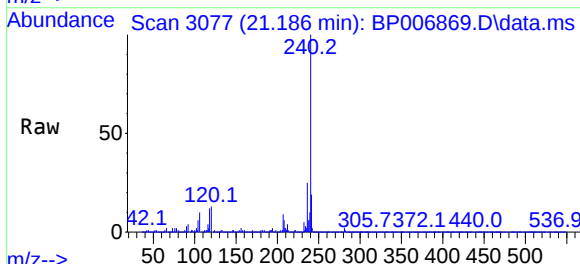




#79
Terphenyl-d14
Concen: 99.717 ng
RT: 19.669 min Scan# 2819
Delta R.T. -0.018 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55

Instrument :
BNA_P
ClientSampleId :
SAMPLE-5-(184.50)

Tgt Ion:244 Resp: 3870790
Ion Ratio Lower Upper
244 100
212 8.1 6.0 9.0
122 12.3 7.1 10.7#

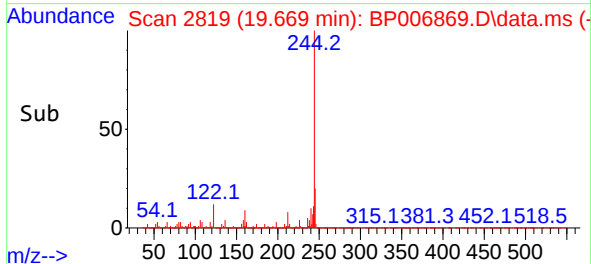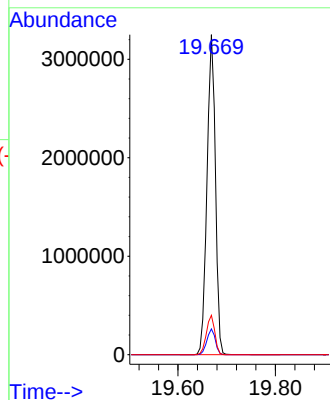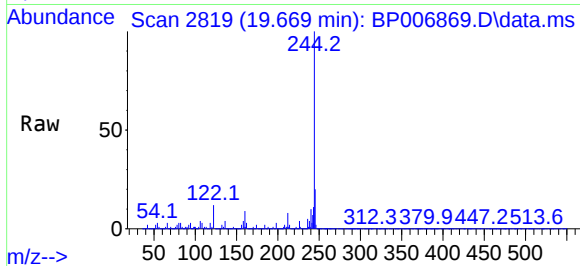

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.492 min Scan# 3469
Delta R.T. -0.035 min
Lab File: BP006869.D
Acq: 25 Aug 2021 03:55

Tgt Ion:264 Resp: 838588
Ion Ratio Lower Upper
264 100
260 24.2 18.6 28.0
265 22.3 17.6 26.4

