

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006844.D
 Acq On : 24 Aug 2021 12:44
 Operator : CG/JU
 Sample : PB138597BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB138597BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006844.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.840	295	298	305	rVB	72675	100125	1.12%	0.237%
2	5.293	369	375	388	rVB	3129897	4369783	48.71%	10.362%
3	6.881	638	645	658	rVB	2849098	4387269	48.91%	10.403%
4	7.687	776	782	789	rBV	556083	852049	9.50%	2.020%
5	8.852	972	980	993	rVB	1796952	2935694	32.73%	6.961%
6	10.475	1249	1256	1265	rVB	711382	1195808	13.33%	2.836%
7	12.957	1670	1678	1691	rBV	4294731	6135767	68.40%	14.549%
8	14.334	1905	1912	1920	rBV	1013608	1464380	16.32%	3.472%
9	15.834	2160	2167	2178	rBV	3136179	4549908	50.72%	10.789%
10	17.098	2375	2382	2390	rBV	1186539	1678889	18.72%	3.981%
11	19.681	2816	2821	2826	rBV	7436836	8970417	100.00%	21.271%
12	20.892	3023	3027	3032	rBV	150989	228728	2.55%	0.542%
13	20.945	3032	3036	3040	rBV	226805	295744	3.30%	0.701%
14	20.998	3041	3045	3052	rBV	809014	955261	10.65%	2.265%
15	21.204	3075	3080	3085	rBV	1592908	1967999	21.94%	4.667%
16	23.522	3468	3474	3481	rVB2	1071271	2084698	23.24%	4.943%




Sum of corrected areas: 42172519

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006844.D
Acq On : 24 Aug 2021 12:44
Operator : CG/JU
Sample : PB138597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138597BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

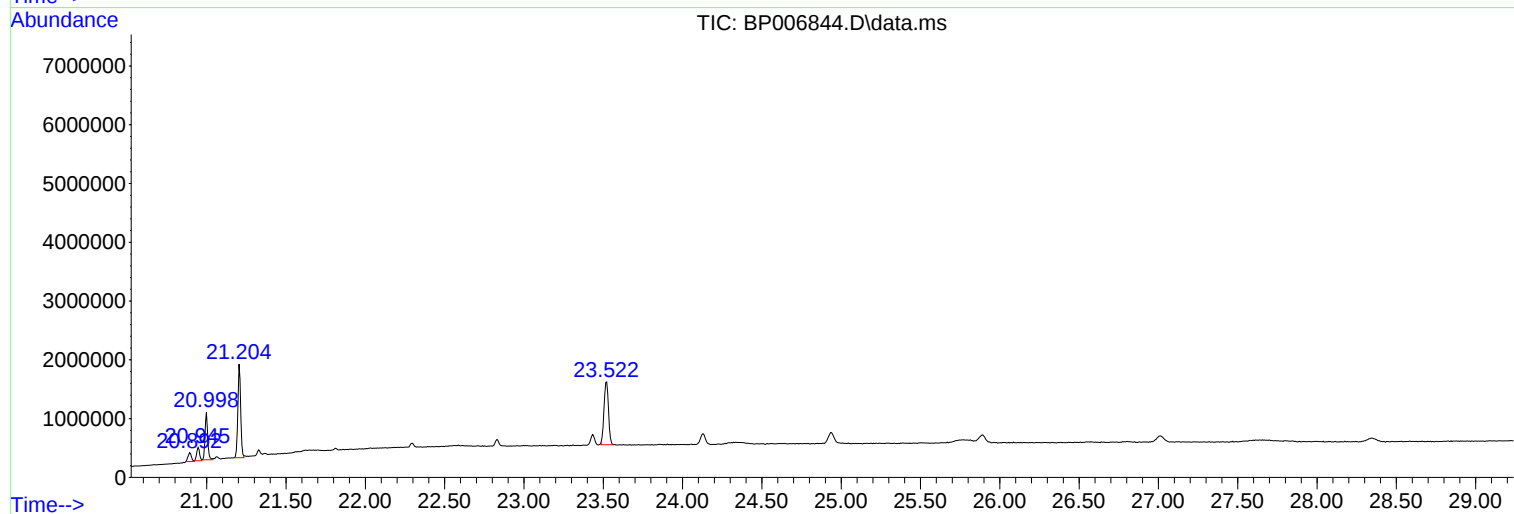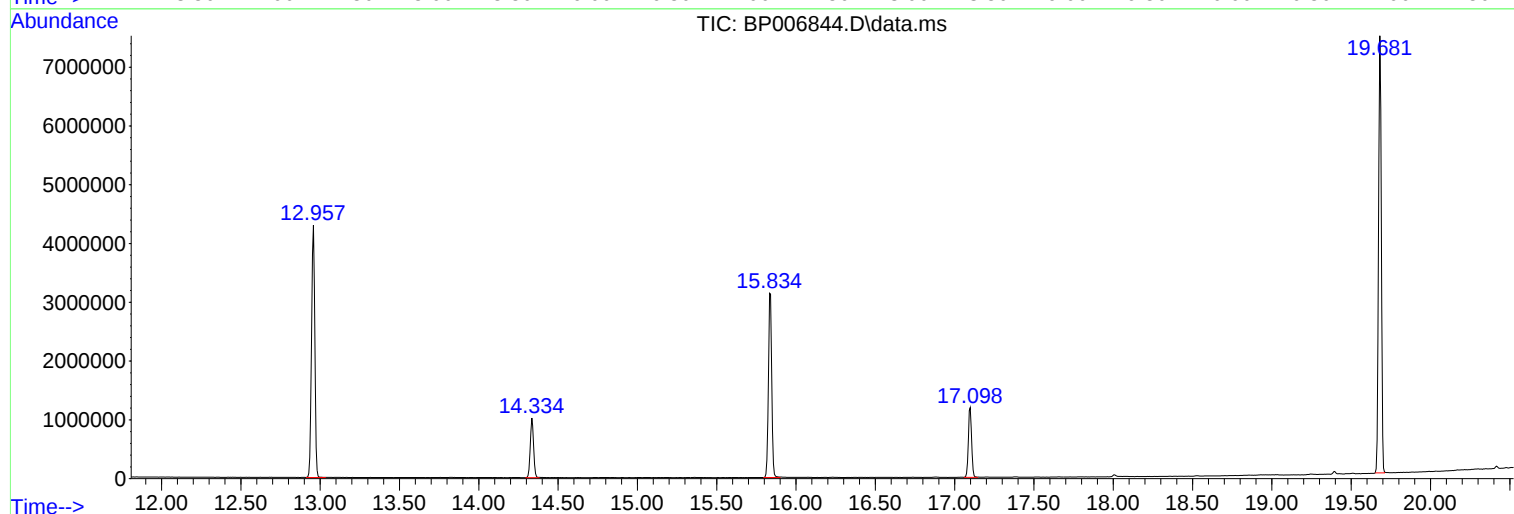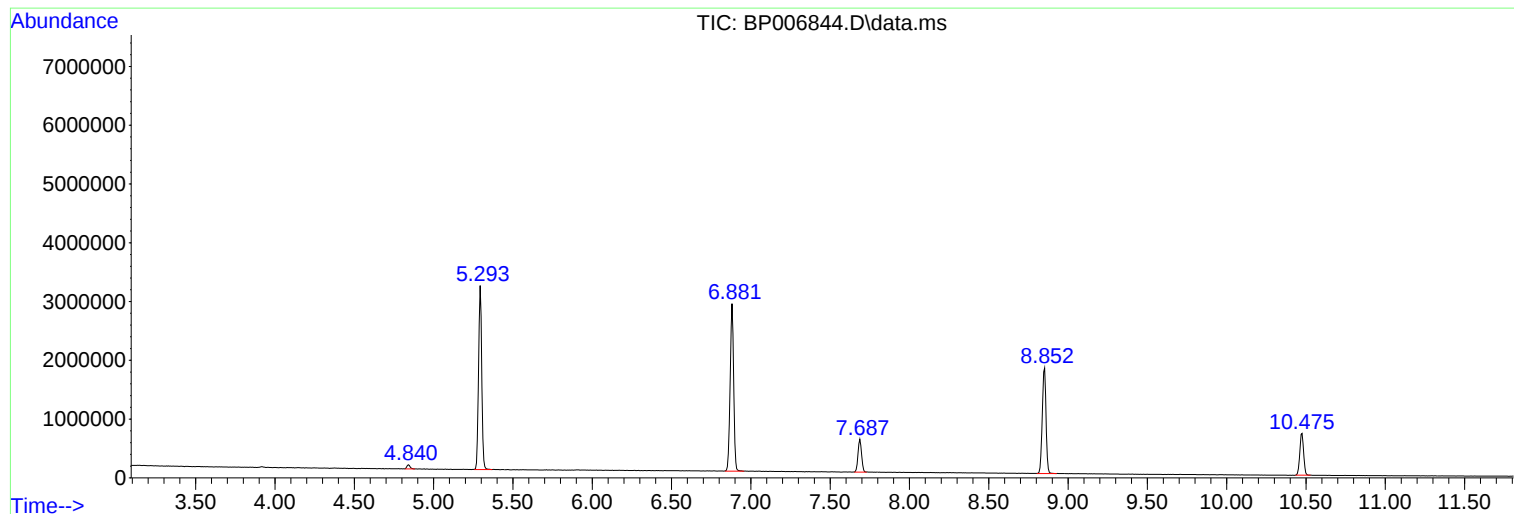

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006844.D
Acq On : 24 Aug 2021 12:44
Operator : CG/JU
Sample : PB138597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138597BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006844.D
Acq On : 24 Aug 2021 12:44
Operator : CG/JU
Sample : PB138597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138597BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------