

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006850.D
 Acq On : 24 Aug 2021 16:24
 Operator : CG/JU
 Sample : M3502-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 POST-MAEC-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.293	369	375	382	rBV	2637886	3763680	28.64%	4.641%
2	6.881	638	645	656	rVB	2556652	4020250	30.59%	4.957%
3	7.687	776	782	790	rVB	569628	872537	6.64%	1.076%
4	8.845	972	979	987	rBV	1589138	2643452	20.12%	3.259%
5	9.775	1128	1137	1143	rBV	133334	296301	2.25%	0.365%
6	10.269	1215	1221	1233	rBV	92067	178658	1.36%	0.220%
7	10.469	1248	1255	1262	rBV	727736	1241994	9.45%	1.531%
8	12.951	1669	1677	1687	rVB	3611842	5209394	39.64%	6.423%
9	13.239	1720	1726	1734	rBV	159212	261792	1.99%	0.323%
10	14.333	1906	1912	1918	rVB	1044716	1498270	11.40%	1.847%
11	15.833	2158	2167	2176	rVV	2868757	4092399	31.14%	5.046%
12	17.092	2375	2381	2385	rBV	1227318	1701570	12.95%	2.098%
13	17.133	2385	2388	2395	rVB	212459	285652	2.17%	0.352%
14	18.021	2532	2539	2558	rBV	3997835	6720239	51.14%	8.286%
15	18.274	2578	2582	2588	rBV2	291022	432335	3.29%	0.533%
16	18.480	2612	2617	2622	rBV	788694	1052073	8.01%	1.297%
17	18.845	2676	2679	2682	rBV3	115044	156933	1.19%	0.193%
18	18.880	2682	2685	2693	rVB	600930	778377	5.92%	0.960%
19	19.116	2721	2725	2732	rBV	435372	1136020	8.64%	1.401%
20	19.268	2744	2751	2764	rBV	8283845	13141187	100.00%	16.203%
21	19.468	2782	2785	2788	rVB	304209	333545	2.54%	0.411%
22	19.674	2815	2820	2831	rVB	5496825	6728714	51.20%	8.296%
23	19.880	2851	2855	2860	rVB	498262	572201	4.35%	0.706%
24	20.680	2987	2991	2996	rVB3	493602	619008	4.71%	0.763%
25	20.892	3021	3027	3030	rBV	1213077	2020661	15.38%	2.491%
26	20.945	3030	3036	3040	rVV	2100531	3727868	28.37%	4.596%
27	20.998	3040	3045	3052	rVV	4861427	6398381	48.69%	7.889%
28	21.062	3053	3056	3060	rVB	337627	376057	2.86%	0.464%
29	21.204	3075	3080	3083	rBV	1534374	2164930	16.47%	2.669%
30	21.598	3144	3147	3154	rVB2	930593	1184352	9.01%	1.460%
31	21.668	3156	3159	3164	rVB	857694	1067679	8.12%	1.316%
32	22.257	3255	3259	3263	rBV2	569314	804597	6.12%	0.992%
33	22.721	3333	3338	3344	rVB	831079	1283795	9.77%	1.583%
34	23.515	3467	3473	3479	rVB2	1064650	2036166	15.49%	2.511%
35	24.174	3581	3585	3597	rVB2	461193	1023438	7.79%	1.262%
36	24.798	3686	3691	3702	rVB2	525319	1278690	9.73%	1.577%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006850.D
Acq On : 24 Aug 2021 16:24
Operator : CG/JU
Sample : M3502-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 81103195

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006850.D
Acq On : 24 Aug 2021 16:24
Operator : CG/JU
Sample : M3502-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

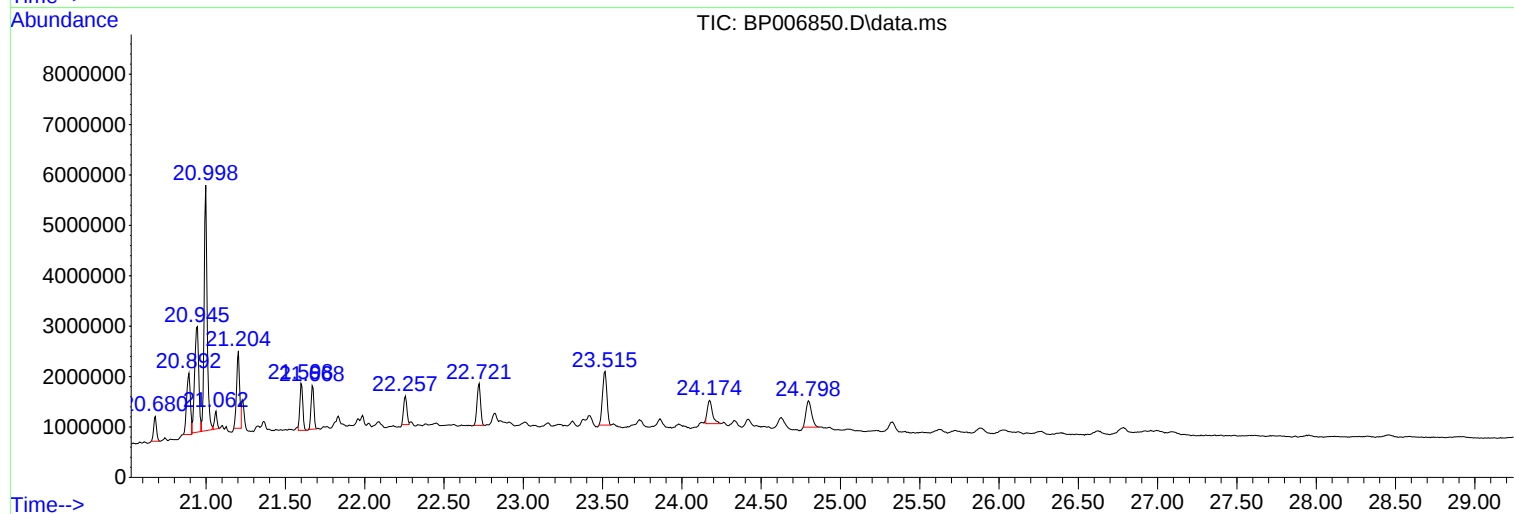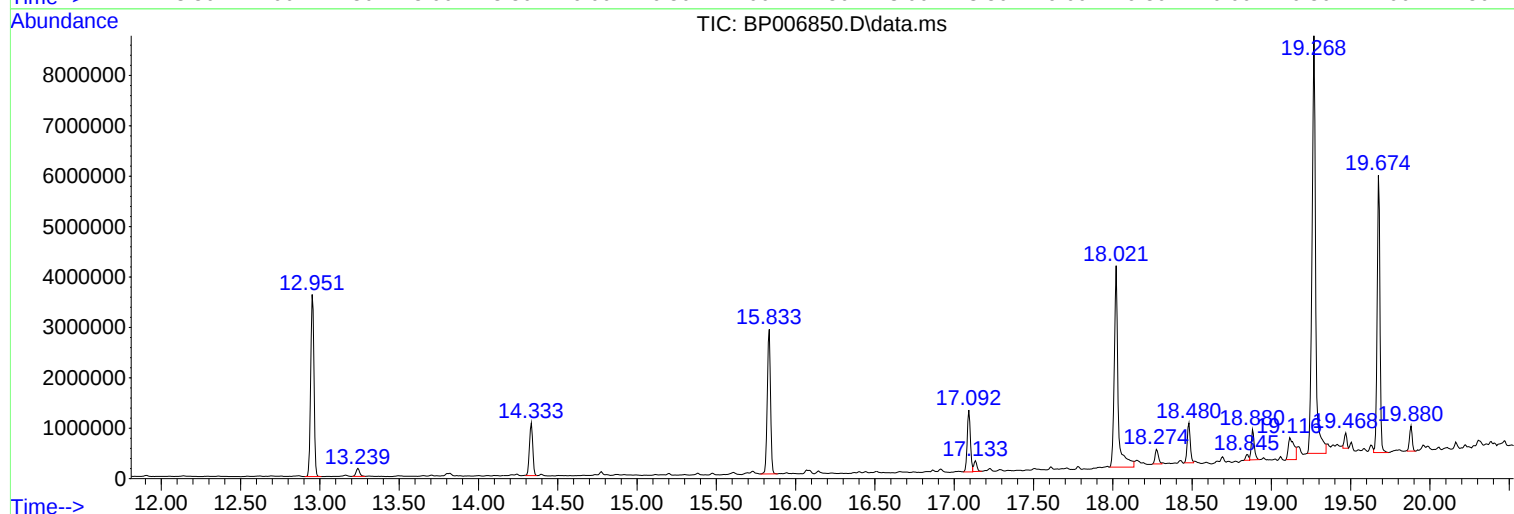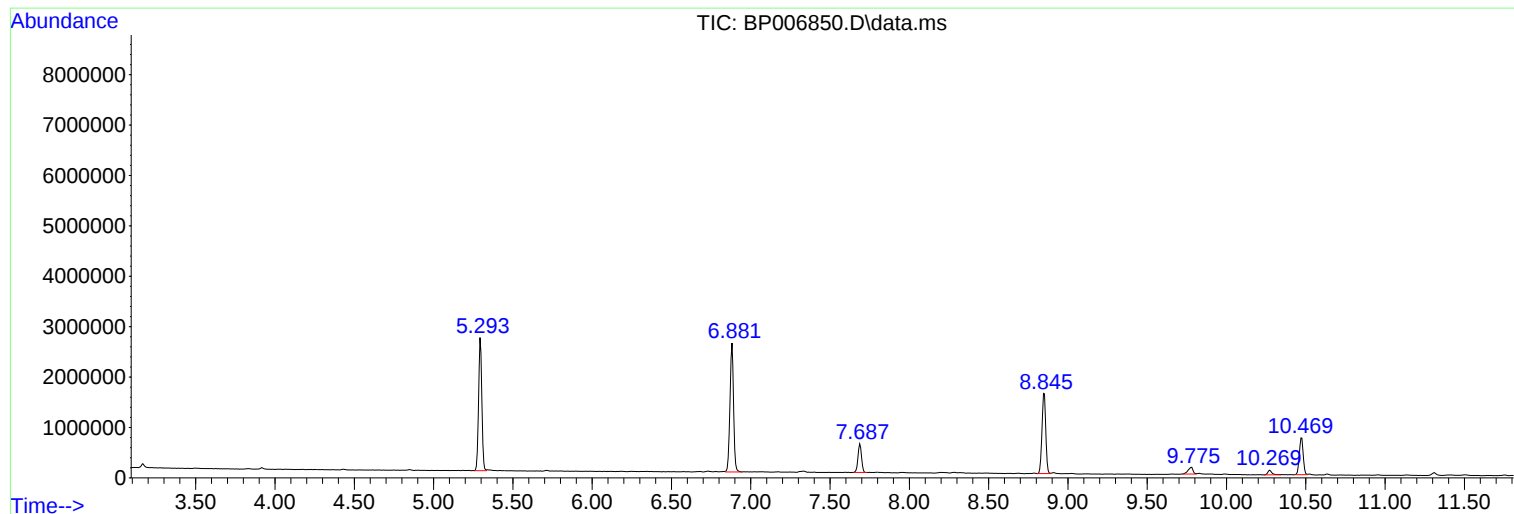

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006850.D
Acq On : 24 Aug 2021 16:24
Operator : CG/JU
Sample : M3502-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006850.D
Acq On : 24 Aug 2021 16:24
Operator : CG/JU
Sample : M3502-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------