

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006851.D
 Acq On : 24 Aug 2021 16:58
 Operator : CG/JU
 Sample : M3502-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 POST-MAEC-01

Integration Parameters: rteint.p

Integrator: RTE

Smothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	10	14	22	rVB	165293	232484	3.04%	0.350%
2	5.293	369	375	395	rVB	2864324	4188551	54.78%	6.298%
3	6.881	638	645	659	rVB	2806503	4347291	56.86%	6.537%
4	7.687	776	782	790	rVB	636060	973732	12.74%	1.464%
5	8.852	972	980	987	rBV	1728233	2860618	37.42%	4.302%
6	10.269	1216	1221	1229	rBV	104939	180501	2.36%	0.271%
7	10.469	1247	1255	1261	rBV	839029	1424637	18.63%	2.142%
8	11.310	1389	1398	1406	rBV2	55031	111929	1.46%	0.168%
9	12.951	1670	1677	1687	rVB	3909054	5664227	74.09%	8.518%
10	13.240	1720	1726	1734	rVB	54960	95742	1.25%	0.144%
11	13.798	1816	1821	1830	rBV	83244	180725	2.36%	0.272%
12	14.334	1906	1912	1918	rVB	1213298	1739641	22.75%	2.616%
13	15.604	2123	2128	2136	rVB2	50370	92693	1.21%	0.139%
14	15.834	2160	2167	2175	rVB	3247029	4565052	59.71%	6.865%
15	16.069	2203	2207	2208	rBV	81378	95740	1.25%	0.144%
16	16.916	2348	2351	2360	rVB3	77067	119816	1.57%	0.180%
17	17.092	2375	2381	2385	rBV	1430086	2008565	26.27%	3.020%
18	17.134	2385	2388	2395	rVB	153512	228786	2.99%	0.344%
19	18.010	2532	2537	2545	rBV	1577837	2293462	30.00%	3.449%
20	18.275	2578	2582	2590	rBV3	306747	491706	6.43%	0.739%
21	18.475	2612	2616	2627	rBV	778013	1150309	15.05%	1.730%
22	18.881	2682	2685	2692	rVB	580309	756485	9.89%	1.138%
23	19.116	2721	2725	2729	rBV	332266	567064	7.42%	0.853%
24	19.251	2744	2748	2759	rBV2	1428699	2276659	29.78%	3.423%
25	19.469	2782	2785	2788	rVB	229746	252966	3.31%	0.380%
26	19.675	2815	2820	2830	rVB	6275895	7645448	100.00%	11.497%
27	19.880	2851	2855	2859	rVB	571605	682896	8.93%	1.027%
28	20.675	2987	2990	2995	rVB3	570970	713330	9.33%	1.073%
29	20.892	3022	3027	3030	rBV	1072908	1727911	22.60%	2.598%
30	20.939	3030	3035	3040	rVV2	2062118	3769598	49.31%	5.668%
31	20.998	3040	3045	3052	rVB	4063526	5698553	74.54%	8.569%
32	21.198	3075	3079	3082	rBV	1714830	2302177	30.11%	3.462%
33	21.598	3144	3147	3154	rVB	1075601	1355000	17.72%	2.038%
34	21.669	3155	3159	3167	rVB	992205	1233273	16.13%	1.855%
35	22.251	3255	3258	3263	rBV2	647719	881512	11.53%	1.326%
36	22.721	3334	3338	3343	rVB	876398	1276052	16.69%	1.919%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006851.D
Acq On : 24 Aug 2021 16:58
Operator : CG/JU
Sample : M3502-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	23.516	3468	3473	3479	rVB2	1229284	2315888	30.29%	3.482%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 66501019

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006851.D
Acq On : 24 Aug 2021 16:58
Operator : CG/JU
Sample : M3502-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

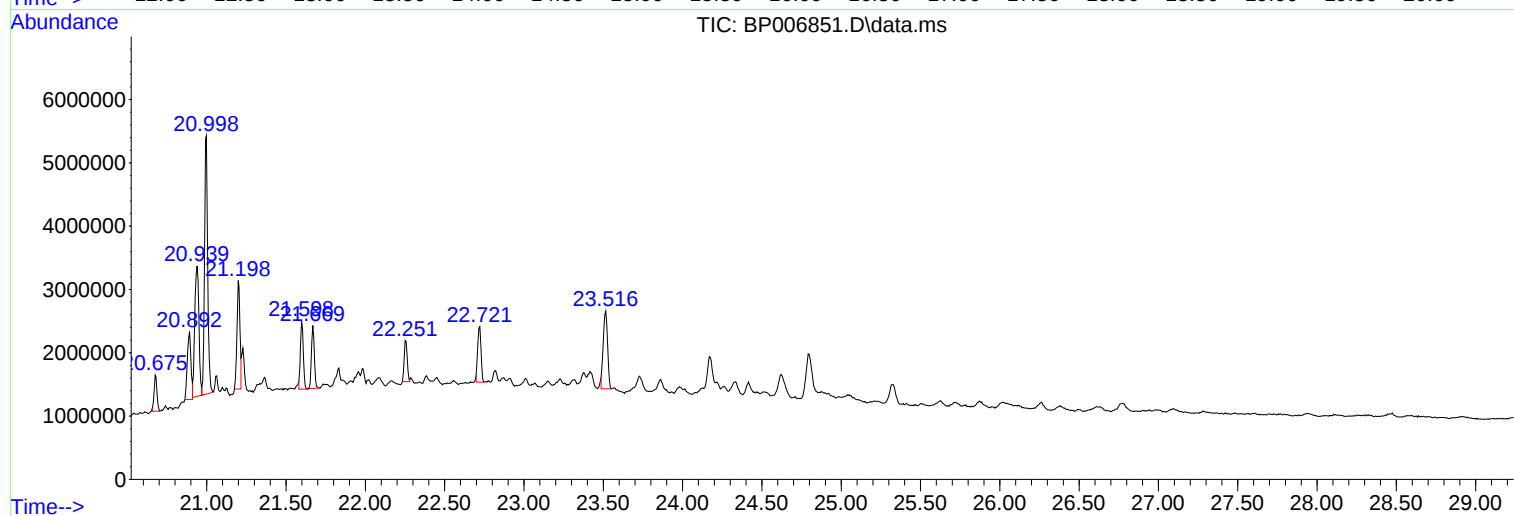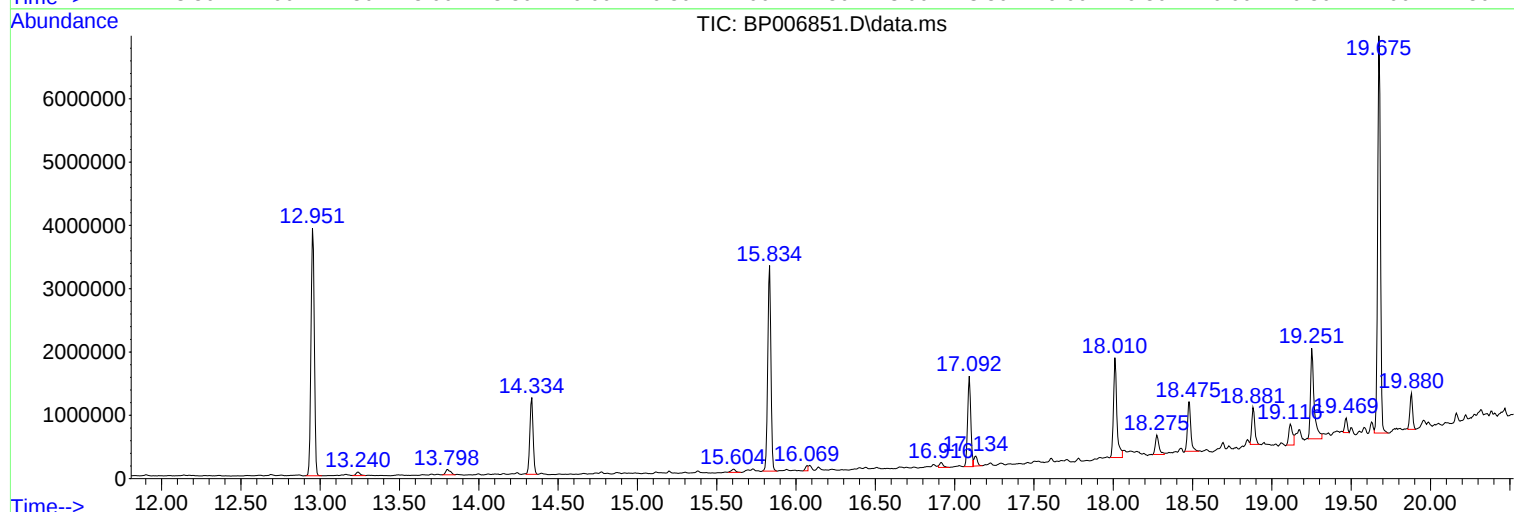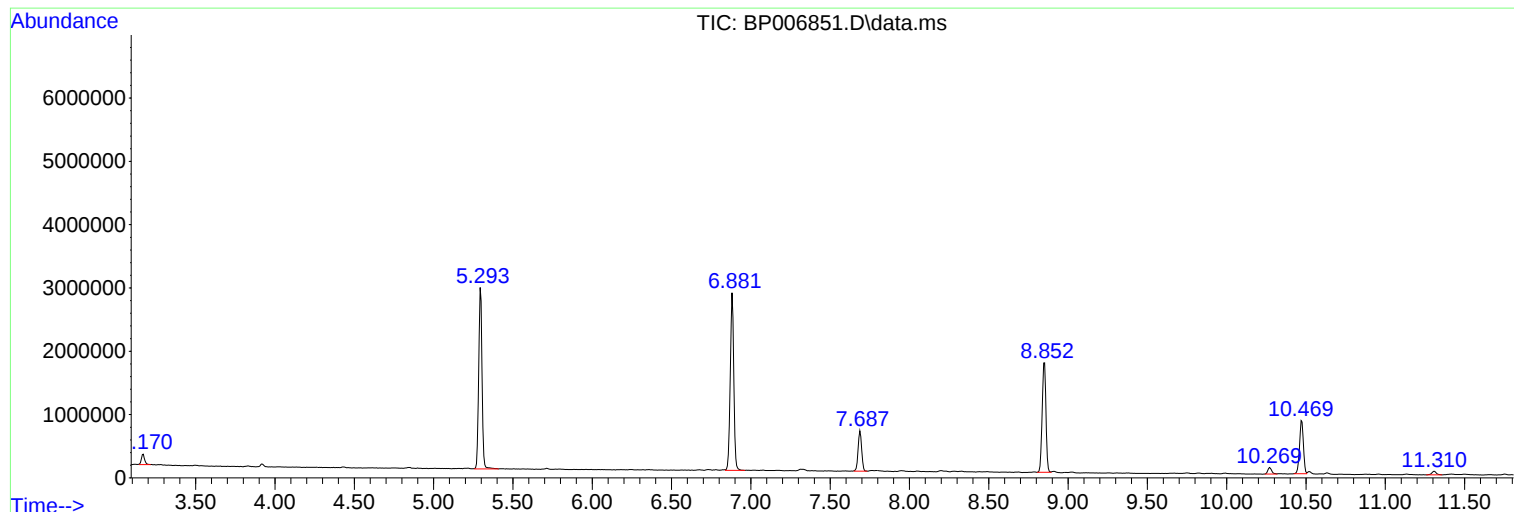

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006851.D
Acq On : 24 Aug 2021 16:58
Operator : CG/JU
Sample : M3502-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006851.D
Acq On : 24 Aug 2021 16:58
Operator : CG/JU
Sample : M3502-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc