

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006858.D
 Acq On : 24 Aug 2021 21:39
 Operator : CG/JU
 Sample : M3502-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 POST-MAEC-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	24	27	38	rVB	199585	222600	2.17%	0.462%
2	4.358	212	216	224	rVB	219309	282903	2.76%	0.587%
3	4.805	288	292	297	rBV	131484	163968	1.60%	0.340%
4	5.293	369	375	388	rBV	3142621	4626529	45.16%	9.601%
5	6.881	638	645	655	rVB	2743636	4315629	42.13%	8.956%
6	7.687	776	782	789	rVB	656519	1016525	9.92%	2.110%
7	8.846	972	979	995	rVB	2047089	3433346	33.51%	7.125%
8	10.269	1215	1221	1232	rBV	165913	320462	3.13%	0.665%
9	10.469	1248	1255	1263	rBV	885994	1434252	14.00%	2.976%
10	12.951	1669	1677	1687	rBV	4921109	7118134	69.48%	14.772%
11	14.328	1904	1911	1919	rBV	1195282	1761682	17.20%	3.656%
12	15.828	2156	2166	2177	rBV	3895056	5594238	54.61%	11.610%
13	17.086	2374	2380	2393	rBV	1448885	2014750	19.67%	4.181%
14	17.998	2530	2535	2544	rBV	148797	240352	2.35%	0.499%
15	19.239	2742	2746	2757	rBV	68490	124657	1.22%	0.259%
16	19.675	2814	2820	2825	rBV	8402504	10244733	100.00%	21.261%
17	20.927	3029	3033	3039	rBV2	202600	326324	3.19%	0.677%
18	20.986	3039	3043	3049	rVV	311891	379498	3.70%	0.788%
19	21.192	3073	3078	3083	rBV	1797886	2225501	21.72%	4.619%
20	23.498	3464	3470	3483	rVB2	1229790	2339792	22.84%	4.856%




Sum of corrected areas: 48185875

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006858.D
Acq On : 24 Aug 2021 21:39
Operator : CG/JU
Sample : M3502-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

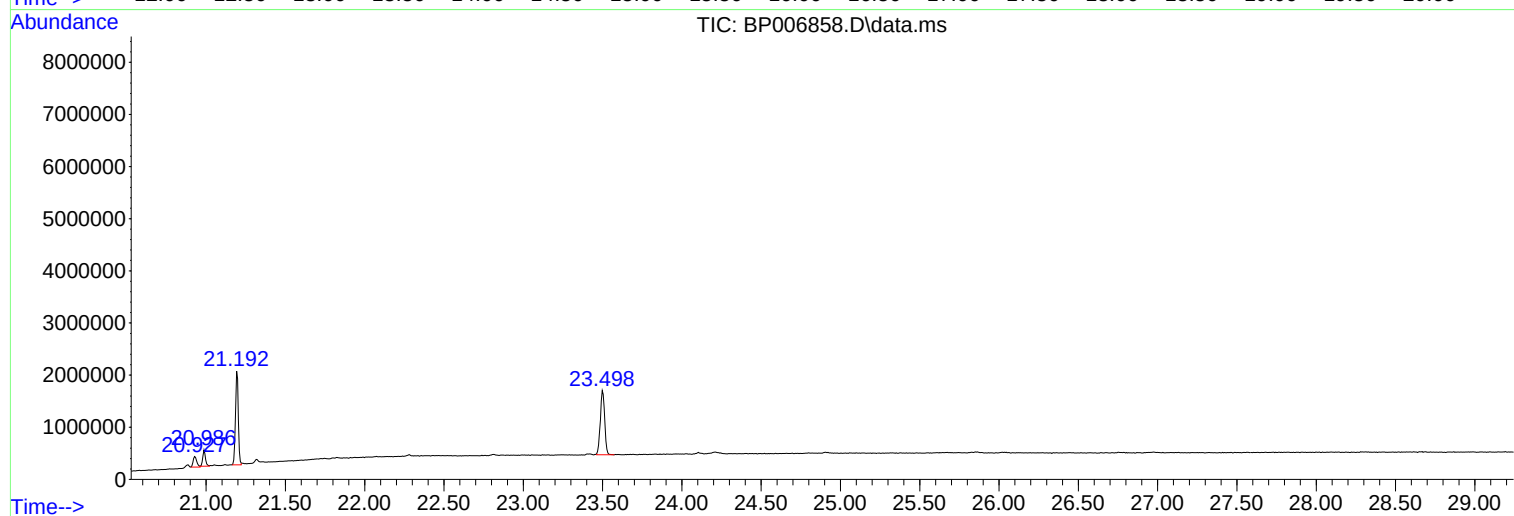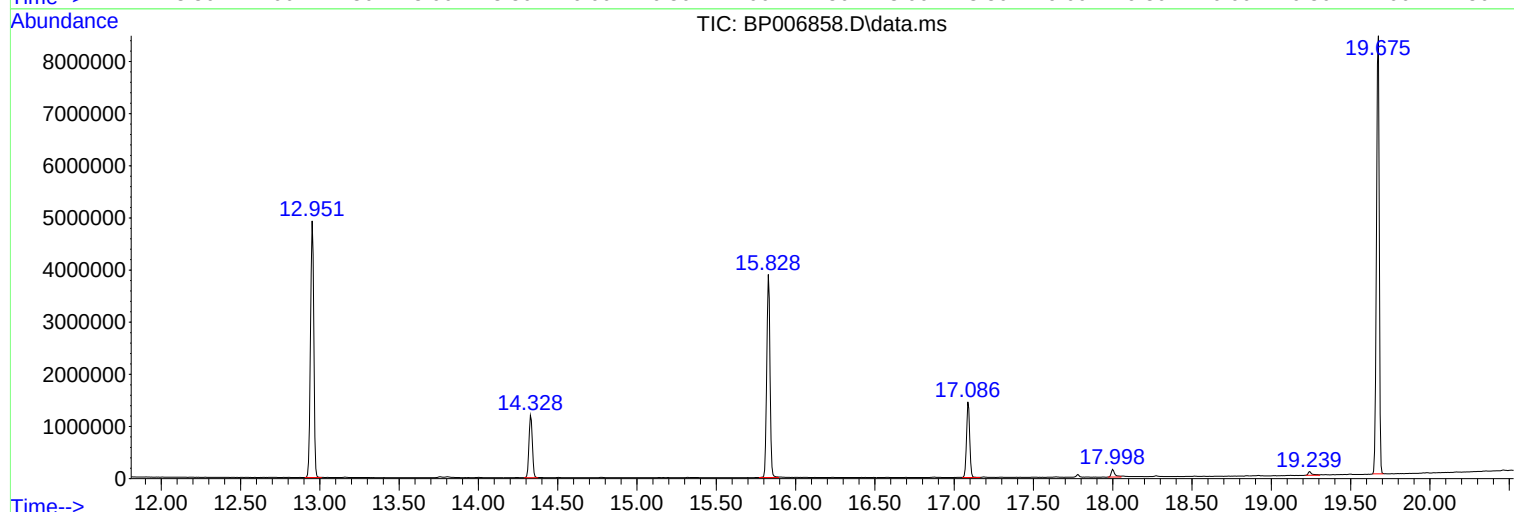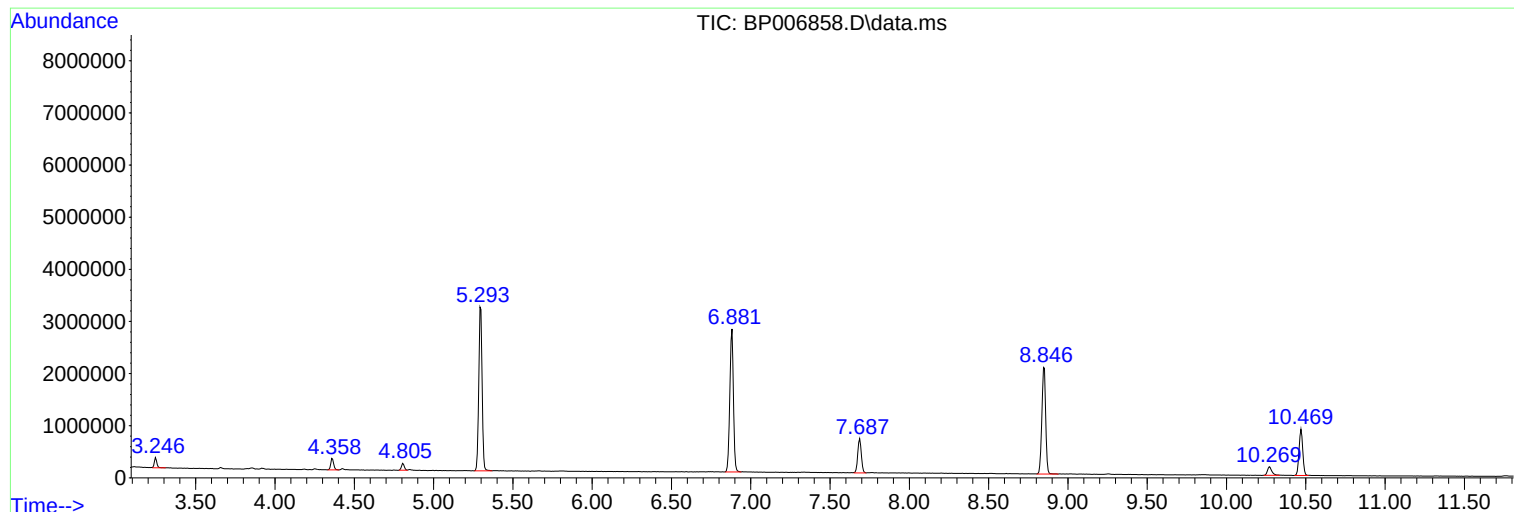

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006858.D
Acq On : 24 Aug 2021 21:39
Operator : CG/JU
Sample : M3502-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006858.D
Acq On : 24 Aug 2021 21:39
Operator : CG/JU
Sample : M3502-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------