

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006862.D
 Acq On : 24 Aug 2021 23:56
 Operator : CG/JU
 Sample : M3502-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 POST-MAEC-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	34	rVB	127823	143735	1.65%	0.360%
2	4.358	212	216	223	rVB	157760	194795	2.24%	0.487%
3	4.805	288	292	295	rBV	88335	112259	1.29%	0.281%
4	4.840	295	298	306	rVB	257724	359342	4.13%	0.899%
5	5.293	369	375	388	rVB	2827895	3922351	45.10%	9.812%
6	6.875	638	644	659	rVB	2383988	3746985	43.08%	9.373%
7	7.687	776	782	789	rVB	548046	861567	9.91%	2.155%
8	8.846	972	979	986	rBV	1744940	2806873	32.27%	7.021%
9	10.469	1248	1255	1265	rVB	724572	1195603	13.75%	2.991%
10	12.951	1669	1677	1690	rBV	3946103	5783624	66.50%	14.467%
11	14.328	1904	1911	1920	rBV	1006832	1447853	16.65%	3.622%
12	15.828	2159	2166	2180	rBV	3222561	4468033	51.37%	11.177%
13	17.087	2373	2380	2392	rBV	1203444	1673819	19.25%	4.187%
14	17.998	2530	2535	2542	rBV	72918	116620	1.34%	0.292%
15	19.669	2813	2819	2824	rBV	7505358	8697084	100.00%	21.755%
16	20.928	3030	3033	3038	rVB2	84030	126524	1.45%	0.316%
17	20.986	3039	3043	3050	rVV	187504	245023	2.82%	0.613%
18	21.192	3073	3078	3085	rBV	1610434	1949431	22.41%	4.876%
19	23.498	3463	3470	3478	rVB2	1064009	2125287	24.44%	5.316%




Sum of corrected areas: 39976808

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006862.D
Acq On : 24 Aug 2021 23:56
Operator : CG/JU
Sample : M3502-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

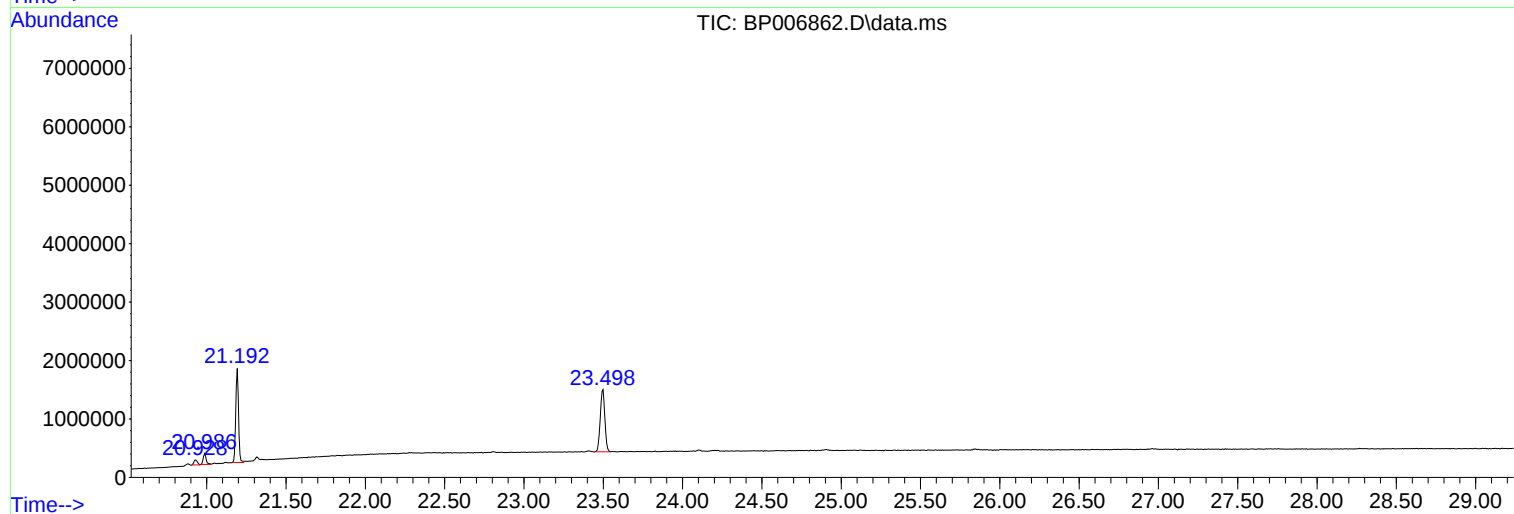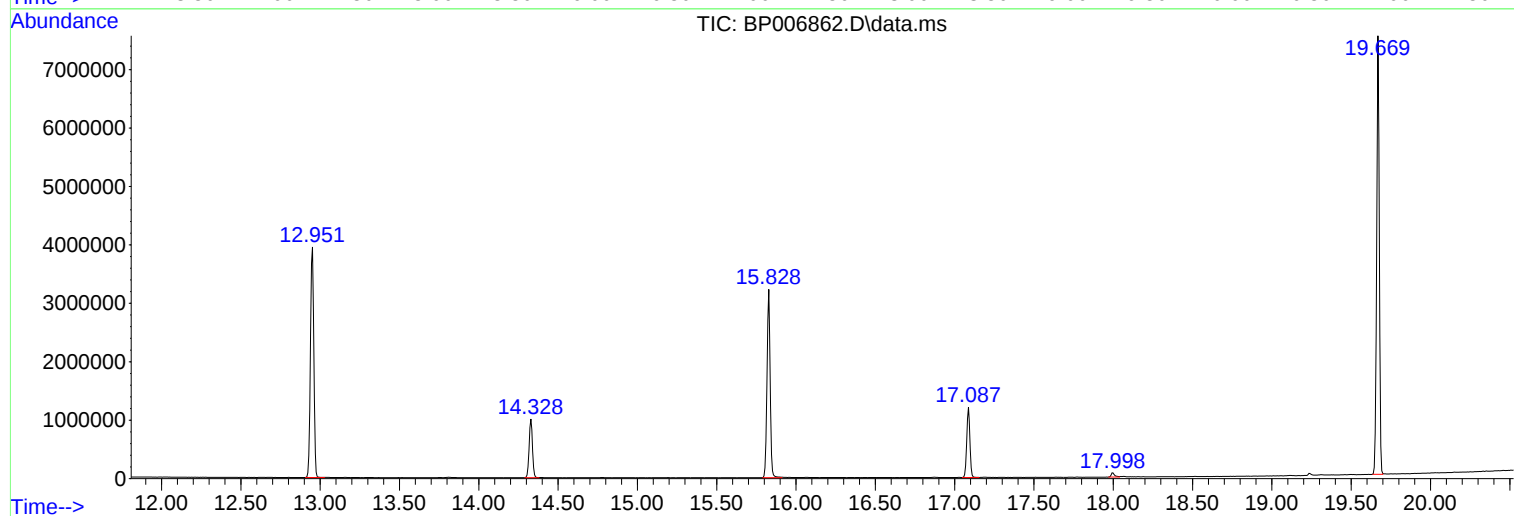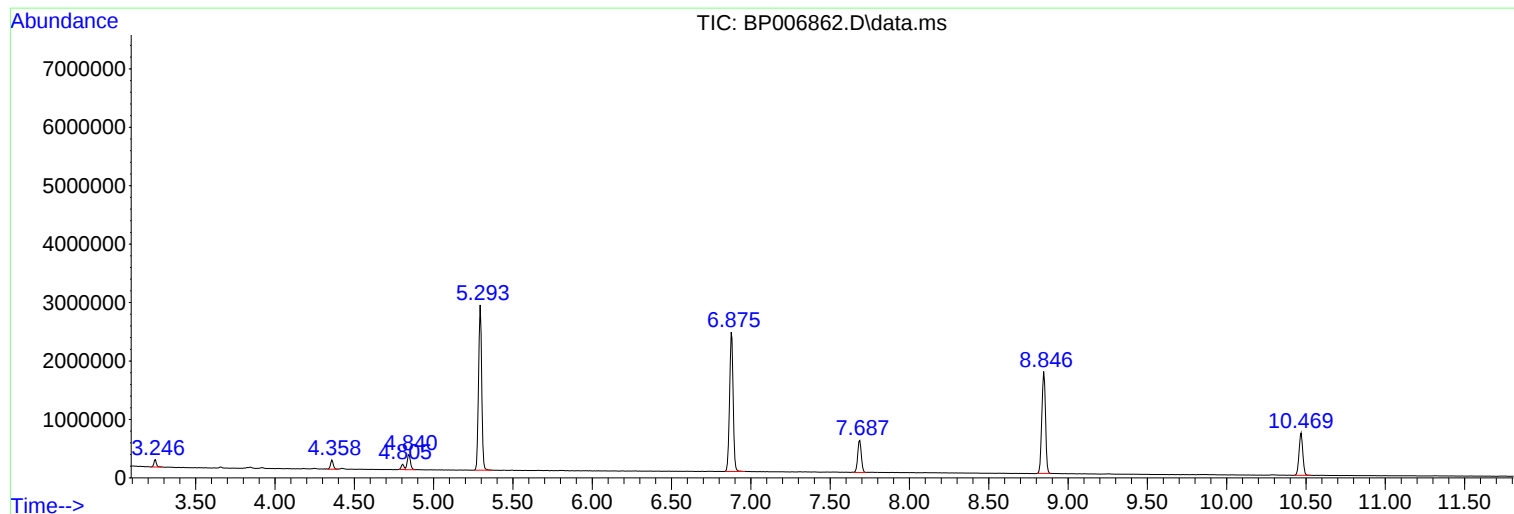

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006862.D
Acq On : 24 Aug 2021 23:56
Operator : CG/JU
Sample : M3502-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006862.D
Acq On : 24 Aug 2021 23:56
Operator : CG/JU
Sample : M3502-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
POST-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------