
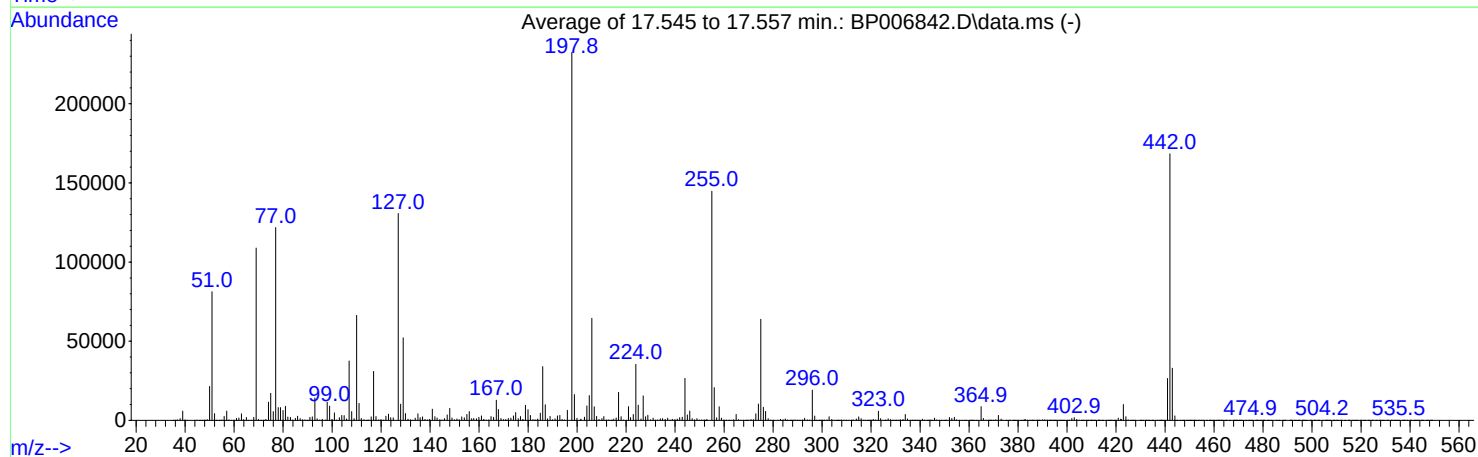


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006842.D
 Acq On : 24 Aug 2021 10:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 25 11:27:41 2021

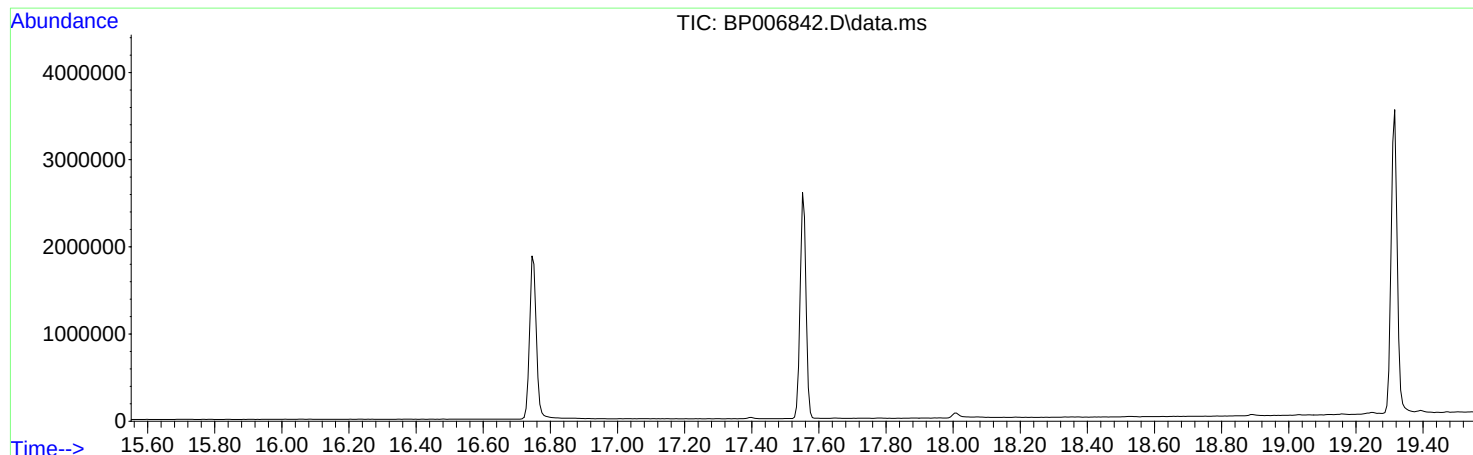




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	81235	PASS
68	69	0.00	2	1.7	1881	PASS
69	198	0.00	100	46.9	108895	PASS
70	69	0.00	2	0.5	571	PASS
127	198	10	80	56.2	130681	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	232368	PASS
199	198	5	9	7.0	16316	PASS
275	198	10	60	27.5	63909	PASS
365	198	1	100	3.7	8685	PASS
441	198	0.01	100	11.4	26535	PASS
442	442	100	100	100.0	168363	PASS
443	442	15	24	19.6	32990	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
Data File : BP006842.D
Acq On : 24 Aug 2021 10:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 24 13:36:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 11:39:38 2021
Response via : Initial Calibration

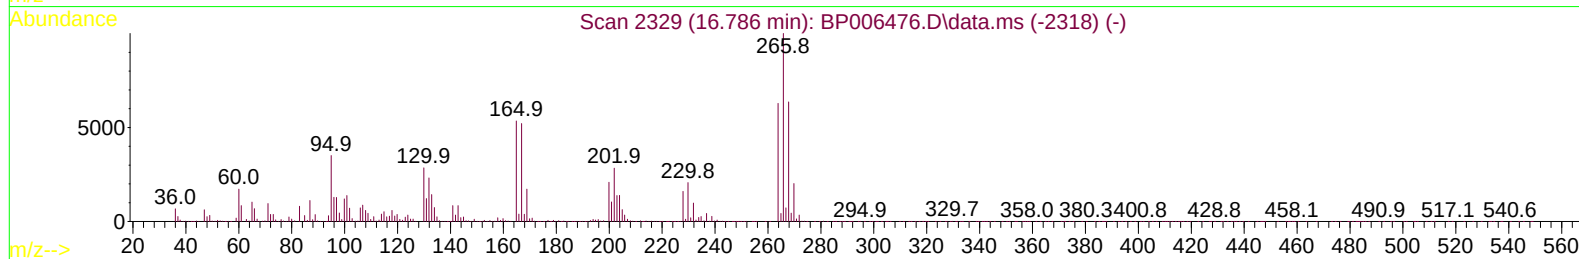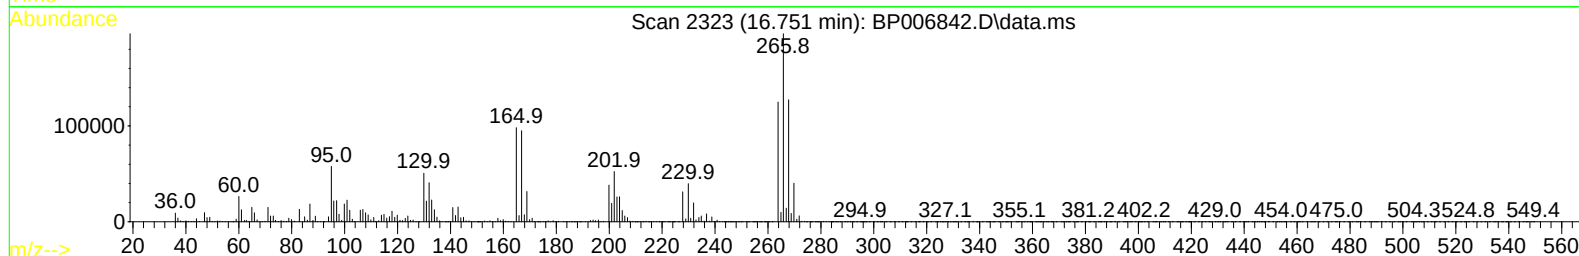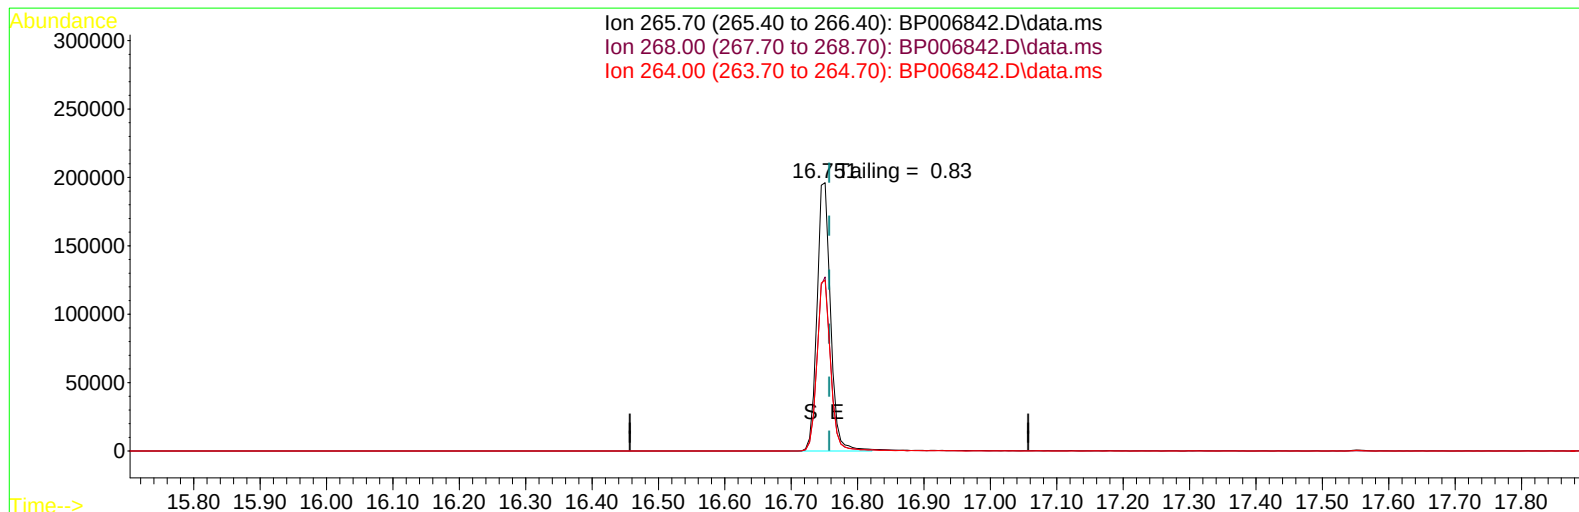

TIC: BP006842.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.006) 3685146.18 ng




response 280828

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.86
264.00	62.90	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006842.D
 Acq On : 24 Aug 2021 10:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 24 13:36:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 23 11:39:38 2021
 Response via : Initial Calibration

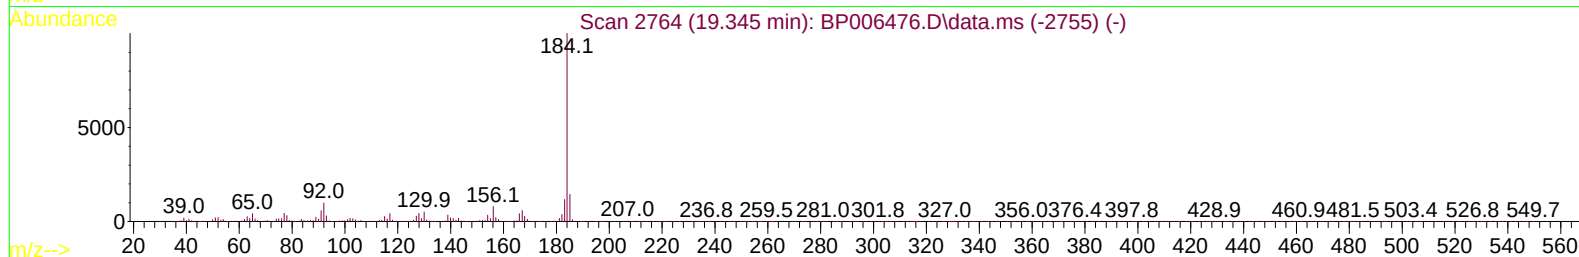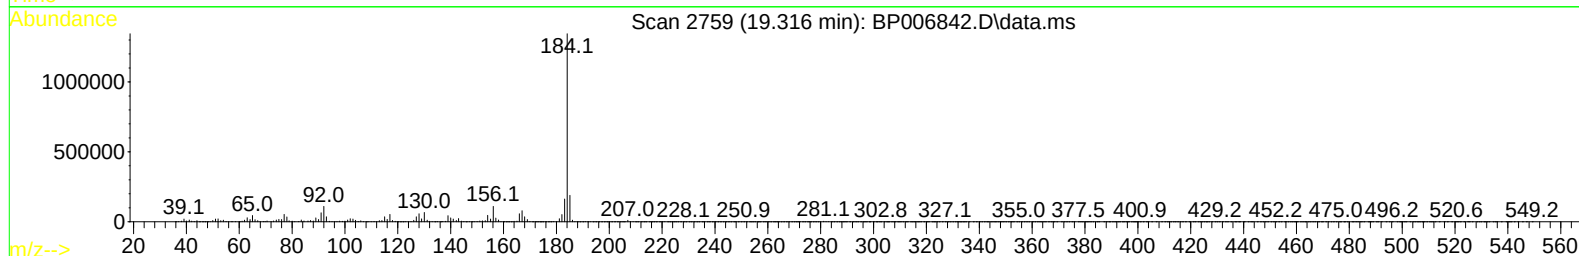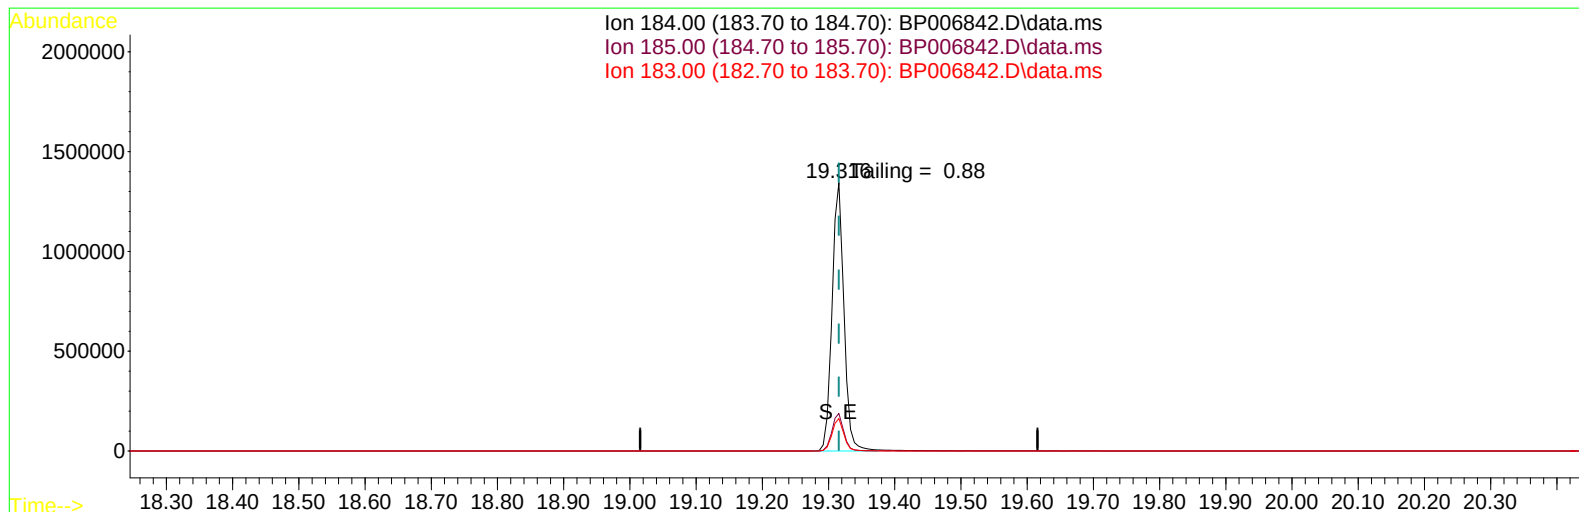

TIC: BP006842.D\data.ms

(77) Benzidine

19.316min (-0.000) 420550.98 ng

response 1694297

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.05
183.00	11.90	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2021	BNA_P	<u>BP006842.D</u>
Compound Name	Response	Retention Time
DDT	826718	20.51
DDD	16575	20.08
DDE	2212	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18787	845505	2.22