
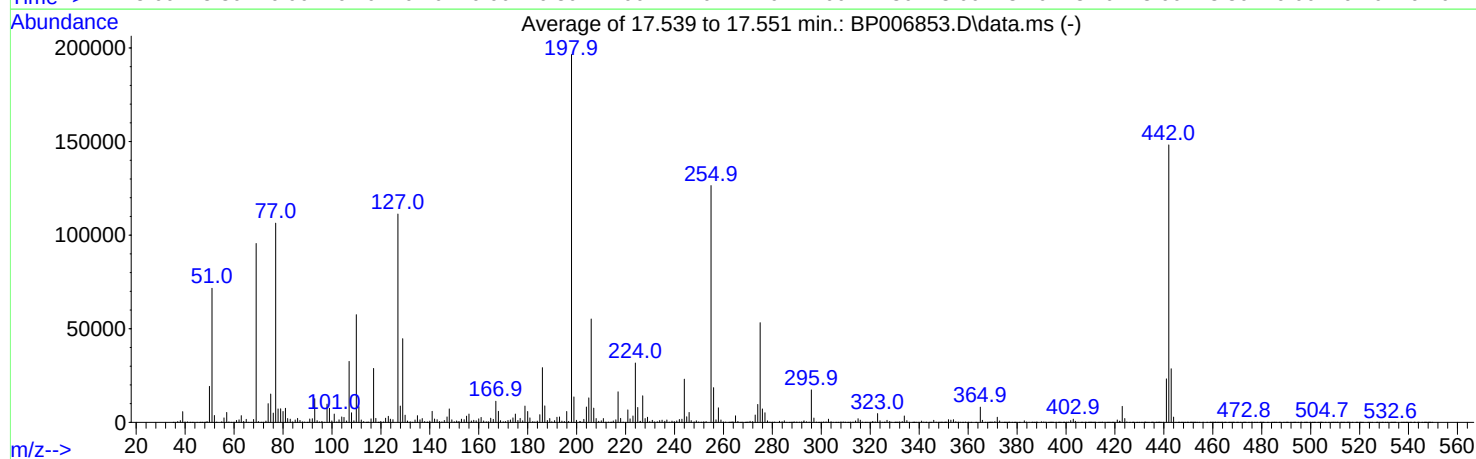


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006853.D
 Acq On : 24 Aug 2021 18:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 25 11:27:41 2021

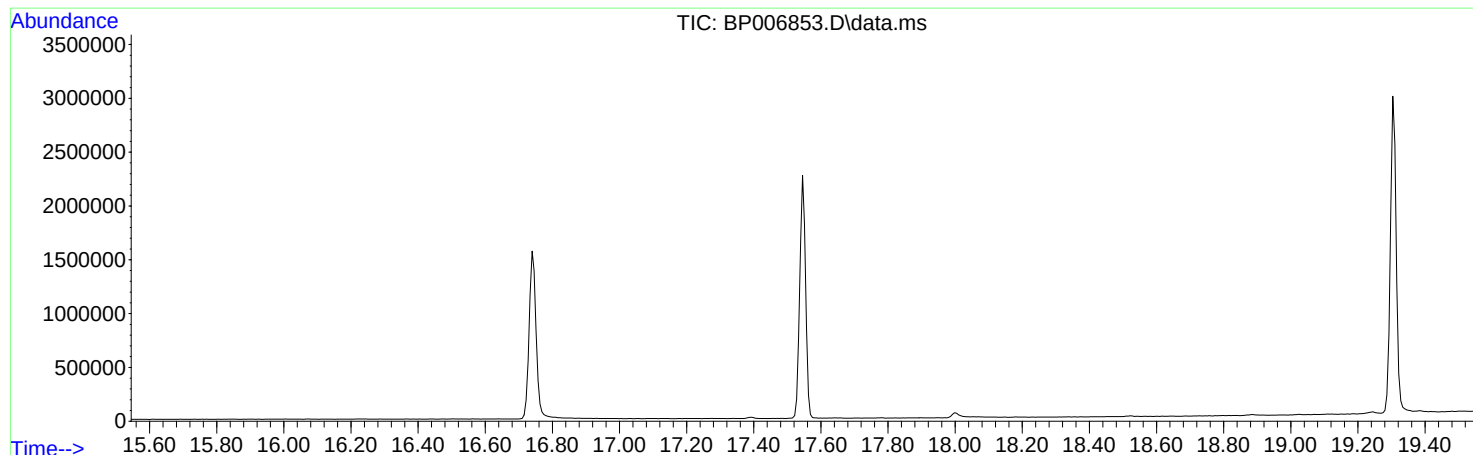




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	71675	PASS
68	69	0.00	2	1.6	1541	PASS
69	198	0.00	100	48.6	95541	PASS
70	69	0.00	2	0.5	465	PASS
127	198	10	80	56.6	111272	PASS
197	198	0.00	2	0.3	535	PASS
198	198	100	100	100.0	196536	PASS
199	198	5	9	6.9	13553	PASS
275	198	10	60	27.1	53248	PASS
365	198	1	100	4.1	8142	PASS
441	198	0.01	100	11.8	23242	PASS
442	442	100	100	100.0	148192	PASS
443	442	15	24	19.3	28608	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006853.D
 Acq On : 24 Aug 2021 18:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 05:40:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 13:40:38 2021
 Response via : Initial Calibration

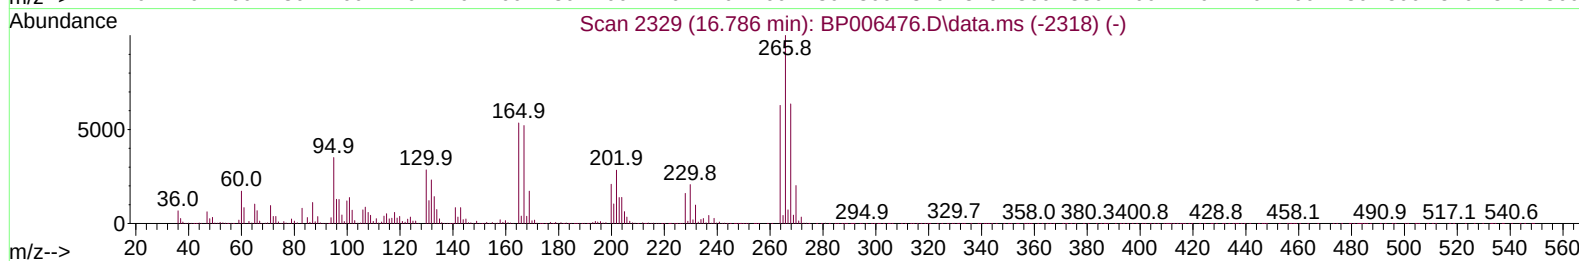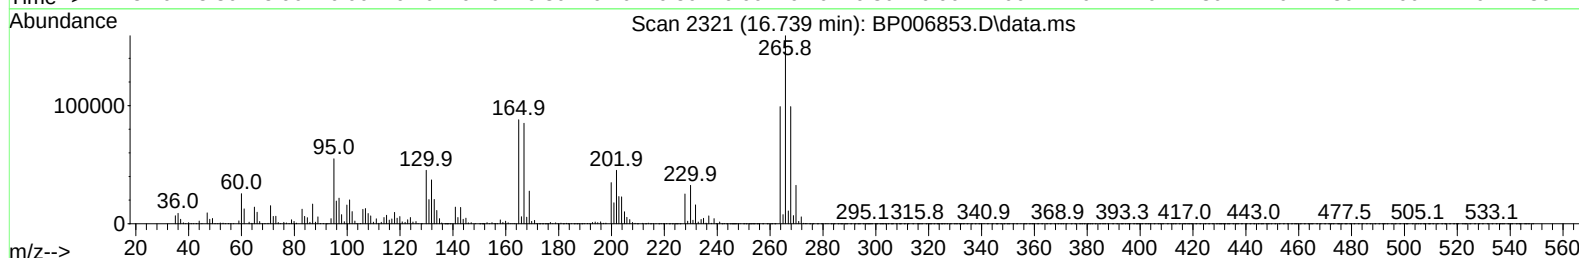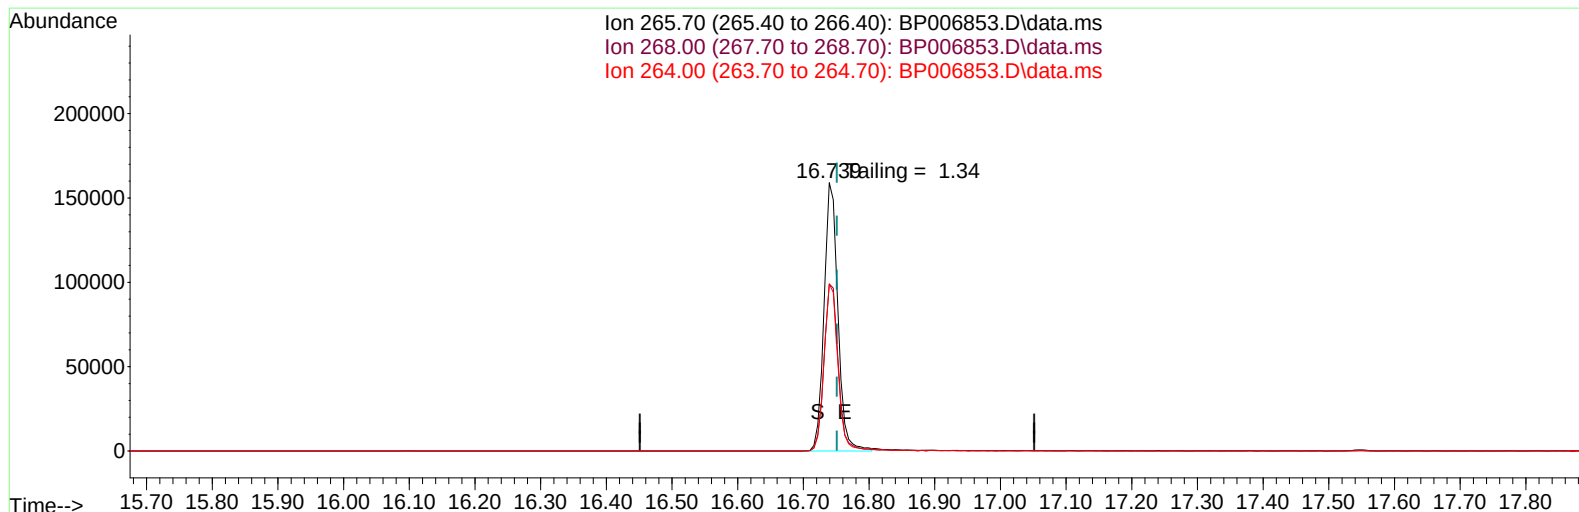

TIC: BP006853.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 1172618.21 ng




response 235585

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.28
264.00	62.90	62.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082421\
 Data File : BP006853.D
 Acq On : 24 Aug 2021 18:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 05:40:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 13:40:38 2021
 Response via : Initial Calibration

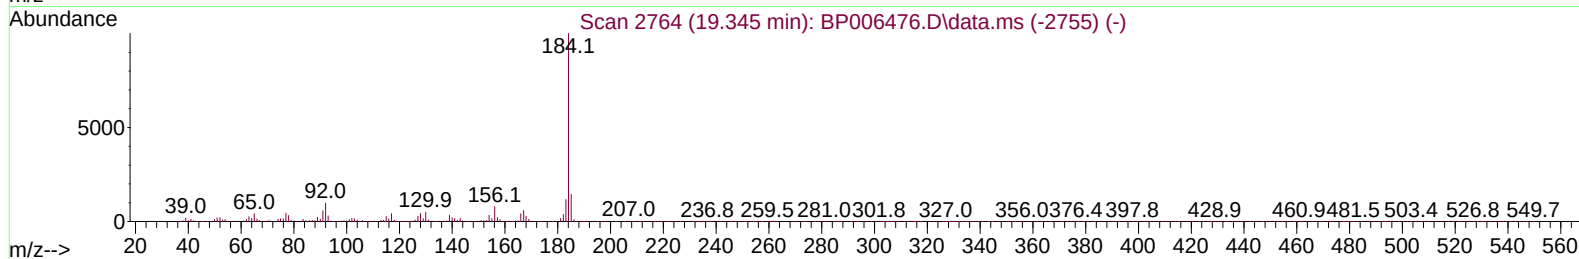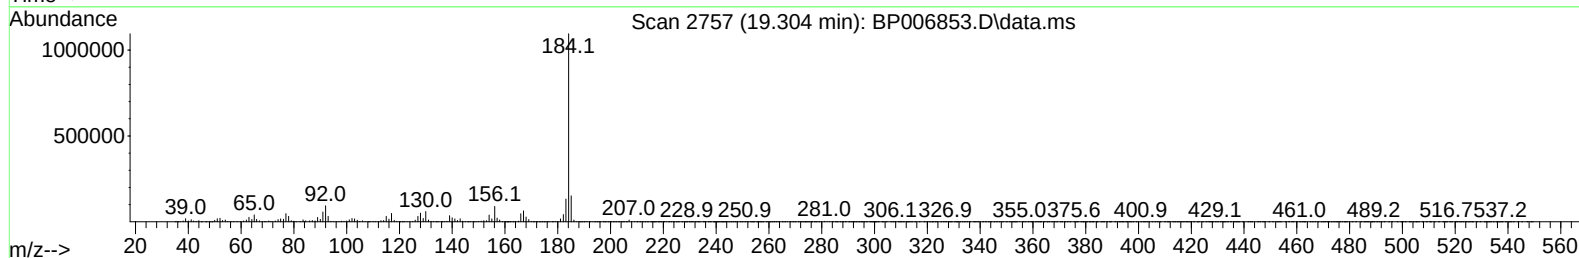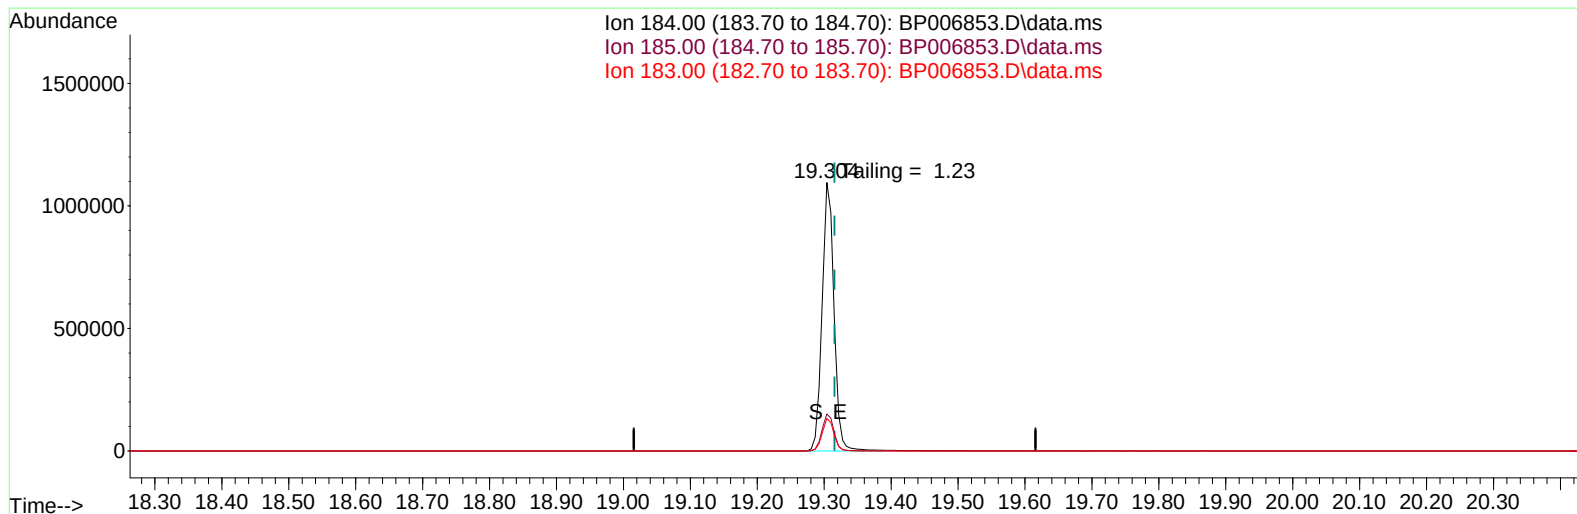

TIC: BP006853.D\data.ms

(77) Benzidine

19.304min (-0.012) 433477.16 ng

response 1355880

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.81
183.00	11.90	12.13
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
8/24/2021	BNA_P	<u>BP006853.D</u>
Compound Name	Response	Retention Time
DDT	665992	20.504
DDD	16733	20.075
DDE	2207	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18940	684932	2.77