

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011567.D
 Acq On : 25 Aug 2022 17:52
 Operator : CG/JU
 Sample : N4349-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Aug 26 01:06:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	60592	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	265836	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.216	164	161460	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	326739	20.000	ng/ul	0.00
79) Chrysene-d12	21.122	240	297711	20.000	ng/ul	0.00
88) Perylene-d12	23.404	264	312535	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	10271	5.260	ng/uL	0.00
4) Pyridine-d5	3.481	84	46731	9.348	ng/ul	0.00
7) Phenol-d5	6.734	99	37323	6.703	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.899	67	123827	34.230	ng/ul	0.00
11) 2-Chlorophenol-d4	7.081	132	110907	27.081	ng/ul	0.00
15) 4-Methylphenol-d8	8.269	113	71712	16.091	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	72124	37.686	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	38051	19.536	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	110271	30.671	ng/ul	0.00
31) 4-Chloroaniline-d4	10.487	131	200166	33.445	ng/ul	0.00
46) Dimethylphthalate-d6	13.646	166	435881	38.169	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	475853	37.492	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	13	0.006	ng/ul	0.00
60) Fluorene-d10	15.222	176	359989	37.470	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	209	0.118	ng/ul	0.03
73) Anthracene-d10	17.092	188	621689	42.961	ng/ul	0.00
81) Pyrene-d10	19.357	212	666871	44.273	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.257	264	636121	41.842	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.657	107	18206	3.914	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011567.D
Acq On : 25 Aug 2022 17:52
Operator : CG/JU
Sample : N4349-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Aug 26 01:06:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

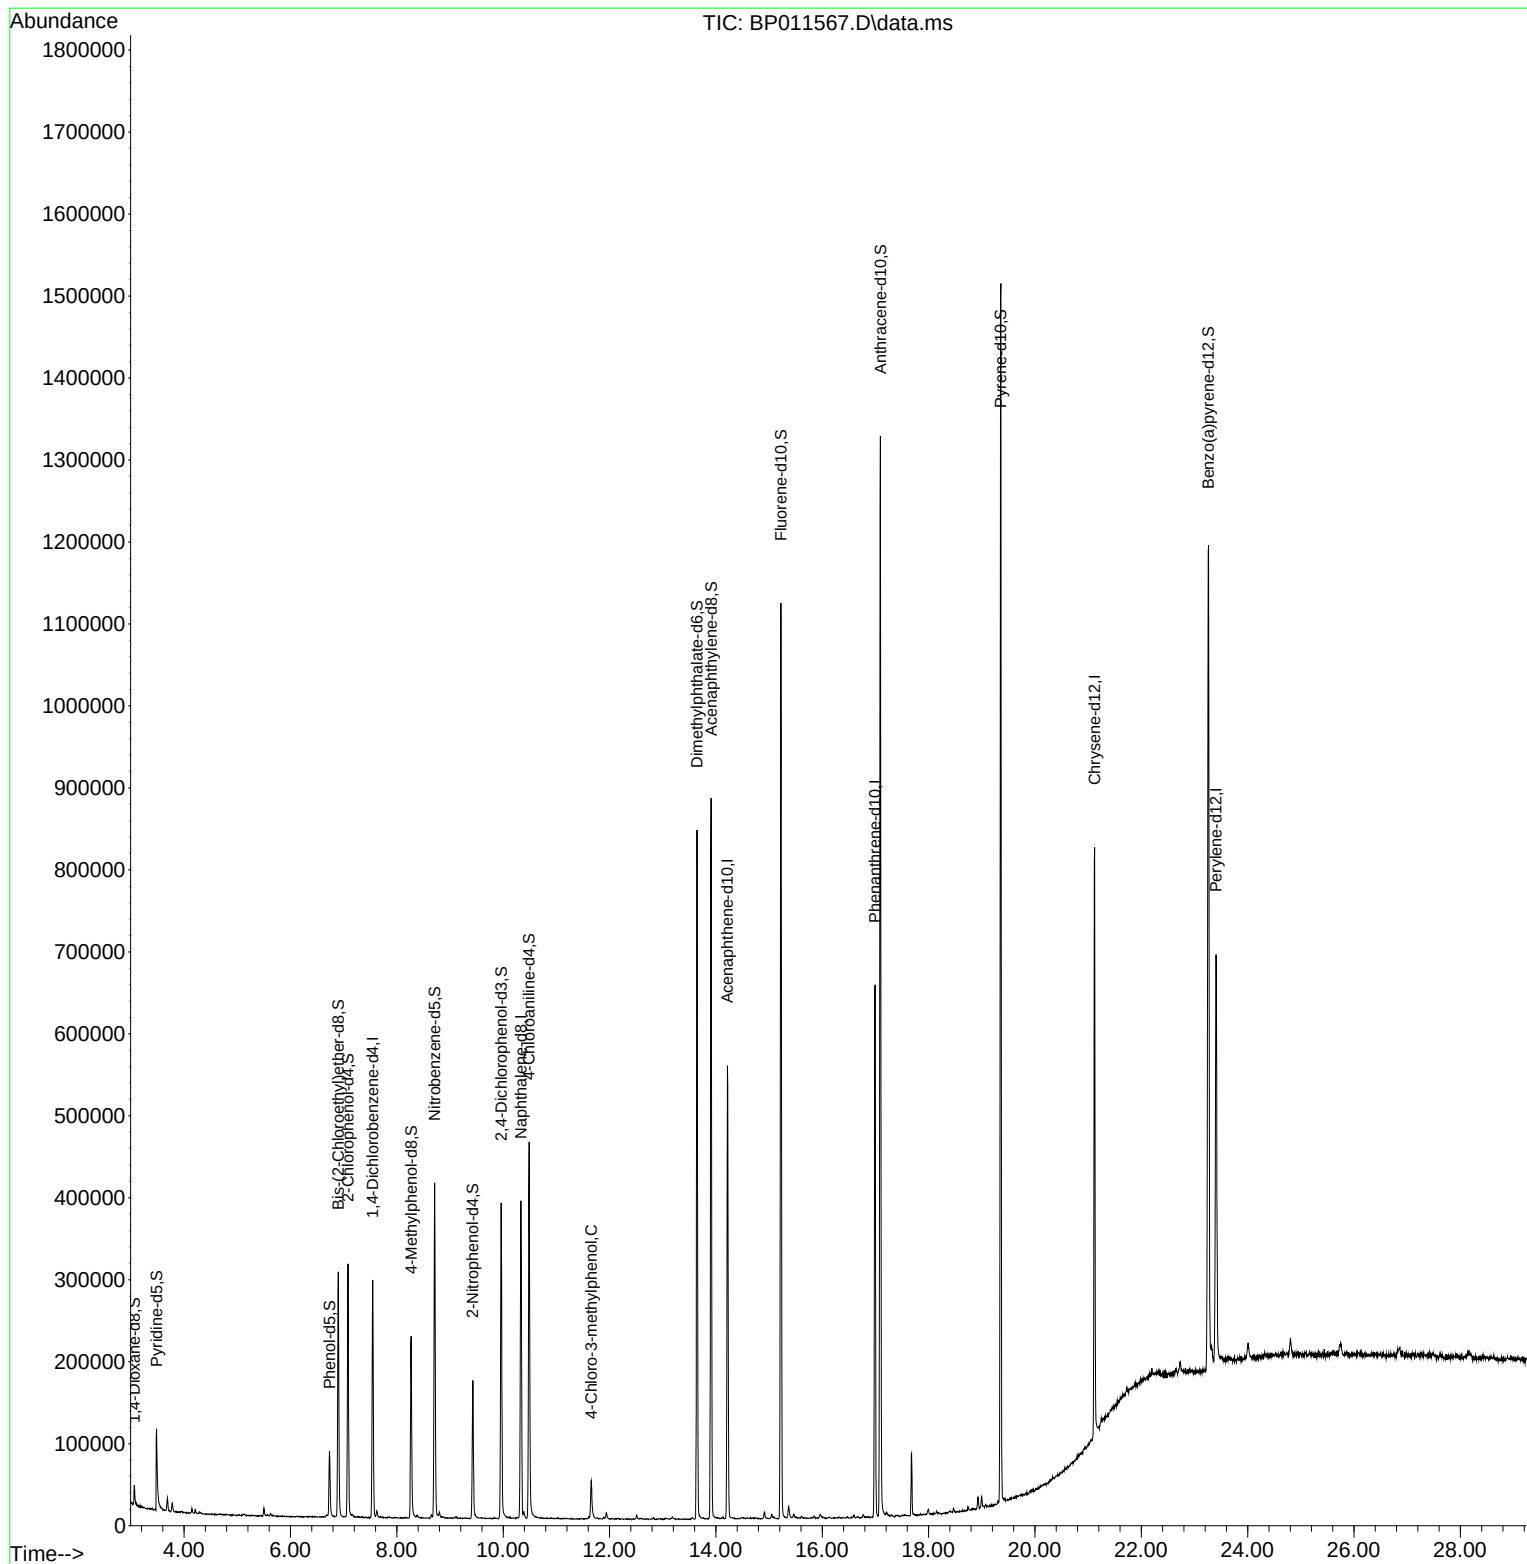

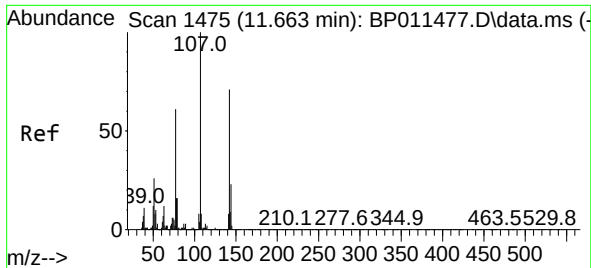

#35
 4-Chloro-3-methylphenol
 Concen: 3.914 ng/ul
 RT: 11.657 min Scan# 14
 Delta R.T. 0.000 min
 Lab File: BP011567.D
 Acq: 25 Aug 2022 17:52

Instrument :
 BNA_P
 ClientSampleId :

Tgt Ion:	107	Resp:	18206
Ion	Ratio	Lower	Upper
107	100		
144	23.0	18.3	27.5
142	72.1	55.8	83.8

