

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP082422\  
 Data File : BP011569.D  
 Acq On : 25 Aug 2022 19:02  
 Operator : CG/JU  
 Sample : N4349-04  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :

Quant Time: Aug 26 01:07:44 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP081622.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Aug 25 02:14:54 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| -----                         |        |      |          |        |       |          |
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.546  | 152  | 58908    | 20.000 | ng/ul | 0.00     |
| 20) Naphthalene-d8            | 10.334 | 136  | 251036   | 20.000 | ng/ul | 0.00     |
| 38) Acenaphthene-d10          | 14.216 | 164  | 154588   | 20.000 | ng/ul | 0.00     |
| 64) Phenanthrene-d10          | 16.986 | 188  | 304944   | 20.000 | ng/ul | 0.00     |
| 79) Chrysene-d12              | 21.116 | 240  | 283297   | 20.000 | ng/ul | -0.01    |
| 88) Perylene-d12              | 23.404 | 264  | 304268   | 20.000 | ng/ul | -0.01    |
|                               |        |      |          |        |       |          |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.063  | 96   | 8814     | 4.643  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.481  | 84   | 40068    | 8.244  | ng/ul | 0.00     |
| 7) Phenol-d5                  | 6.734  | 99   | 34440    | 6.362  | ng/ul | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 6.893  | 67   | 102722   | 29.207 | ng/ul | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.081  | 132  | 96689    | 24.284 | ng/ul | 0.00     |
| 15) 4-Methylphenol-d8         | 8.269  | 113  | 65666    | 15.155 | ng/ul | 0.00     |
| 21) Nitrobenzene-d5           | 8.710  | 128  | 59570    | 32.961 | ng/ul | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.428  | 143  | 53053    | 28.844 | ng/ul | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 9.963  | 165  | 93304    | 27.481 | ng/ul | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.487 | 131  | 127174   | 22.502 | ng/ul | 0.00     |
| 46) Dimethylphthalate-d6      | 13.645 | 166  | 375998   | 34.389 | ng/ul | 0.00     |
| 49) Acenaphthylene-d8         | 13.910 | 160  | 397828   | 32.737 | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.457 | 143  | 5310     | 2.521  | ng/ul | 0.00     |
| 60) Fluorene-d10              | 15.222 | 176  | 313889   | 34.124 | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.363 | 200  | 26622    | 16.156 | ng/ul | 0.00     |
| 73) Anthracene-d10            | 17.092 | 188  | 545000   | 40.354 | ng/ul | 0.00     |
| 81) Pyrene-d10                | 19.351 | 212  | 585925   | 40.879 | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.257 | 264  | 569944   | 38.508 | ng/ul | 0.00     |
|                               |        |      |          |        |       |          |
| Target Compounds              |        |      |          |        |       | Qvalue   |
| 35) 4-Chloro-3-methylphenol   | 11.657 | 107  | 15254    | 3.472  | ng/ul | 93       |
| -----                         |        |      |          |        |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP082422\  
Data File : BP011569.D  
Acq On : 25 Aug 2022 19:02  
Operator : CG/JU  
Sample : N4349-04  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :

Quant Time: Aug 26 01:07:44 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP081622.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Aug 25 02:14:54 2022  
Response via : Initial Calibration

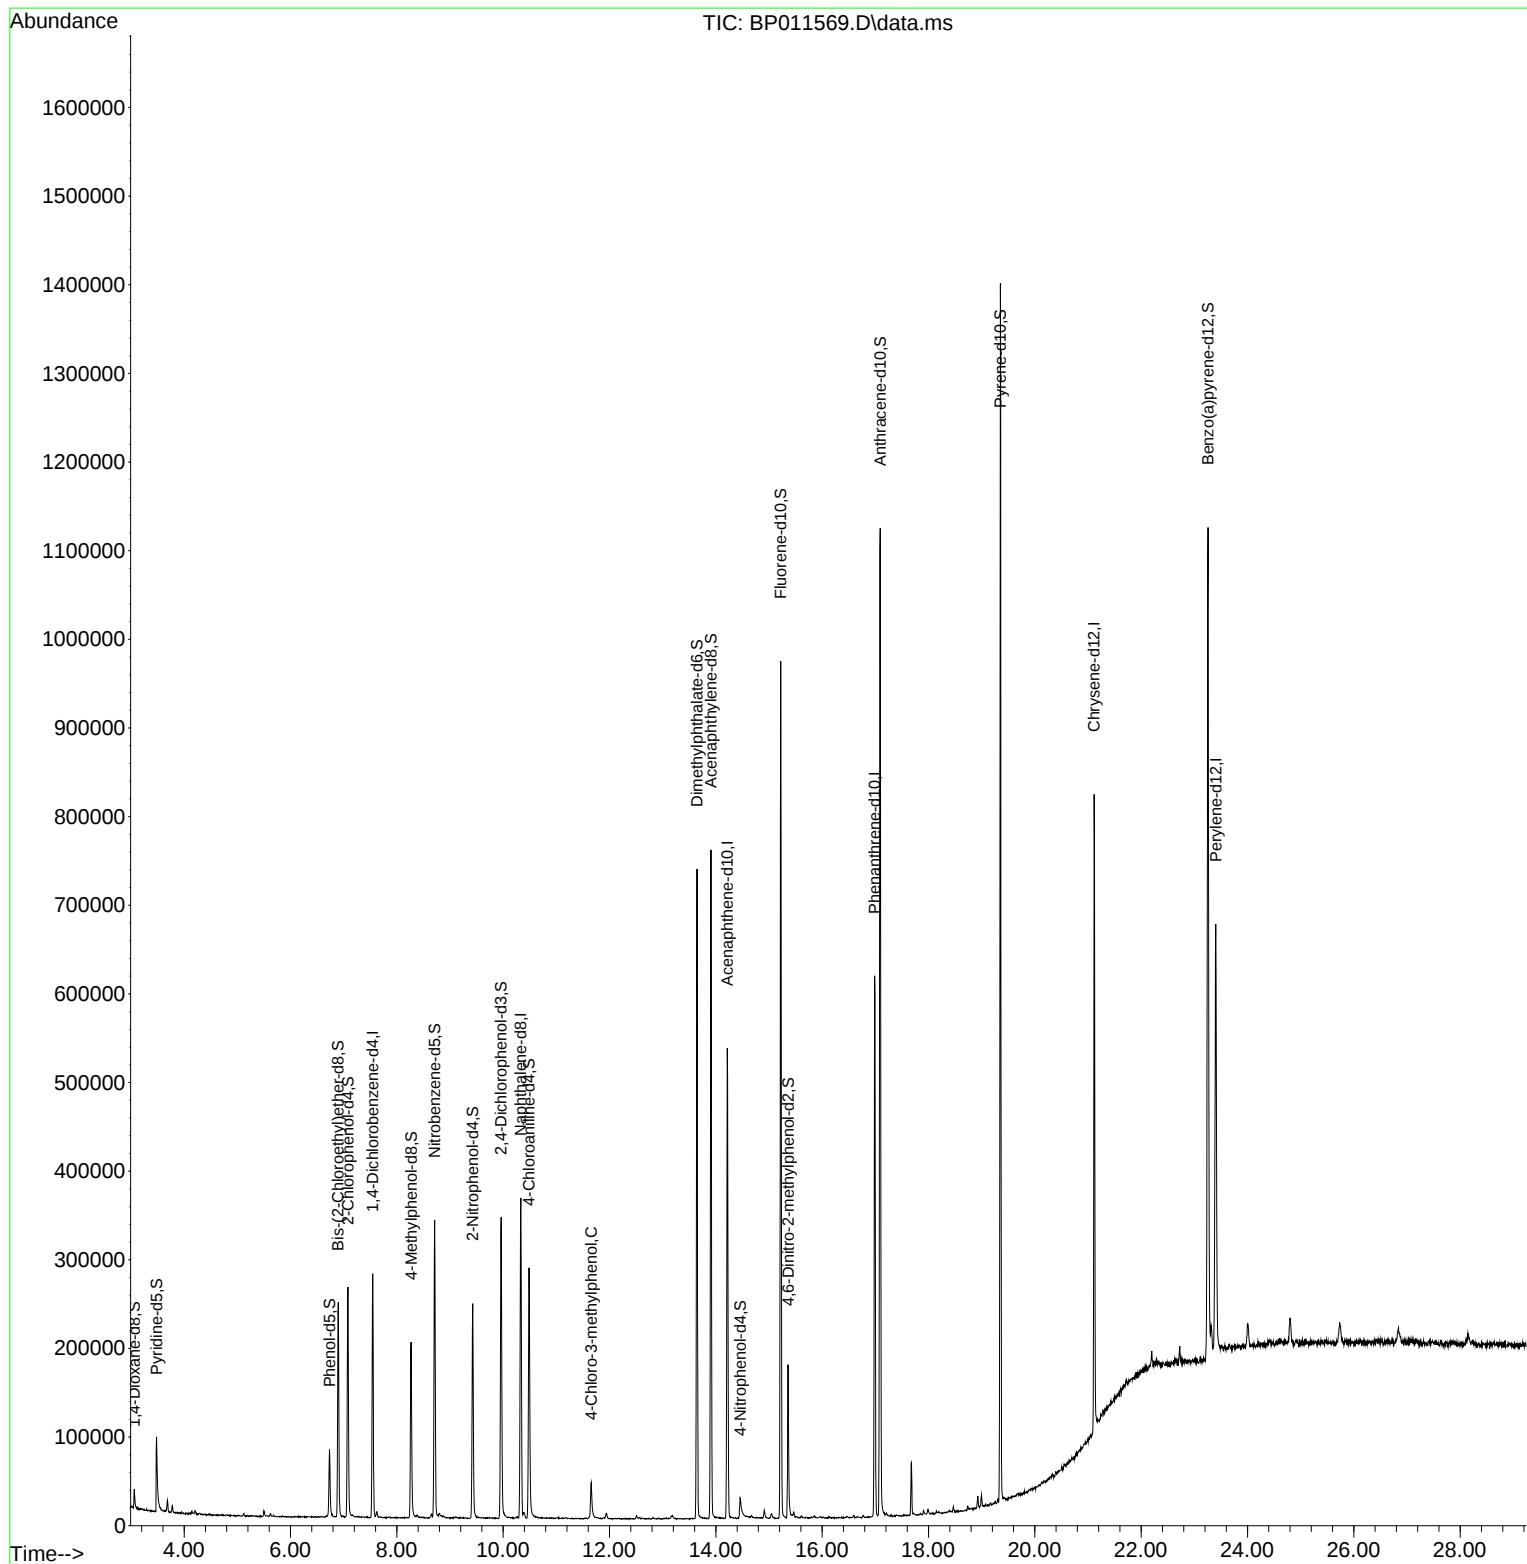

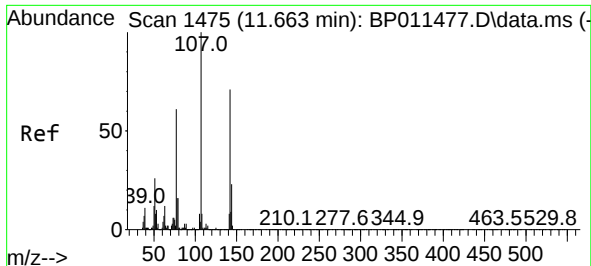

#35  
 4-Chloro-3-methylphenol  
 Concen: 3.472 ng/ul  
 RT: 11.657 min Scan# 14  
 Delta R.T. -0.000 min  
 Lab File: BP011569.D  
 Acq: 25 Aug 2022 19:02

Instrument :  
 BNA\_P  
 ClientSampleId :

Tgt Ion:107 Resp: 15254  
 Ion Ratio Lower Upper  
 107 100  
 144 26.8 18.3 27.5  
 142 64.5 55.8 83.8

