




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011551.D
 Acq On : 24 Aug 2022 21:20
 Operator : CG/JU
 Sample : N4320-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX6

Manual IntegrationsAPPROVED

Quant Time: Aug 25 02:19:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/25/2022
 Supervised By :mohammad ahmed 08/27/2022

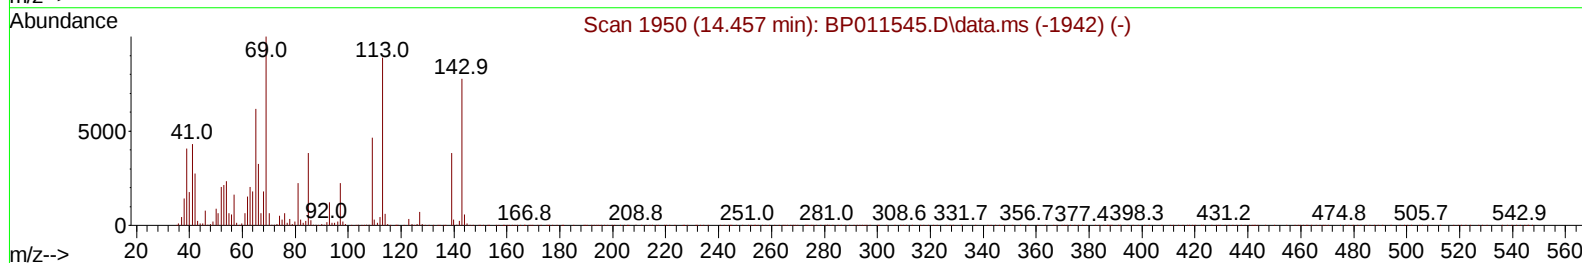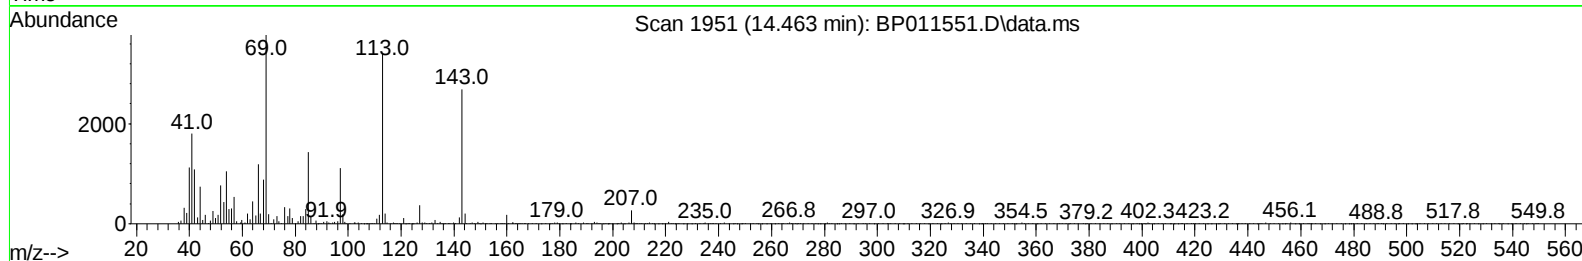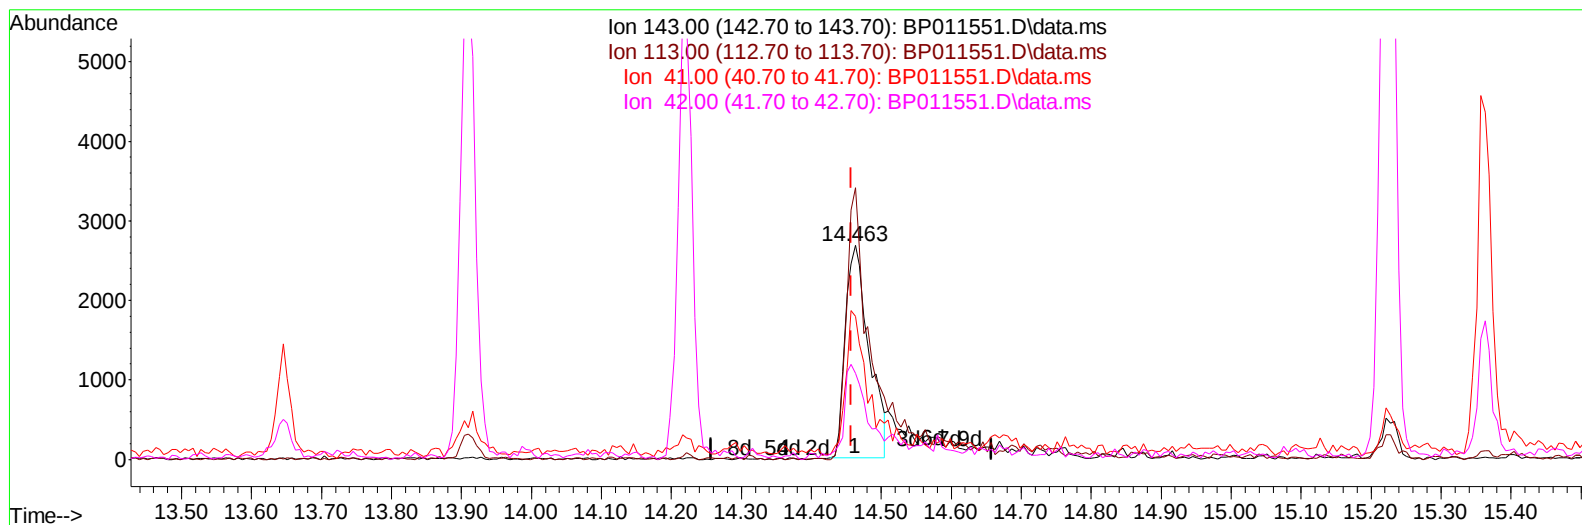

TIC: BP011551.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.463min (+ 0.006) 3.53 ng/ul

response 6239

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	109.60	126.90
41.00	52.50	67.00#
42.00	35.70	40.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011551.D
 Acq On : 24 Aug 2022 21:20
 Operator : CG/JU
 Sample : N4320-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX6

Manual IntegrationsAPPROVED

Quant Time: Aug 25 02:19:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/25/2022
 Supervised By :mohammad ahmed 08/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	53566	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	223727	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.222	164	129623	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	273337	20.000	ng/ul	0.00
79) Chrysene-d12	21.121	240	254717	20.000	ng/ul	0.00
88) Perylene-d12	23.410	264	275440	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	8437	4.888	ng/uL	0.00
4) Pyridine-d5	3.487	84	26594	6.018	ng/ul	0.01
7) Phenol-d5	6.734	99	31421	6.383	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.899	67	101121	31.620	ng/ul	0.00
11) 2-Chlorophenol-d4	7.081	132	94978	26.234	ng/ul	0.00
15) 4-Methylphenol-d8	8.269	113	58969	14.967	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	58551	36.352	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	56752	34.621	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	90428	29.885	ng/ul	0.00
31) 4-Chloroaniline-d4	10.487	131	115076	22.847	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166	354140	38.628	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	382001	37.489	ng/ul	0.00
54) 4-Nitrophenol-d4	14.463	143	6835m	3.869	ng/ul	0.00
60) Fluorene-d10	15.228	176	291218	37.757	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	48653	32.941	ng/ul	0.00
73) Anthracene-d10	17.092	188	536724	44.336	ng/ul	0.00
81) Pyrene-d10	19.357	212	585828	45.458	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.262	264	578103	43.147	ng/ul	0.00
Target Compounds						
78) Di-n-butylphthalate	17.986	149	37283	2.156	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011551.D
Acq On : 24 Aug 2022 21:20
Operator : CG/JU
Sample : N4320-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/25/2022
Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 25 02:19:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

