




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011560.D
 Acq On : 25 Aug 2022 11:53
 Operator : CG/JU
 Sample : N4320-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX8

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:03:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

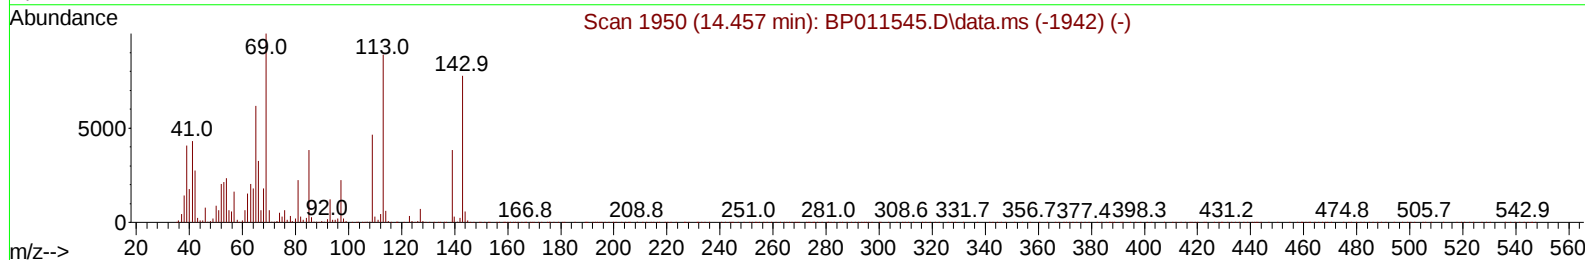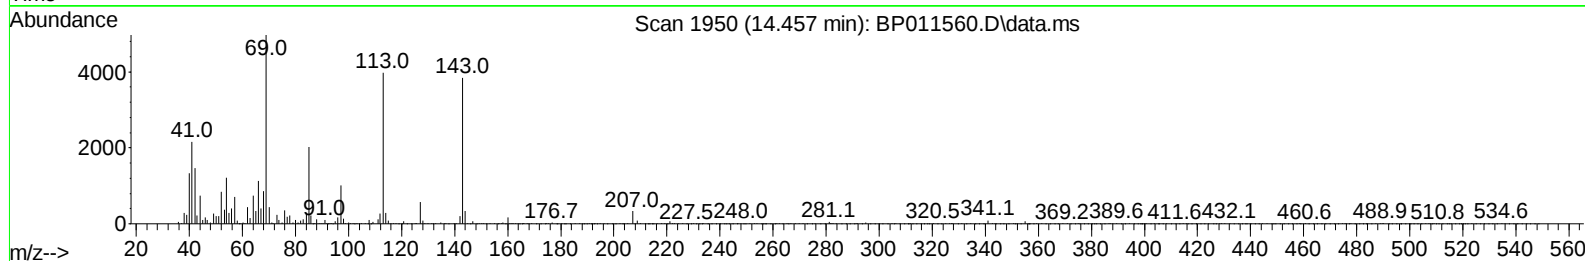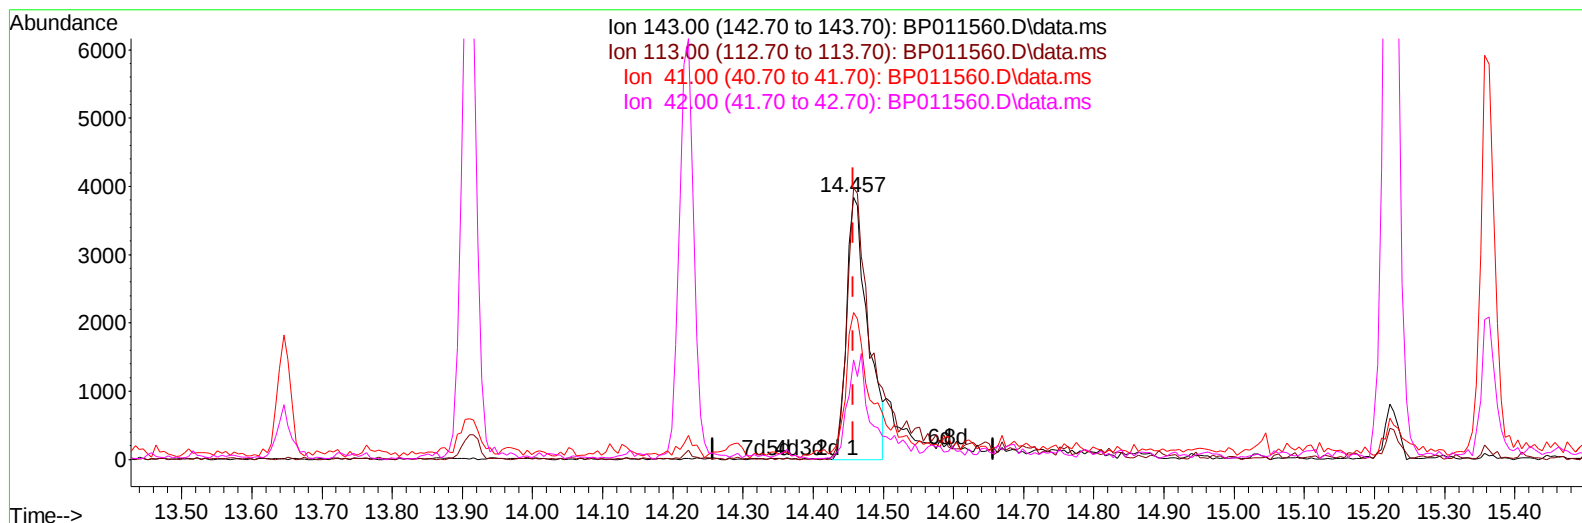

TIC: BP011560.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.457min (+ 0.000) 3.78 ng/u1

response 8055

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	109.60	103.49
41.00	52.50	56.10
42.00	35.70	38.02




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011560.D
 Acq On : 25 Aug 2022 11:53
 Operator : CG/JU
 Sample : N4320-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX8

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:03:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

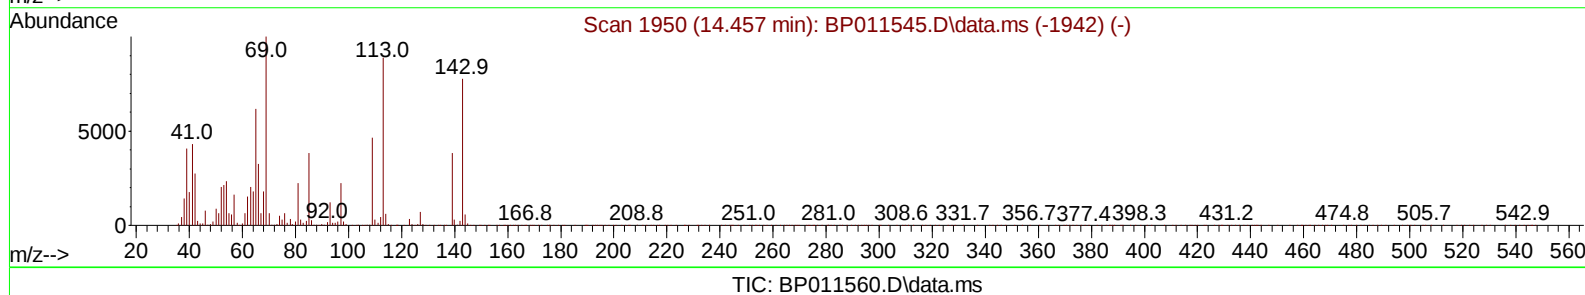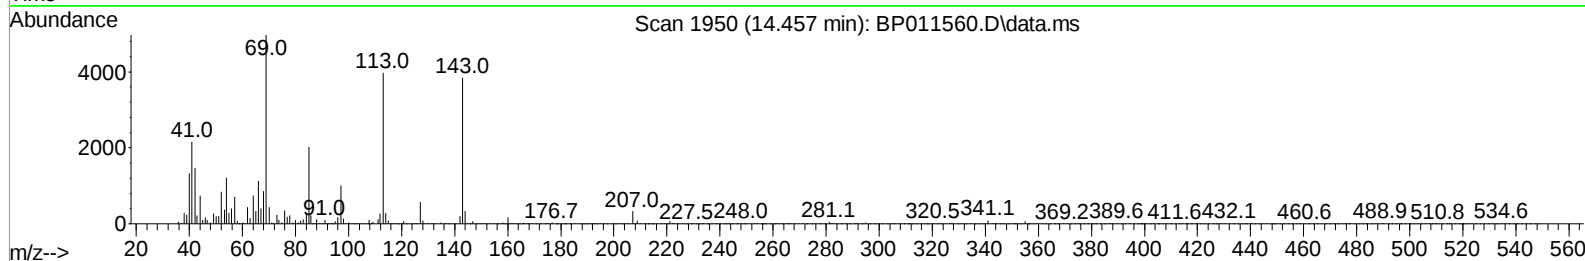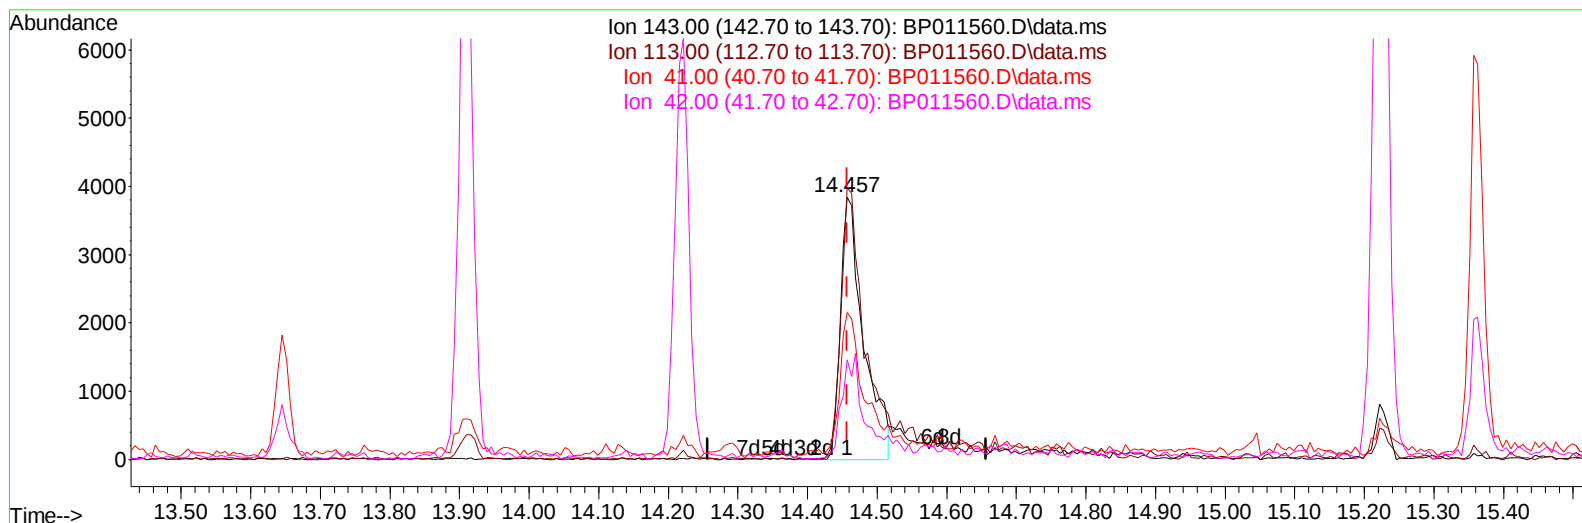

(54) 4-Nitrophenol-d4 (S)

14.457min (+ 0.000) 4.15 ng/ul m

response 8836

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	109.60	103.49
41.00	52.50	56.10
42.00	35.70	38.02

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011560.D
 Acq On : 25 Aug 2022 11:53
 Operator : CG/JU
 Sample : N4320-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX8

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:03:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	62095	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	267751	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.222	164	156307	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	316136	20.000	ng/ul	0.00
79) Chrysene-d12	21.122	240	287067	20.000	ng/ul	0.00
88) Perylene-d12	23.410	264	287913	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	10470	5.232	ng/uL	0.00
4) Pyridine-d5	3.487	84	26531	5.179	ng/ul	0.01
7) Phenol-d5	6.734	99	42388	7.428	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.899	67	132674	35.788	ng/ul	0.00
11) 2-Chlorophenol-d4	7.081	132	125111	29.810	ng/ul	0.00
15) 4-Methylphenol-d8	8.269	113	79606	17.430	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	76977	39.934	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	77205	39.355	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	123450	34.091	ng/ul	0.00
31) 4-Chloroaniline-d4	10.487	131	128219	21.270	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166	473381	42.819	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	511368	41.618	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	8836m	4.148	ng/ul	0.00
60) Fluorene-d10	15.228	176	388174	41.736	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	61464	35.981	ng/ul	0.00
73) Anthracene-d10	17.092	188	627281	44.802	ng/ul	0.00
81) Pyrene-d10	19.357	212	676580	46.583	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.268	264	632880	45.189	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011560.D
Acq On : 25 Aug 2022 11:53
Operator : CG/JU
Sample : N4320-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:03:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

