




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011563.D
 Acq On : 25 Aug 2022 13:38
 Operator : CG/JU
 Sample : N4320-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX5

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:04:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

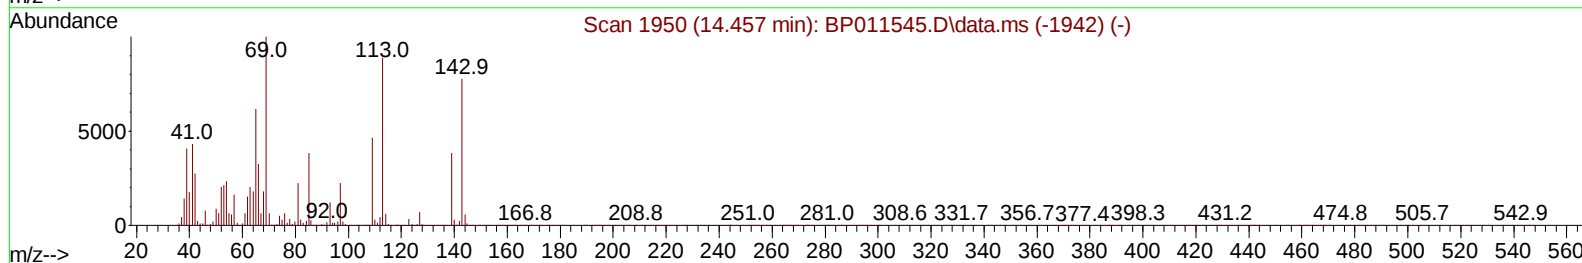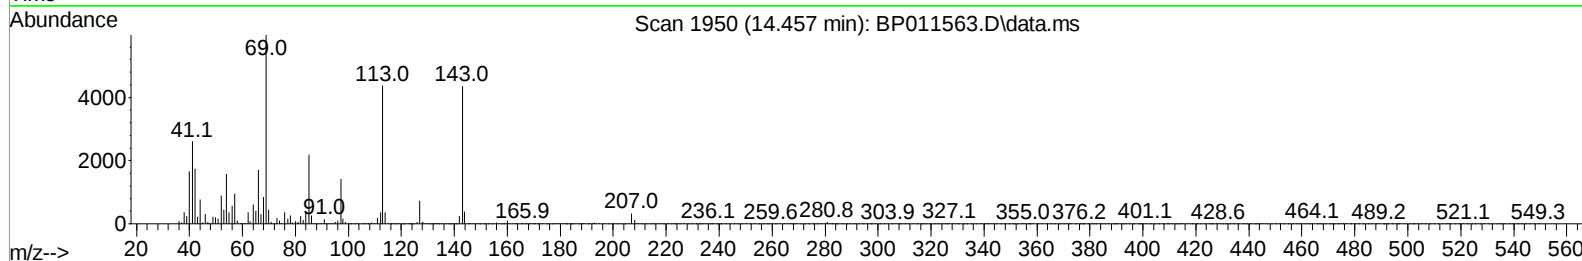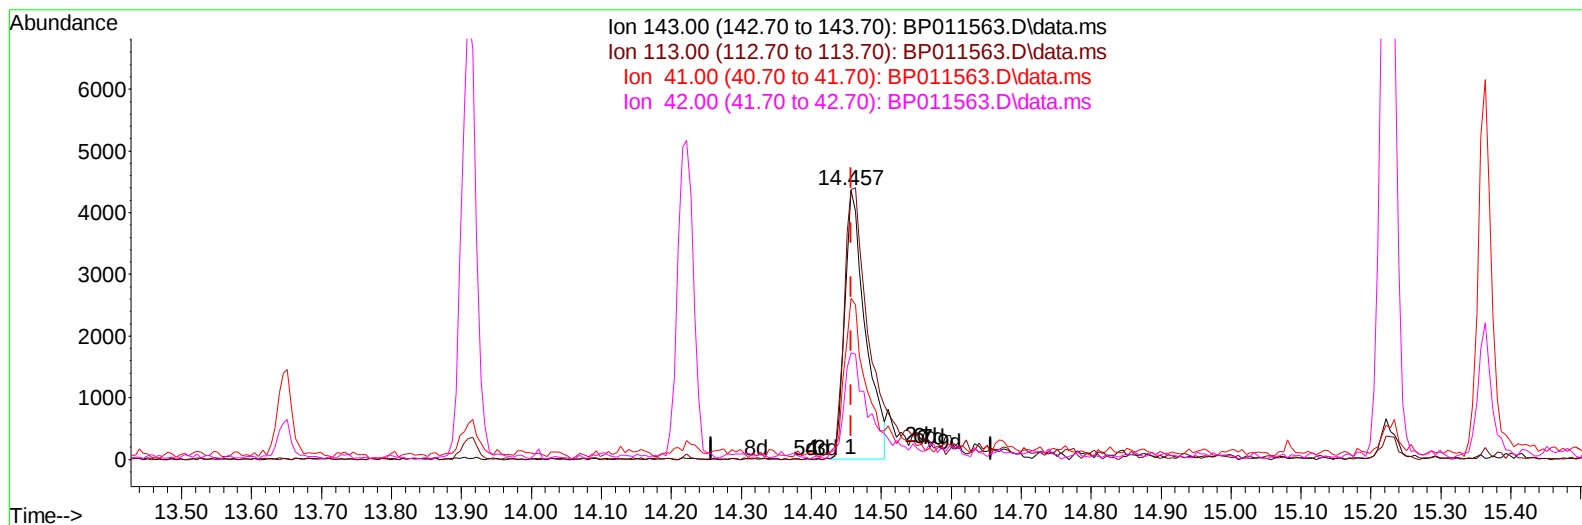

TIC: BP011563.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.457min (-0.000) 4.72 ng/u1

response 8863

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	109.60	100.07
41.00	52.50	59.85
42.00	35.70	39.69




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011563.D
 Acq On : 25 Aug 2022 13:38
 Operator : CG/JU
 Sample : N4320-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX5

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:04:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

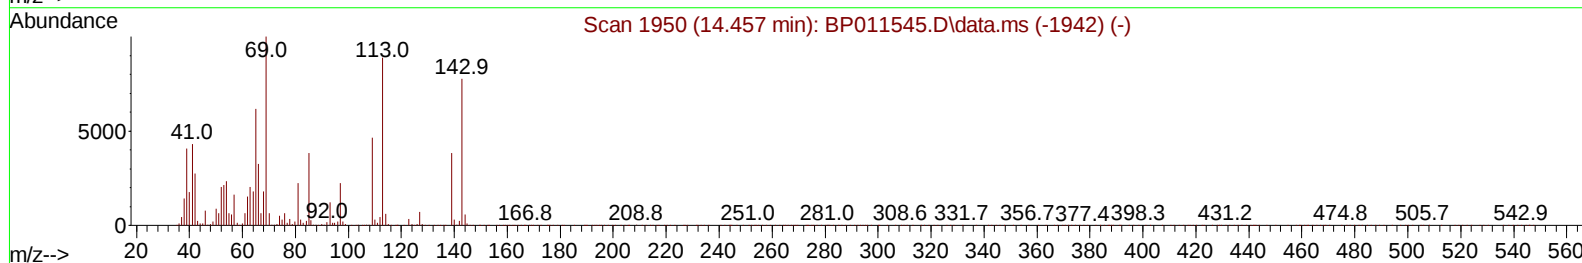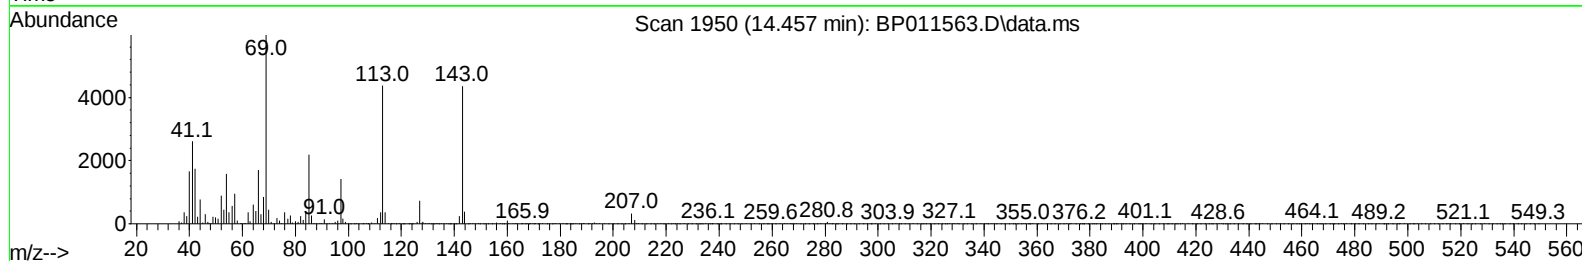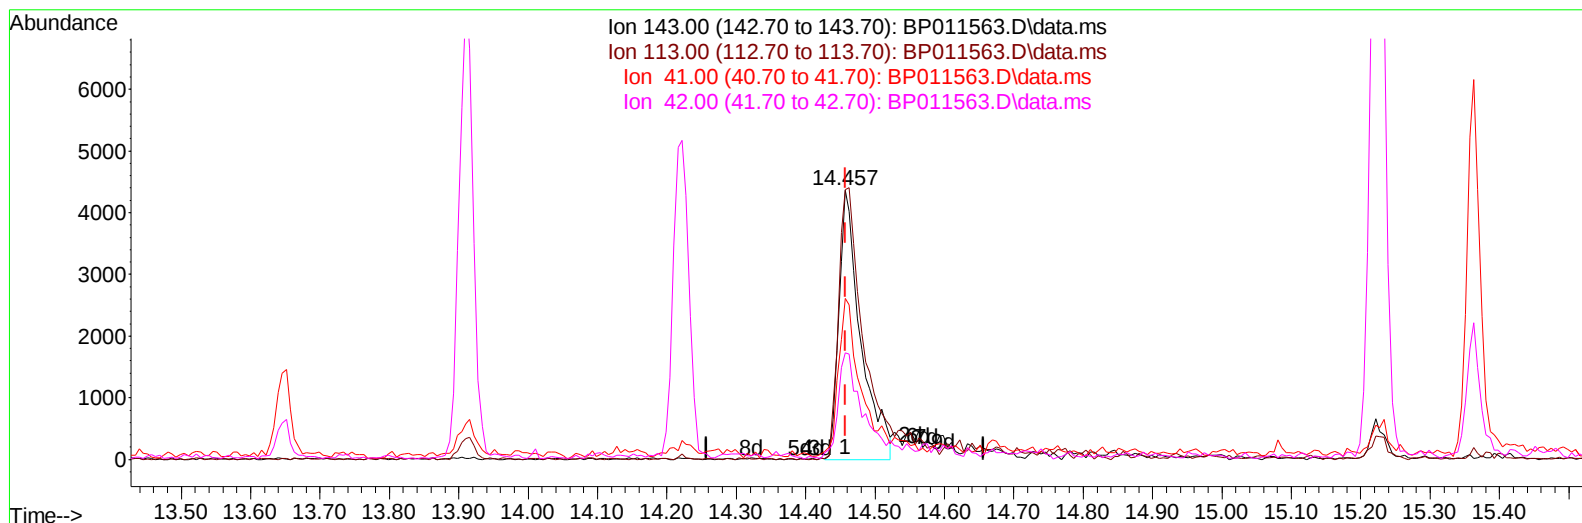

TIC: BP011563.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.457min (-0.000) 5.07 ng/ul m

response 9508

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	109.60	100.07
41.00	52.50	59.85
42.00	35.70	39.69

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011563.D
 Acq On : 25 Aug 2022 13:38
 Operator : CG/JU
 Sample : N4320-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:04:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	51735	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	225827	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.222	164	137747	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	281279	20.000	ng/ul	0.00
79) Chrysene-d12	21.121	240	252815	20.000	ng/ul	0.00
88) Perylene-d12	23.415	264	272779	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	8422	5.052	ng/uL	0.00
4) Pyridine-d5	3.481	84	32880	7.703	ng/ul	0.00
7) Phenol-d5	6.734	99	36192	7.613	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.899	67	106500	34.480	ng/ul	0.00
11) 2-Chlorophenol-d4	7.081	132	100668	28.789	ng/ul	0.00
15) 4-Methylphenol-d8	8.269	113	69953	18.383	ng/ul	0.00
21) Nitrobenzene-d5	8.716	128	62834	38.648	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	62497	37.771	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	102906	33.693	ng/ul	0.00
31) 4-Chloroaniline-d4	10.493	131	119170	23.439	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166	417175	42.819	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	425912	39.334	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	9508m	5.065	ng/ul	0.00
60) Fluorene-d10	15.228	176	347273	42.369	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	56594	37.235	ng/ul	0.00
73) Anthracene-d10	17.092	188	591659	47.494	ng/ul	0.00
81) Pyrene-d10	19.357	212	634438	49.600	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.268	264	610955	46.044	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011563.D
Acq On : 25 Aug 2022 13:38
Operator : CG/JU
Sample : N4320-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:04:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

