




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011566.D
Acq On : 25 Aug 2022 17:17
Operator : CG/JU
Sample : N4349-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGN62

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:06:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

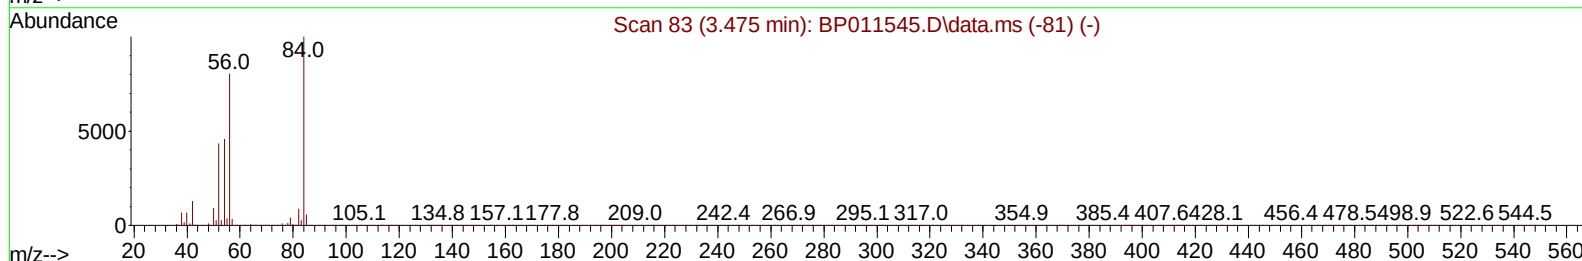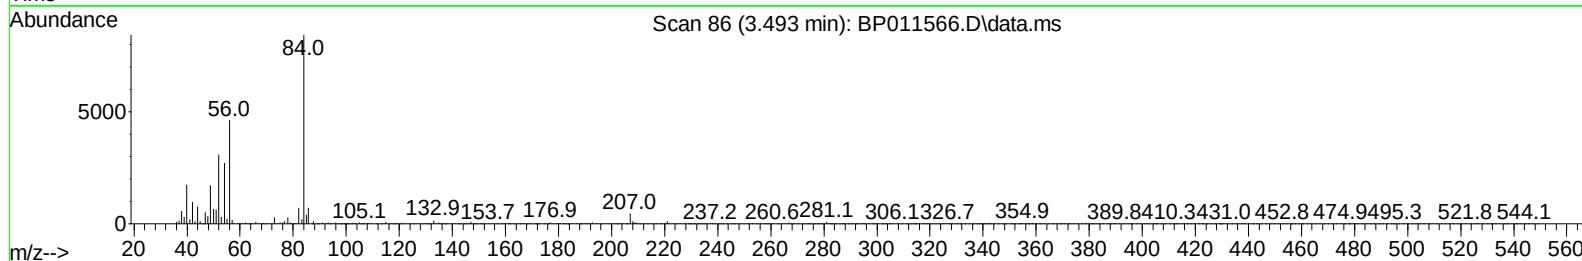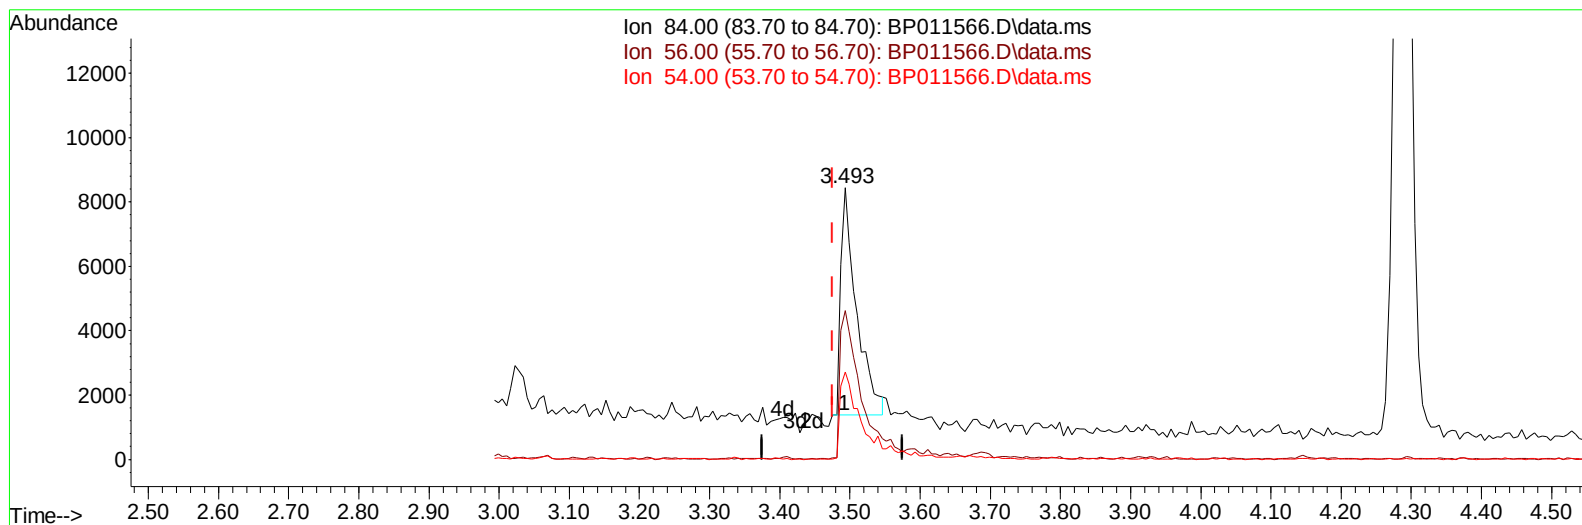

TIC: BP011566.D\data.ms

(4) Pyridine-d5 (S)

3.493min (+ 0.018) 2.19 ng/u1

response 10958

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	72.90	54.81#
54.00	42.10	32.27#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011566.D
 Acq On : 25 Aug 2022 17:17
 Operator : CG/JU
 Sample : N4349-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGN62

Manual IntegrationsAPPROVED

Quant Time: Aug 26 01:06:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

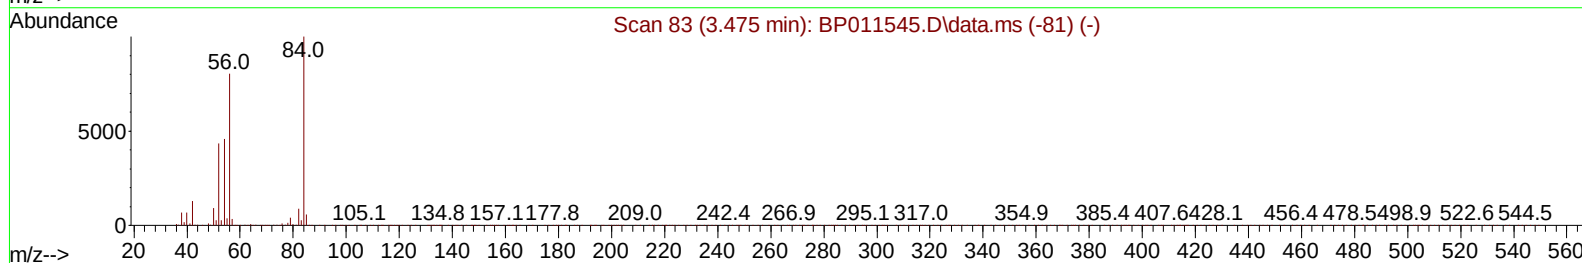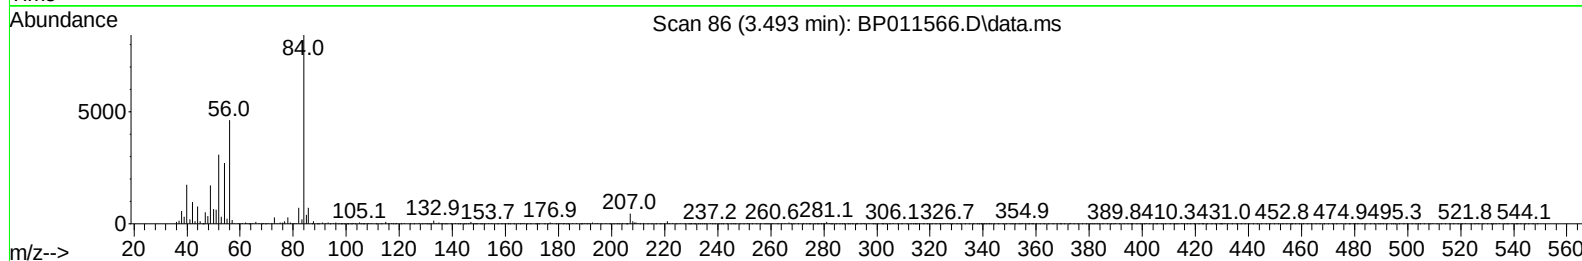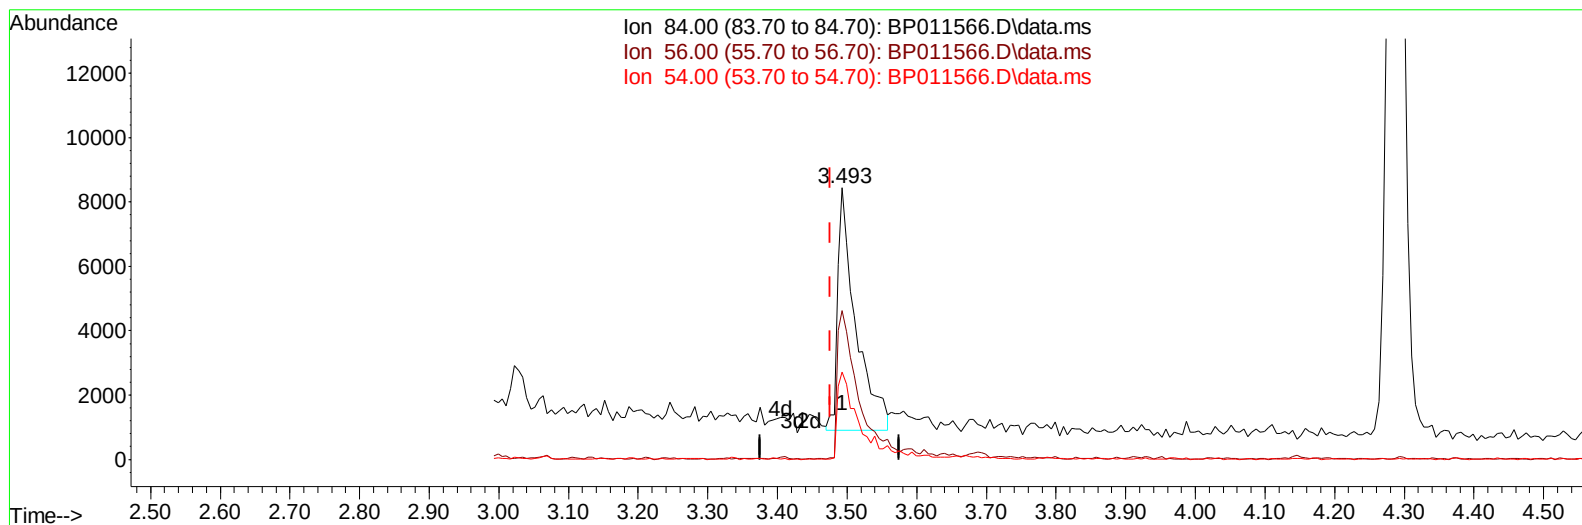

TIC: BP011566.D\data.ms

(4) Pyridine-d5 (S)

3.493min (+ 0.018) 2.73 ng/ul m

response 13673

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	72.90	54.81#
54.00	42.10	32.27#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011566.D
 Acq On : 25 Aug 2022 17:17
 Operator : CG/JU
 Sample : N4349-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGN62

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:06:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	60692	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	259679	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.222	164	155083	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	306546	20.000	ng/ul	0.00
79) Chrysene-d12	21.121	240	288455	20.000	ng/ul	0.00
88) Perylene-d12	23.410	264	306423	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	8316	4.252	ng/uL	0.00
4) Pyridine-d5	3.493	84	13673m	2.731	ng/ul	0.02
7) Phenol-d5	6.734	99	33984	6.093	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.899	67	96007	26.496	ng/ul	0.00
11) 2-Chlorophenol-d4	7.081	132	92933	22.655	ng/ul	0.00
15) 4-Methylphenol-d8	8.269	113	62642	14.032	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	55266	29.562	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	56137	29.505	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	93251	26.552	ng/ul	0.00
31) 4-Chloroaniline-d4	10.487	131	112160	19.185	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166	371903	33.906	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	371903	30.506	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	9119	4.315	ng/ul	0.00
60) Fluorene-d10	15.222	176	303449	32.884	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	51364	31.009	ng/ul	0.00
73) Anthracene-d10	17.092	188	543853	40.058	ng/ul	0.00
81) Pyrene-d10	19.351	212	591995	40.564	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.262	264	582590	39.085	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.099	88	2481	1.217	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011566.D
Acq On : 25 Aug 2022 17:17
Operator : CG/JU
Sample : N4349-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGN62

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:06:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

