




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011569.D
Acq On : 25 Aug 2022 19:02
Operator : CG/JU
Sample : N4349-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGN94

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:07:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

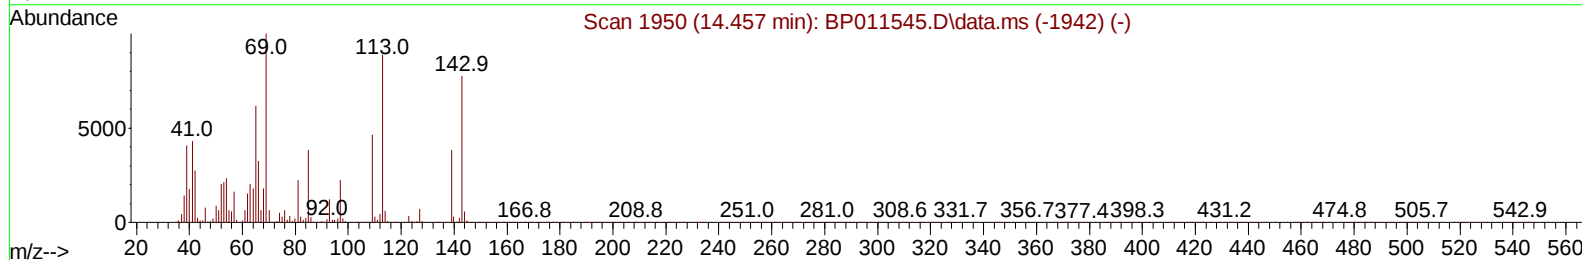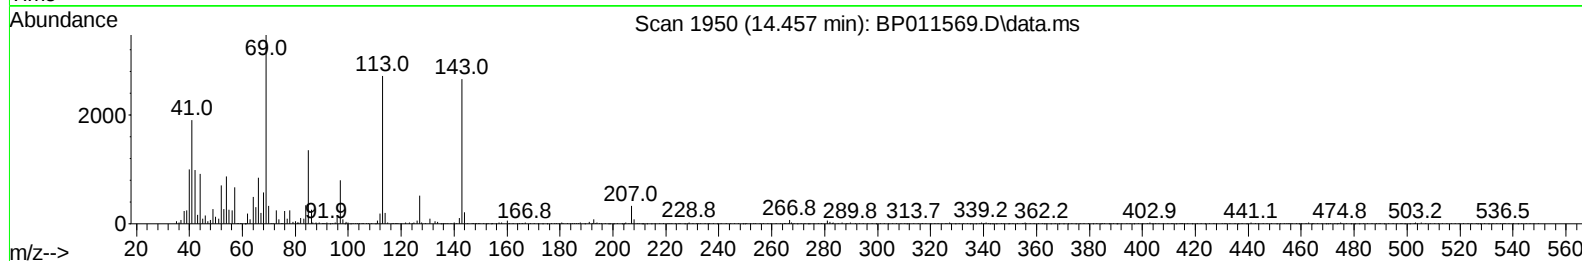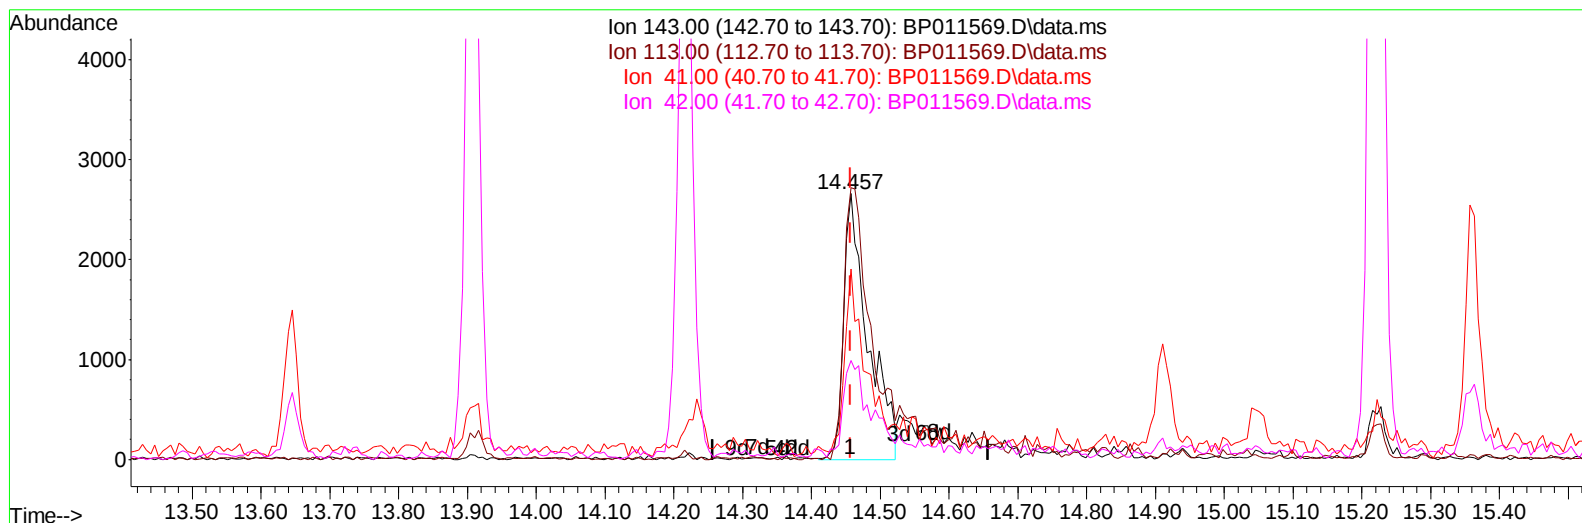

TIC: BP011569.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.457min (-0.000) 3.09 ng/ul m

response 6513

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	109.60	102.14
41.00	52.50	71.74#
42.00	35.70	37.20

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011569.D
 Acq On : 25 Aug 2022 19:02
 Operator : CG/JU
 Sample : N4349-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGN94

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
 Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:07:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	58908	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	251036	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.216	164	154588	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.986	188	304944	20.000	ng/ul	0.00
79) Chrysene-d12	21.116	240	283297	20.000	ng/ul	-0.01
88) Perylene-d12	23.404	264	304268	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.063	96	8814	4.643	ng/uL	0.00
4) Pyridine-d5	3.481	84	40068	8.244	ng/ul	0.00
7) Phenol-d5	6.734	99	34440	6.362	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.893	67	102722	29.207	ng/ul	0.00
11) 2-Chlorophenol-d4	7.081	132	96689	24.284	ng/ul	0.00
15) 4-Methylphenol-d8	8.269	113	65666	15.155	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	59570	32.961	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	53053	28.844	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	93304	27.481	ng/ul	0.00
31) 4-Chloroaniline-d4	10.487	131	127174	22.502	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166	375998	34.389	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	397828	32.737	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	6513m	3.092	ng/ul	0.00
60) Fluorene-d10	15.222	176	313889	34.124	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	26622	16.156	ng/ul	0.00
73) Anthracene-d10	17.092	188	545000	40.354	ng/ul	0.00
81) Pyrene-d10	19.351	212	585925	40.879	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.257	264	569944	38.508	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011569.D
Acq On : 25 Aug 2022 19:02
Operator : CG/JU
Sample : N4349-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGN94

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/26/2022
Supervised By :mohammad ahmed 08/27/2022

Quant Time: Aug 26 01:07:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

