

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011549.D
 Acq On : 24 Aug 2022 20:10
 Operator : CG/JU
 Sample : N4320-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX2

Quant Time: Aug 25 02:18:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	70927	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	295173	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.222	164	170211	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	344056	20.000	ng/ul	0.00
79) Chrysene-d12	21.121	240	332450	20.000	ng/ul	0.00
88) Perylene-d12	23.410	264	343353	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	11371	4.975	ng/uL	0.00
4) Pyridine-d5	3.487	84	34896	5.963	ng/ul	0.01
7) Phenol-d5	6.740	99	44784	6.871	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.899	67	131349	31.018	ng/ul	0.00
11) 2-Chlorophenol-d4	7.081	132	125162	26.109	ng/ul	0.00
15) 4-Methylphenol-d8	8.269	113	81182	15.561	ng/ul	0.00
21) Nitrobenzene-d5	8.716	128	75367	35.466	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	74945	34.653	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	119285	29.880	ng/ul	0.00
31) 4-Chloroaniline-d4	10.493	131	144067	21.679	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166	426327	35.413	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	461342	34.480	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	9706	4.185	ng/ul	0.00
60) Fluorene-d10	15.228	176	355321	35.083	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	56276	30.270	ng/ul	0.00
73) Anthracene-d10	17.092	188	598381	39.269	ng/ul	0.00
81) Pyrene-d10	19.357	212	676360	40.211	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.263	264	664831	39.806	ng/ul	0.00
Target Compounds						
78) Di-n-butylphthalate	17.980	149	105755	4.860	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011549.D
Acq On : 24 Aug 2022 20:10
Operator : CG/JU
Sample : N4320-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX2

Quant Time: Aug 25 02:18:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

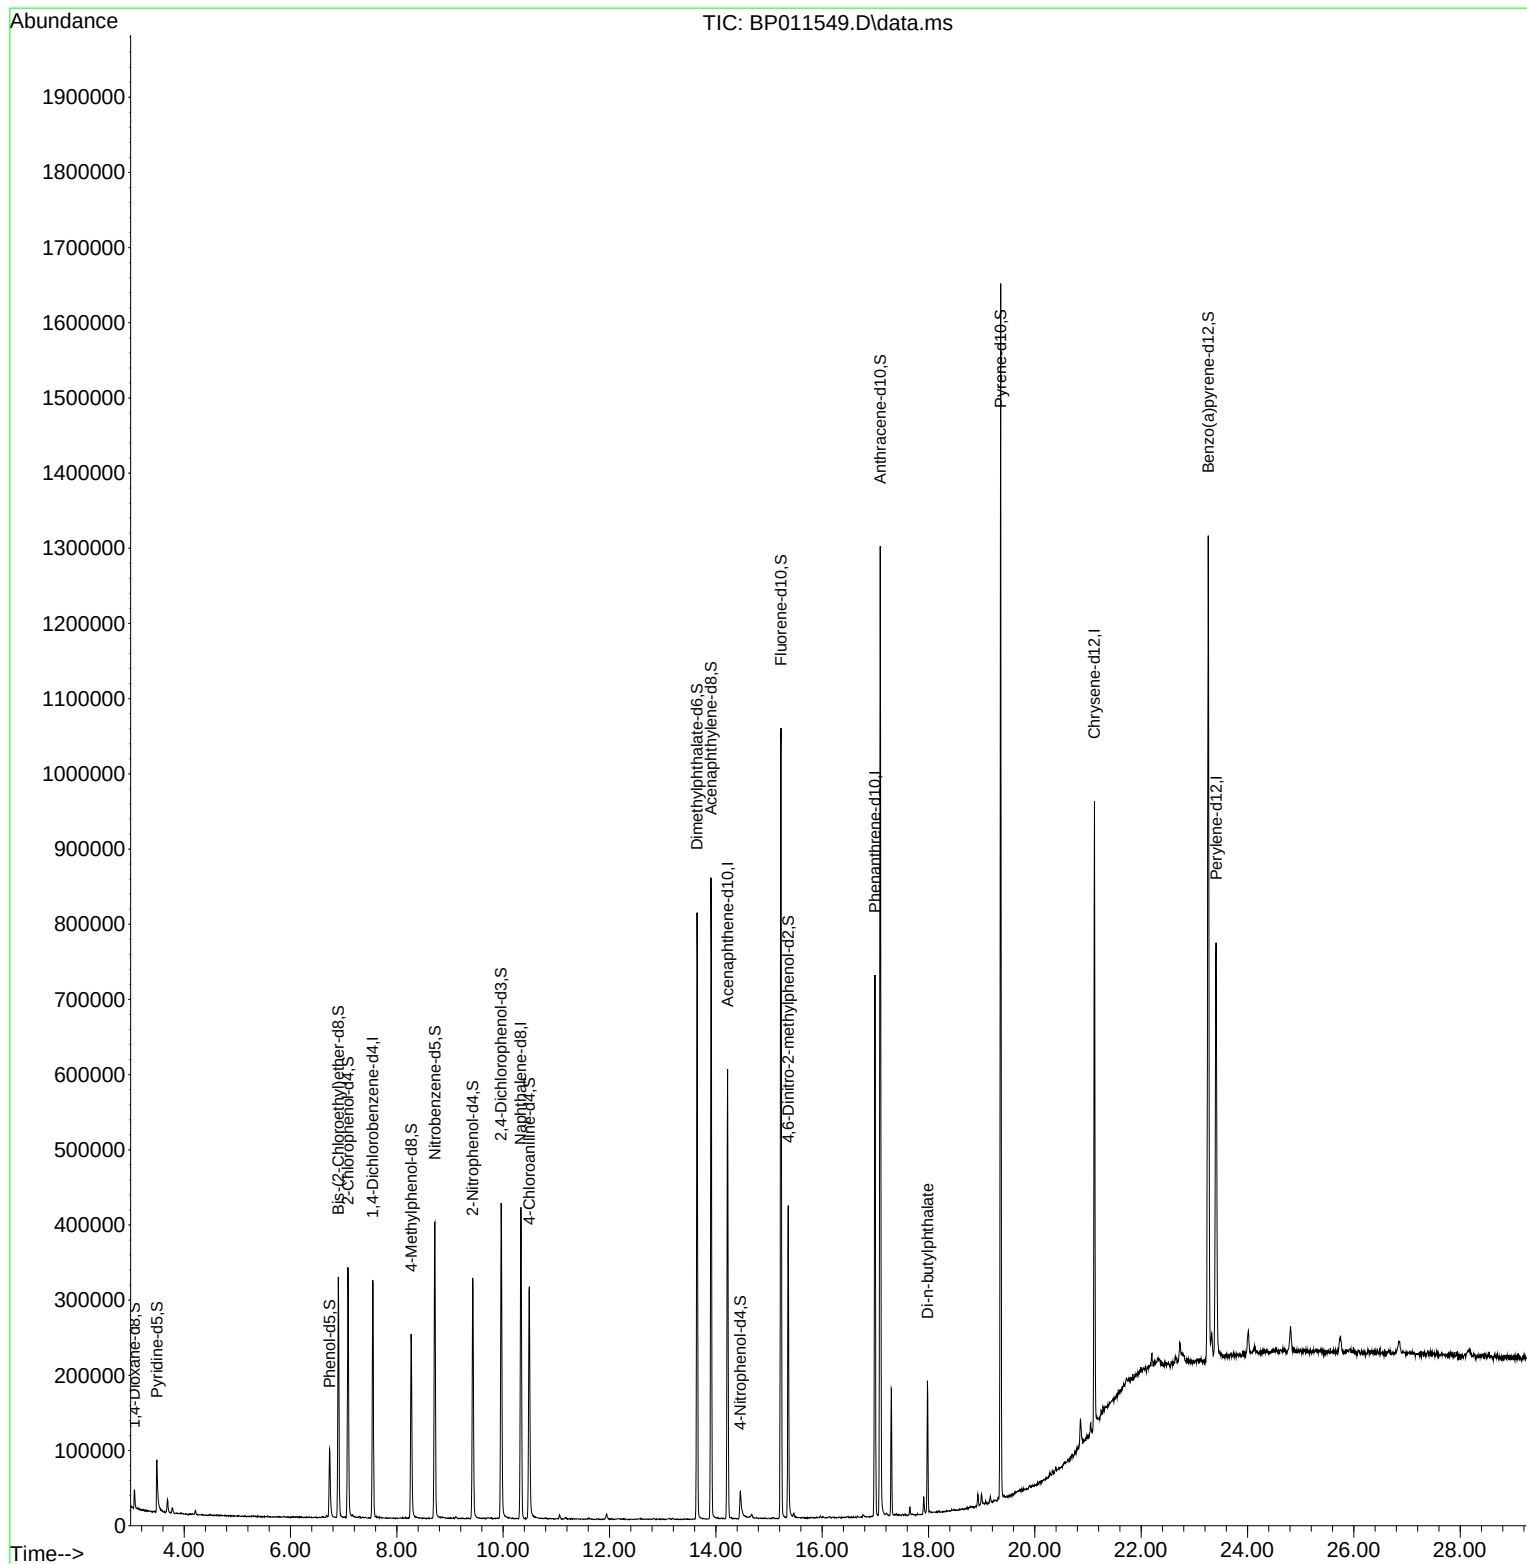

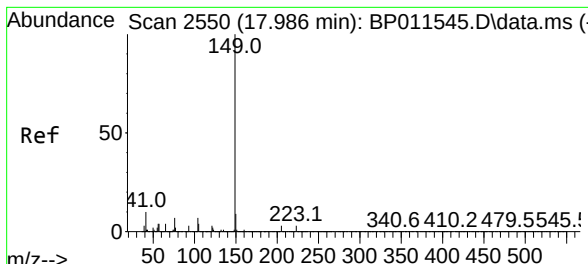

#78
 Di-n-butylphthalate
 Concen: 4.860 ng/ul
 RT: 17.980 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP011549.D
 Acq: 24 Aug 2022 20:10

Instrument :
 BNA_P
 ClientSampleId :
 C0AX2

Tgt Ion:149 Resp: 105755

Ion	Ratio	Lower	Upper
149	100		
150	9.1	7.4	11.2
104	7.1	5.5	8.3

