

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011552.D
 Acq On : 24 Aug 2022 21:55
 Operator : CG/JU
 Sample : N4320-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX7

Quant Time: Aug 25 02:19:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 25 02:14:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	53517	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	224762	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.222	164	133534	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	268798	20.000	ng/ul	0.00
79) Chrysene-d12	21.122	240	254042	20.000	ng/ul	0.00
88) Perylene-d12	23.410	264	271576	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	9251	5.364	ng/uL	0.00
4) Pyridine-d5	3.481	84	45414	10.285	ng/ul	0.00
7) Phenol-d5	6.734	99	37814	7.689	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.899	67	103830	32.496	ng/ul	0.00
11) 2-Chlorophenol-d4	7.081	132	100711	27.843	ng/ul	0.00
15) 4-Methylphenol-d8	8.269	113	66645	16.931	ng/ul	0.00
21) Nitrobenzene-d5	8.716	128	60620	37.463	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	60688	36.852	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	98432	32.381	ng/ul	0.00
31) 4-Chloroaniline-d4	10.493	131	125780	24.857	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166	371887	39.375	ng/ul	0.00
49) Acenaphthylene-d8	13.910	160	389008	37.059	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	8054	4.426	ng/ul	0.00
60) Fluorene-d10	15.228	176	308481	38.824	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	47148	32.461	ng/ul	0.00
73) Anthracene-d10	17.092	188	532568	44.736	ng/ul	0.00
81) Pyrene-d10	19.357	212	582726	45.337	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.263	264	581708	44.034	ng/ul	0.00
Target Compounds						Qvalue
86) Bis(2-ethylhexyl)phtha...	21.051	149	14250	1.292	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011552.D
Acq On : 24 Aug 2022 21:55
Operator : CG/JU
Sample : N4320-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX7

Quant Time: Aug 25 02:19:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 25 02:14:54 2022
Response via : Initial Calibration

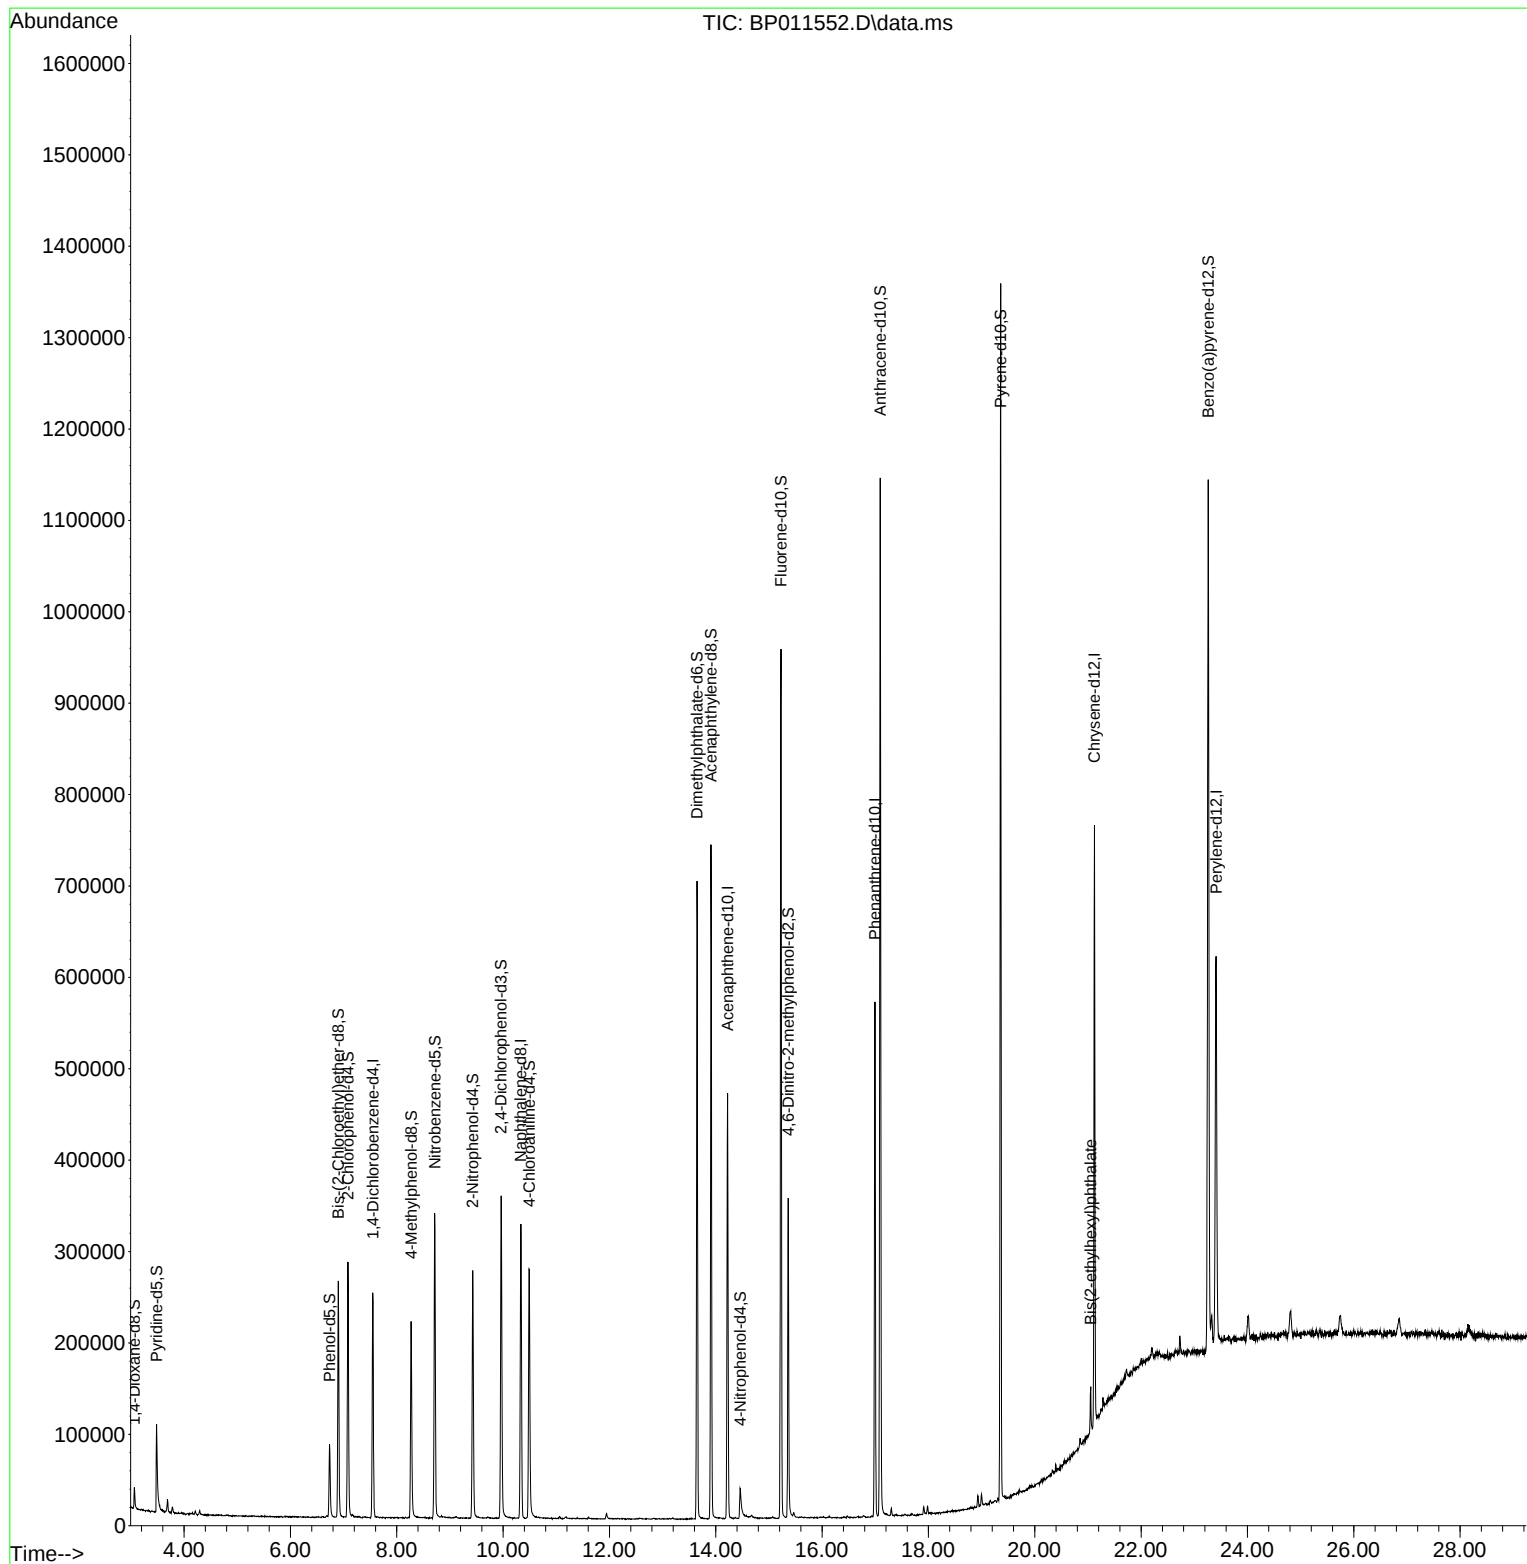

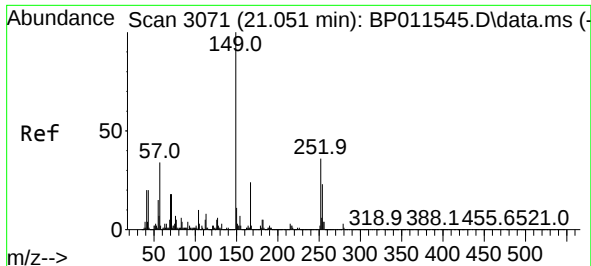

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.292 ng/ul
 RT: 21.051 min Scan# 3071
 Delta R.T. 0.000 min
 Lab File: BP011552.D
 Acq: 24 Aug 2022 21:55

Instrument :
 BNA_P
 ClientSampleId :
 C0AX7

Tgt Ion:	149	Resp:	14250
Ion	Ratio	Lower	Upper
149	100		
167	23.6	19.8	29.8
279	3.6	2.7	4.1

