

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011547.D
 Acq On : 24 Aug 2022 19:00
 Operator : CG/JU
 Sample : N4266-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.546	91	95	96	rBV4	1417	1175	0.16%	0.031%
2	3.664	113	115	116	rBV2	1190	822	0.11%	0.022%
3	3.781	131	135	140	rVB2	6084	7155	0.97%	0.190%
4	4.099	187	189	191	rBV3	1280	1248	0.17%	0.033%
5	4.140	194	196	199	rBV4	1240	1149	0.16%	0.031%
6	4.458	249	250	253	rBV3	1315	1457	0.20%	0.039%
7	4.758	298	301	302	rBV3	1173	1122	0.15%	0.030%
8	5.134	364	365	367	rBV2	983	860	0.12%	0.023%
9	5.275	386	389	390	rVB3	1062	808	0.11%	0.021%
10	5.334	396	399	401	rVB3	1067	1125	0.15%	0.030%
11	5.664	453	455	457	rBV3	1588	1307	0.18%	0.035%
12	5.793	475	477	478	rBV2	1144	807	0.11%	0.021%
13	5.811	478	480	483	rVV4	1279	1012	0.14%	0.027%
14	6.181	541	543	546	rVB4	1227	1278	0.17%	0.034%
15	6.475	591	593	598	rVB5	1095	966	0.13%	0.026%
16	6.546	603	605	608	rBV3	803	1019	0.14%	0.027%
17	6.605	613	615	618	rBV3	862	1104	0.15%	0.029%
18	6.881	660	662	666	rVB4	903	995	0.13%	0.026%
19	7.034	686	688	693	rBV6	760	1415	0.19%	0.038%
20	7.228	719	721	723	rBV3	911	803	0.11%	0.021%
21	7.346	738	741	743	rBV4	871	892	0.12%	0.024%
22	7.487	763	765	767	rVB3	947	901	0.12%	0.024%
23	7.552	767	776	786	rBV	233968	376930	51.09%	10.029%
24	7.634	788	790	792	rVB3	1398	1139	0.15%	0.030%
25	7.922	836	839	842	rBV4	690	987	0.13%	0.026%
26	8.040	857	859	862	rVB4	861	882	0.12%	0.023%
27	8.075	862	865	866	rBV3	1063	1179	0.16%	0.031%
28	8.152	874	878	882	rVB6	861	957	0.13%	0.025%
29	8.299	899	903	905	rBV5	1326	1552	0.21%	0.041%
30	8.405	917	921	924	rBV5	684	1093	0.15%	0.029%
31	8.487	931	935	939	rVB7	942	1319	0.18%	0.035%
32	8.934	1008	1011	1014	rBV5	901	1016	0.14%	0.027%
33	8.981	1018	1019	1025	rVB5	775	1150	0.16%	0.031%
34	9.122	1041	1043	1045	rVB3	937	833	0.11%	0.022%
35	9.599	1120	1124	1127	rVB6	703	824	0.11%	0.022%
36	9.699	1139	1141	1145	rVB5	847	803	0.11%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011547.D
 Acq On : 24 Aug 2022 19:00
 Operator : CG/JU
 Sample : N4266-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	9.781	1152	1155	1156	rVB4	822	795	0.11%	0.021%
38	9.822	1159	1162	1163	rBV3	943	969	0.13%	0.026%
39	9.905	1173	1176	1179	rBV5	681	841	0.11%	0.022%
40	10.152	1215	1218	1219	rBV3	819	982	0.13%	0.026%
41	10.269	1234	1238	1241	rBV5	884	1309	0.18%	0.035%
42	10.340	1241	1250	1260	rBV	290468	498222	67.54%	13.257%
43	11.399	1429	1430	1435	rVB4	930	966	0.13%	0.026%
44	11.446	1435	1438	1440	rBV4	1023	1303	0.18%	0.035%
45	11.534	1452	1453	1457	rBV4	683	892	0.12%	0.024%
46	11.587	1459	1462	1465	rVV5	718	998	0.14%	0.027%
47	11.940	1519	1522	1526	rVB5	730	1151	0.16%	0.031%
48	12.081	1543	1546	1549	rBV4	739	882	0.12%	0.023%
49	12.140	1553	1556	1558	rVB5	914	1050	0.14%	0.028%
50	12.169	1558	1561	1564	rBV5	731	1284	0.17%	0.034%
51	12.293	1579	1582	1586	rBV5	734	1466	0.20%	0.039%
52	12.334	1586	1589	1590	rVB3	970	900	0.12%	0.024%
53	12.499	1616	1617	1620	rBV3	900	1072	0.15%	0.029%
54	12.893	1681	1684	1686	rBV4	827	857	0.12%	0.023%
55	12.999	1700	1702	1705	rVB3	786	799	0.11%	0.021%
56	13.269	1745	1748	1751	rBV5	788	964	0.13%	0.026%
57	13.451	1778	1779	1783	rVB4	908	877	0.12%	0.023%
58	14.140	1894	1896	1900	rBV5	762	1036	0.14%	0.028%
59	14.222	1902	1910	1920	rBV	414185	605326	82.05%	16.106%
60	14.340	1929	1930	1934	rVB4	1246	869	0.12%	0.023%
61	14.381	1935	1937	1939	rVB2	1003	784	0.11%	0.021%
62	14.951	2031	2034	2036	rVB4	931	933	0.13%	0.025%
63	15.098	2057	2059	2061	rBV3	718	791	0.11%	0.021%
64	15.204	2075	2077	2083	rVB7	862	1494	0.20%	0.040%
65	15.269	2087	2088	2091	rVB3	1019	924	0.13%	0.025%
66	15.416	2111	2113	2116	rVB3	990	831	0.11%	0.022%
67	15.640	2149	2151	2154	rVB4	899	870	0.12%	0.023%
68	15.810	2177	2180	2181	rBV3	997	809	0.11%	0.022%
69	15.834	2183	2184	2187	rBV3	814	868	0.12%	0.023%
70	15.987	2207	2210	2212	rVB4	891	987	0.13%	0.026%
71	16.051	2215	2221	2223	rBV7	731	1363	0.18%	0.036%
72	16.251	2251	2255	2258	rBV5	867	1573	0.21%	0.042%
73	16.304	2262	2264	2267	rVB4	725	803	0.11%	0.021%
74	16.351	2270	2272	2273	rBV2	944	786	0.11%	0.021%
75	16.481	2293	2294	2298	rBV4	981	857	0.12%	0.023%
76	16.569	2306	2309	2310	rBV3	992	902	0.12%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011547.D
 Acq On : 24 Aug 2022 19:00
 Operator : CG/JU
 Sample : N4266-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

77	16.728	2334	2336	2339	rVB4	1198	1275	0.17%	0.034%
78	16.781	2342	2345	2347	rBV4	1339	1749	0.24%	0.047%
79	16.939	2369	2372	2374	rBV4	988	1185	0.16%	0.032%
80	16.992	2375	2381	2395	rVV	474971	704638	95.52%	18.749%
81	17.304	2432	2434	2437	rVB4	1094	1089	0.15%	0.029%
82	17.404	2448	2451	2452	rVB3	1122	870	0.12%	0.023%
83	17.439	2452	2457	2459	rBV6	1202	2145	0.29%	0.057%
84	17.481	2461	2464	2465	rBV3	737	782	0.11%	0.021%
85	17.616	2485	2487	2488	rBV2	1166	952	0.13%	0.025%
86	17.792	2516	2517	2520	rBV2	1518	1648	0.22%	0.044%
87	17.822	2520	2522	2527	rVV6	812	1377	0.19%	0.037%
88	17.922	2537	2539	2543	rBV4	1151	1530	0.21%	0.041%
89	17.957	2543	2545	2548	rVB4	1356	1144	0.16%	0.030%
90	17.992	2548	2551	2552	rBV2	1381	1450	0.20%	0.039%
91	18.098	2567	2569	2571	rBV3	1054	809	0.11%	0.022%
92	18.239	2591	2593	2596	rBV4	964	898	0.12%	0.024%
93	18.328	2606	2608	2609	rVB2	1679	896	0.12%	0.024%
94	18.386	2616	2618	2621	rBV4	1218	1394	0.19%	0.037%
95	18.575	2648	2650	2651	rBV2	1215	828	0.11%	0.022%
96	18.622	2656	2658	2660	rBV3	1391	1299	0.18%	0.035%
97	18.822	2690	2692	2693	rBV2	1555	1178	0.16%	0.031%
98	18.886	2701	2703	2706	rVB4	2021	1180	0.16%	0.031%
99	21.122	3079	3083	3092	rBV	590064	737720	100.00%	19.629%
100	23.410	3466	3472	3484	rBV2	396966	728772	98.79%	19.391%




Sum of corrected areas: 3758277

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011547.D
Acq On : 24 Aug 2022 19:00
Operator : CG/JU
Sample : N4266-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

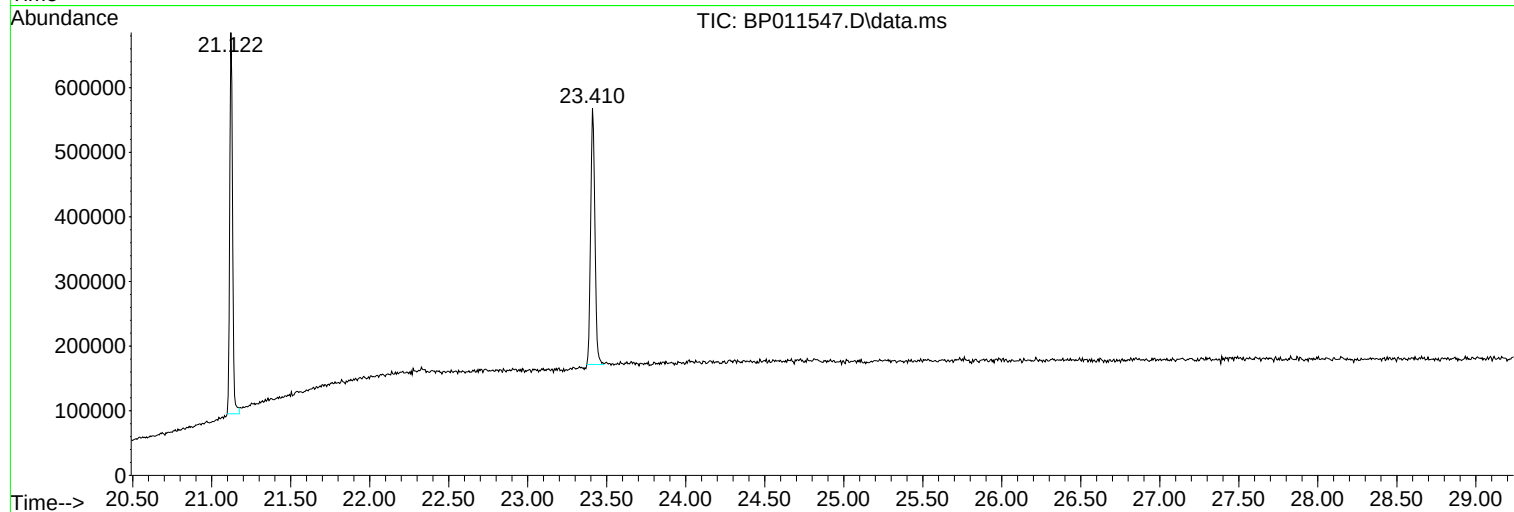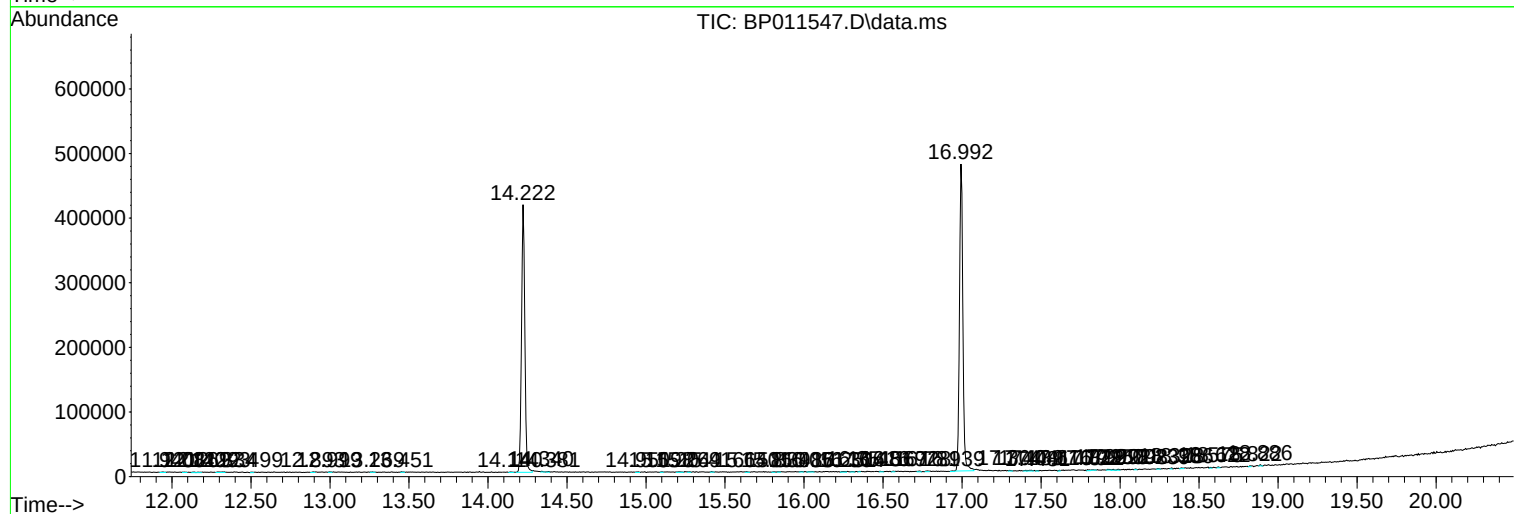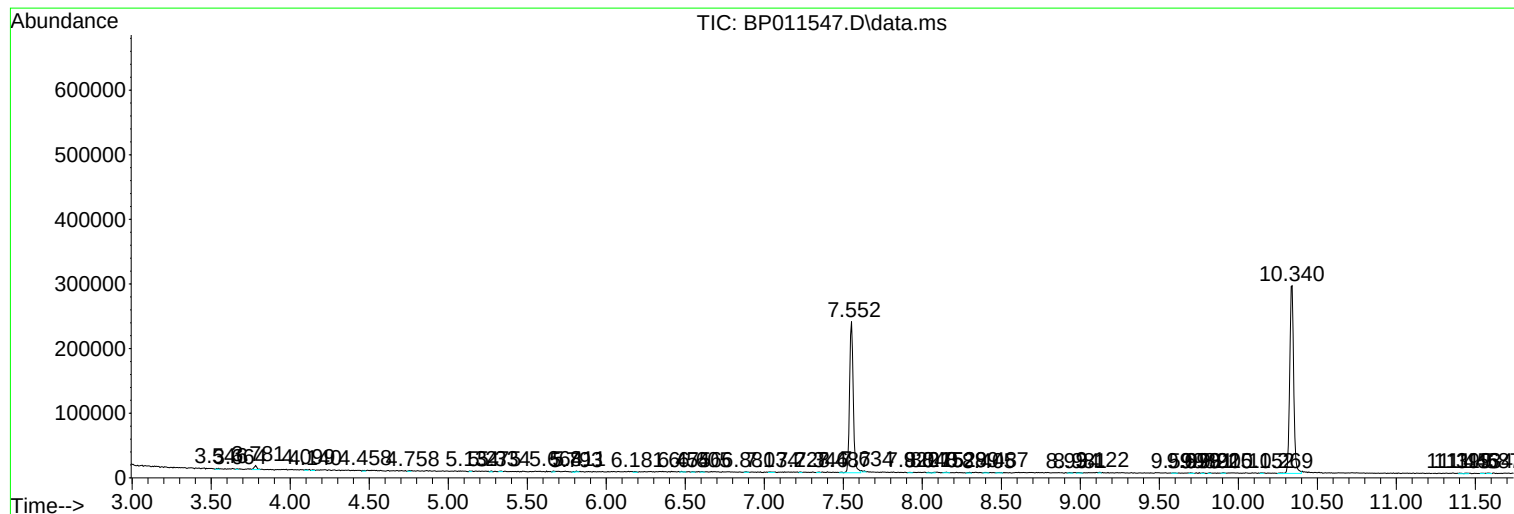

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011547.D
Acq On : 24 Aug 2022 19:00
Operator : CG/JU
Sample : N4266-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011547.D
Acq On : 24 Aug 2022 19:00
Operator : CG/JU
Sample : N4266-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------