

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011549.D
 Acq On : 24 Aug 2022 20:10
 Operator : CG/JU
 Sample : N4320-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	10	13	19	rVB	24321	31203	1.61%	0.157%
2	3.487	82	85	97	rBV	69032	113771	5.85%	0.571%
3	3.687	114	119	126	rVB2	17382	27110	1.39%	0.136%
4	3.781	131	135	141	rVB	7802	12788	0.66%	0.064%
5	4.211	204	208	213	rVB	5656	7357	0.38%	0.037%
6	6.599	609	614	617	rBV7	1834	2783	0.14%	0.014%
7	6.681	624	628	632	rBV6	2860	4876	0.25%	0.024%
8	6.734	632	637	652	rVB	90957	154232	7.94%	0.774%
9	6.899	659	665	678	rBV	319859	477343	24.56%	2.396%
10	7.081	690	696	708	rBV	332675	517895	26.65%	2.599%
11	7.287	729	731	735	rVB5	1834	2669	0.14%	0.013%
12	7.410	749	752	756	rVB5	1273	1989	0.10%	0.010%
13	7.546	768	775	783	rBV	316674	497745	25.61%	2.498%
14	7.987	847	850	854	rBV6	1561	2573	0.13%	0.013%
15	8.269	891	898	912	rBV	245005	405888	20.88%	2.037%
16	8.716	965	974	984	rBV	394111	646407	33.26%	3.244%
17	8.846	993	996	999	rVB5	1362	1945	0.10%	0.010%
18	9.116	1036	1042	1048	rVB9	2492	5495	0.28%	0.028%
19	9.428	1087	1095	1111	rBV	320482	527567	27.14%	2.648%
20	9.710	1138	1143	1145	rBV6	1843	3430	0.18%	0.017%
21	9.963	1179	1186	1198	rBV	419734	689992	35.50%	3.463%
22	10.122	1210	1213	1218	rVB7	1329	2240	0.12%	0.011%
23	10.334	1240	1249	1260	rBV	414621	683974	35.19%	3.433%
24	10.493	1267	1276	1288	rBV	308309	542336	27.90%	2.722%
25	11.057	1369	1372	1378	rVB4	5564	9035	0.46%	0.045%
26	11.169	1386	1391	1395	rBV8	1972	3573	0.18%	0.018%
27	11.945	1516	1523	1531	rBV4	7320	14592	0.75%	0.073%
28	13.187	1729	1734	1737	rBV6	1544	2418	0.12%	0.012%
29	13.645	1805	1812	1823	rBV	806823	1087447	55.95%	5.457%
30	13.910	1850	1857	1870	rBV2	852783	1199164	61.70%	6.018%
31	14.222	1902	1910	1918	rBV	598078	828341	42.62%	4.157%
32	14.463	1944	1951	1967	rBV2	36529	99612	5.13%	0.500%
33	14.675	1983	1987	1993	rVB9	4951	8574	0.44%	0.043%
34	15.228	2073	2081	2091	rBV	1051370	1502175	77.29%	7.539%
35	15.363	2097	2104	2116	rBV	415386	557887	28.70%	2.800%
36	15.463	2118	2121	2127	rVB6	5677	9141	0.47%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011549.D
 Acq On : 24 Aug 2022 20:10
 Operator : CG/JU
 Sample : N4320-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	15.969	2202	2207	2212	rBV9	2526	3821	0.20%	0.019%
38	16.016	2212	2215	2220	rVB7	1797	2313	0.12%	0.012%
39	16.134	2229	2235	2240	rVB10	2123	4209	0.22%	0.021%
40	16.663	2322	2325	2333	rBV10	2142	4039	0.21%	0.020%
41	16.769	2340	2343	2346	rBV5	3728	5682	0.29%	0.029%
42	16.992	2375	2381	2391	rBV	719660	957414	49.26%	4.805%
43	17.092	2391	2398	2413	rBV	1289296	1764817	90.80%	8.857%
44	17.298	2428	2433	2442	rBV	169267	218898	11.26%	1.099%
45	17.510	2466	2469	2473	rVB6	2150	3158	0.16%	0.016%
46	17.557	2473	2477	2479	rBV5	2362	2913	0.15%	0.015%
47	17.651	2490	2493	2497	rBV	10143	11995	0.62%	0.060%
48	17.910	2532	2537	2543	rBV3	23712	31008	1.60%	0.156%
49	17.980	2544	2549	2554	rVV	176399	206727	10.64%	1.037%
50	18.022	2554	2556	2561	rVB6	2605	3875	0.20%	0.019%
51	18.192	2583	2585	2589	rBB5	2023	2575	0.13%	0.013%
52	18.927	2707	2710	2714	rVB	15406	18357	0.94%	0.092%
53	18.998	2719	2722	2727	rVB	13555	18265	0.94%	0.092%
54	19.163	2746	2750	2753	rBV4	9232	12428	0.64%	0.062%
55	19.357	2777	2783	2792	rBV	1616445	1943545	100.00%	9.754%
56	20.857	3035	3038	3046	rBV7	33733	57177	2.94%	0.287%
57	21.121	3078	3083	3089	rBV	834627	1034179	53.21%	5.190%
58	23.263	3440	3447	3454	rBV2	1088905	1925507	99.07%	9.663%
59	23.410	3466	3472	3480	rVB	544516	1007281	51.83%	5.055%




Sum of corrected areas: 19925750

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011549.D
Acq On : 24 Aug 2022 20:10
Operator : CG/JU
Sample : N4320-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

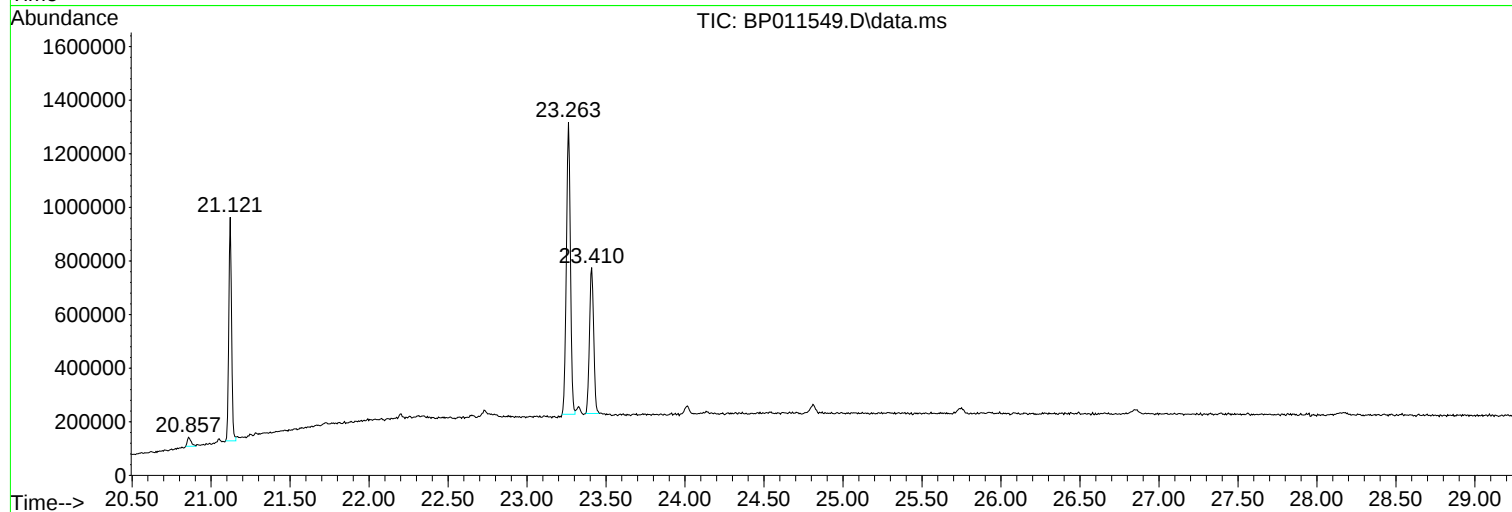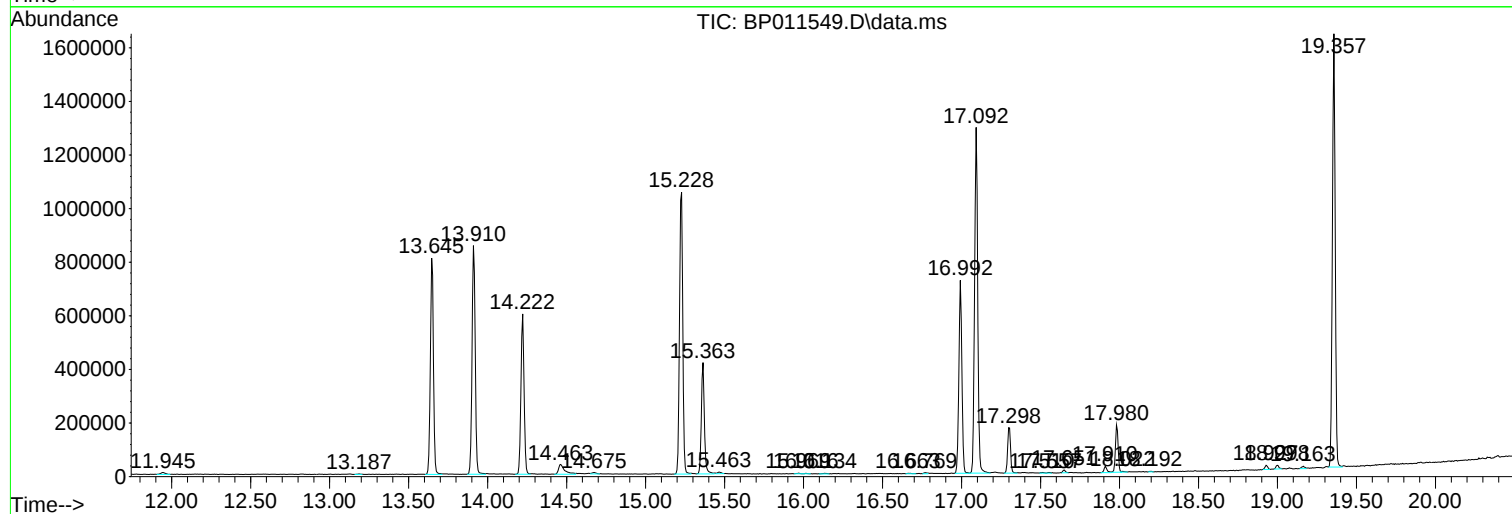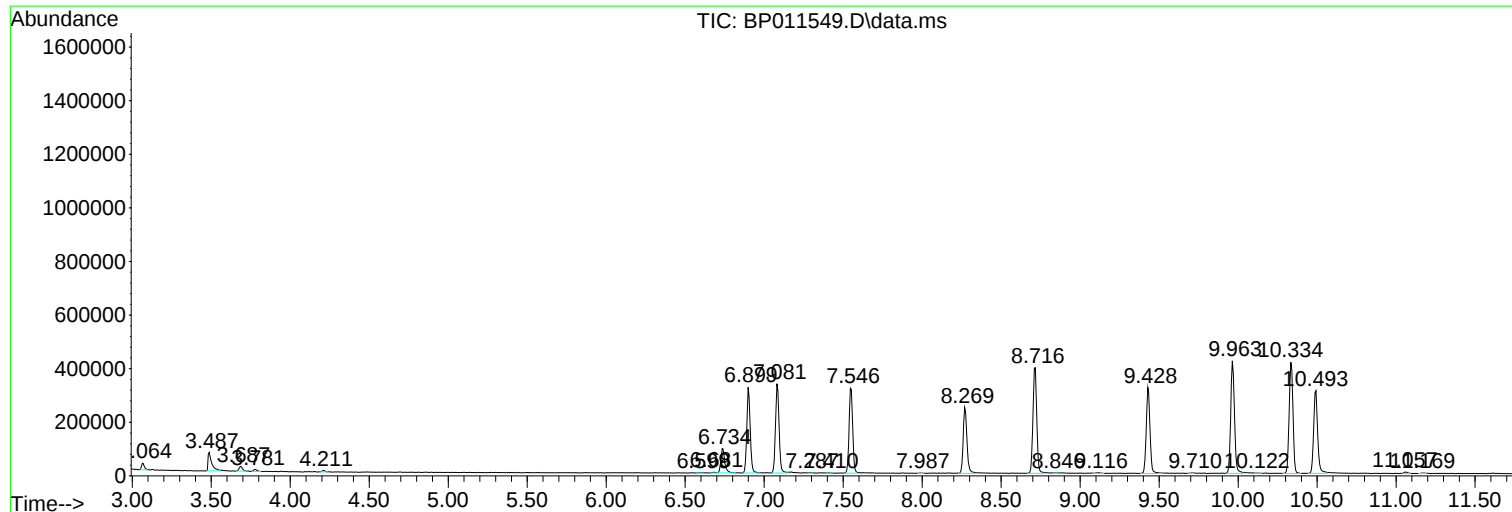

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011549.D
Acq On : 24 Aug 2022 20:10
Operator : CG/JU
Sample : N4320-01
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0AX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1,2-Benzenedicarboxylic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.298	4.57 ng/ul	218898	Phenanthrene-d10	16.992	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,2-Benzenedicarboxylic acid, bi...	278	C16H22O4	000084-69-5	90
2	1,2-Benzenedicarboxylic acid, bi...	278	C16H22O4	000084-69-5	86
3	Phthalic acid, hept-4-yl isobuty...	320	C19H28O4	1000356-78-3	78
4	Phthalic acid, hex-2-yn-4-yl iso...	330	C20H26O4	1000315-20-0	78
5	1,2-Benzenedicarboxylic acid, di...	250	C14H18O4	000131-16-8	78

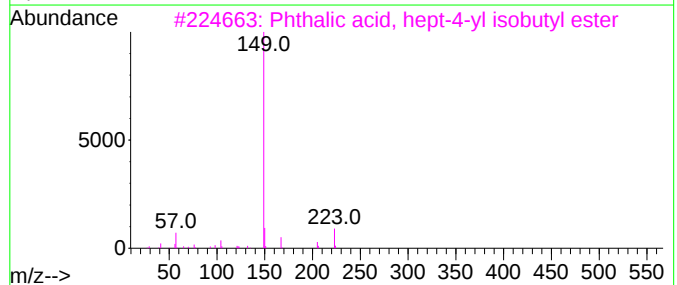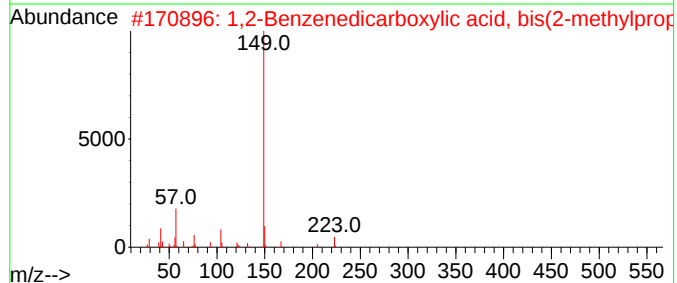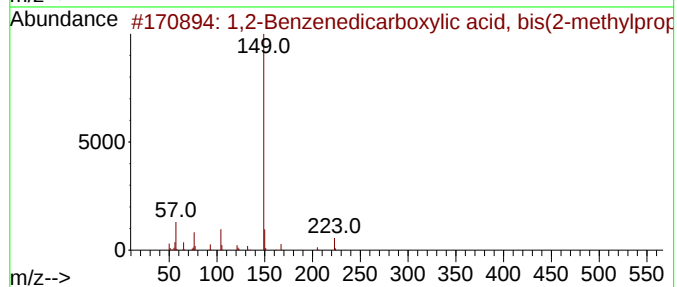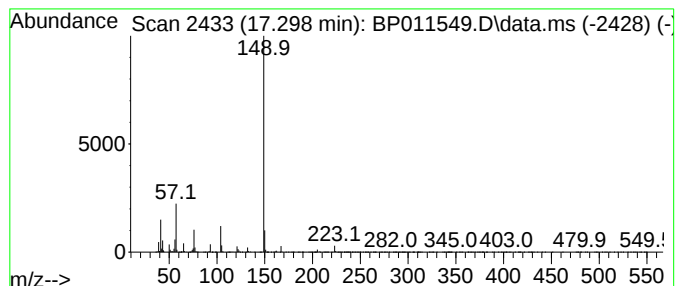

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011549.D
Acq On : 24 Aug 2022 20:10
Operator : CG/JU
Sample : N4320-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,2-Benzenedica...	17.298	4.6	ng/ul	218898	4	16.992	957414	20.0