

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011550.D
 Acq On : 24 Aug 2022 20:45
 Operator : CG/JU
 Sample : N4320-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	10	13	20	rVB	23022	29236	1.74%	0.180%
2	3.152	26	28	33	rVB5	3729	4647	0.28%	0.029%
3	3.481	81	84	97	rBV	95413	147706	8.79%	0.910%
4	3.687	114	119	124	rVB2	13919	22327	1.33%	0.138%
5	3.781	131	135	142	rVB	6755	10304	0.61%	0.064%
6	4.146	195	197	201	rVB4	1809	2239	0.13%	0.014%
7	4.210	206	208	211	rVV2	4623	5270	0.31%	0.032%
8	4.240	211	213	219	rVB6	2929	4474	0.27%	0.028%
9	6.681	626	628	631	rBV3	1690	2002	0.12%	0.012%
10	6.734	631	637	652	rVB	94652	157011	9.35%	0.968%
11	6.899	659	665	678	rBV	233135	354247	21.09%	2.183%
12	7.081	690	696	705	rBV	276737	414878	24.70%	2.557%
13	7.169	709	711	716	rVB6	2002	2653	0.16%	0.016%
14	7.375	743	746	749	rBV5	2013	2162	0.13%	0.013%
15	7.546	768	775	782	rBV	261756	406236	24.18%	2.504%
16	8.269	891	898	910	rBV	226251	369131	21.98%	2.275%
17	8.710	966	973	984	rBV	300608	494898	29.46%	3.050%
18	8.845	991	996	999	rBV7	2014	3016	0.18%	0.019%
19	9.275	1063	1069	1070	rVB6	1251	2026	0.12%	0.012%
20	9.428	1088	1095	1104	rBV	224961	370063	22.03%	2.281%
21	9.963	1179	1186	1203	rBV	329983	546953	32.56%	3.371%
22	10.334	1241	1249	1257	rBV	348212	565192	33.65%	3.483%
23	10.492	1268	1276	1295	rBV	261597	475575	28.31%	2.931%
24	11.198	1393	1396	1401	rVB7	1307	2046	0.12%	0.013%
25	11.622	1464	1468	1475	rVB9	1941	3527	0.21%	0.022%
26	11.945	1517	1523	1529	rBV6	4748	10098	0.60%	0.062%
27	12.086	1543	1547	1552	rVB8	1278	1687	0.10%	0.010%
28	12.416	1598	1603	1605	rBV5	1134	1826	0.11%	0.011%
29	12.822	1666	1672	1675	rBV7	1551	2412	0.14%	0.015%
30	13.186	1732	1734	1738	rVB4	1508	1749	0.10%	0.011%
31	13.645	1806	1812	1825	rBV	672646	919525	54.74%	5.667%
32	13.910	1849	1857	1869	rBV	677947	949822	56.55%	5.854%
33	14.222	1903	1910	1919	rBV	490168	701935	41.79%	4.326%
34	14.457	1945	1950	1963	rBV3	40023	95186	5.67%	0.587%
35	14.551	1964	1966	1972	rVB6	2139	3618	0.22%	0.022%
36	14.675	1986	1987	1992	rVB5	2820	3084	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011550.D
 Acq On : 24 Aug 2022 20:45
 Operator : CG/JU
 Sample : N4320-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	14.757	1998	2001	2005	rVB6	1361	1935	0.12%	0.012%
38	15.227	2073	2081	2089	rBV	894107	1256268	74.79%	7.742%
39	15.363	2097	2104	2114	rBV	276065	374811	22.31%	2.310%
40	15.469	2119	2122	2126	rVB4	4532	6218	0.37%	0.038%
41	15.616	2143	2147	2150	rBV6	1022	1729	0.10%	0.011%
42	15.792	2174	2177	2181	rBV6	1706	1732	0.10%	0.011%
43	15.975	2202	2208	2212	rBV8	1588	3140	0.19%	0.019%
44	16.133	2230	2235	2241	rVV10	1484	3223	0.19%	0.020%
45	16.474	2289	2293	2295	rBV5	1752	2449	0.15%	0.015%
46	16.657	2320	2324	2325	rBV3	1355	1758	0.10%	0.011%
47	16.939	2369	2372	2375	rBV5	1198	1910	0.11%	0.012%
48	16.992	2375	2381	2391	rVV	609315	818799	48.75%	5.046%
49	17.092	2391	2398	2414	rVV	1129286	1569715	93.45%	9.674%
50	17.551	2474	2476	2480	rVB5	1465	1742	0.10%	0.011%
51	17.686	2498	2499	2502	rVB3	2092	1803	0.11%	0.011%
52	17.910	2533	2537	2542	rBV7	6590	10556	0.63%	0.065%
53	17.986	2547	2550	2553	rVB3	3002	3649	0.22%	0.022%
54	18.733	2675	2677	2679	rBV2	2326	2049	0.12%	0.013%
55	18.927	2706	2710	2714	rBV5	13931	19602	1.17%	0.121%
56	18.998	2718	2722	2728	rVV	14041	20069	1.19%	0.124%
57	19.357	2777	2783	2792	rBV	1344787	1679746	100.00%	10.352%
58	21.121	3078	3083	3092	rBV	719205	875584	52.13%	5.396%
59	23.262	3440	3447	3454	rBV2	893229	1638365	97.54%	10.097%
60	23.409	3466	3472	3482	rVB	442240	840308	50.03%	5.179%




Sum of corrected areas: 16225921

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011550.D
Acq On : 24 Aug 2022 20:45
Operator : CG/JU
Sample : N4320-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

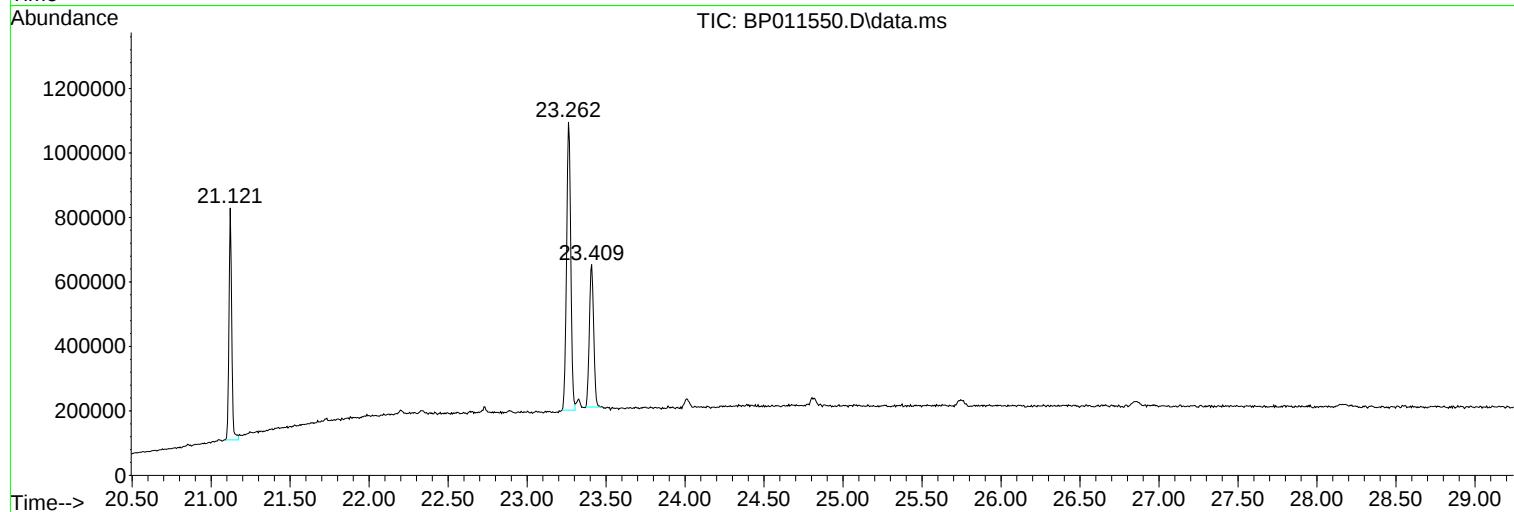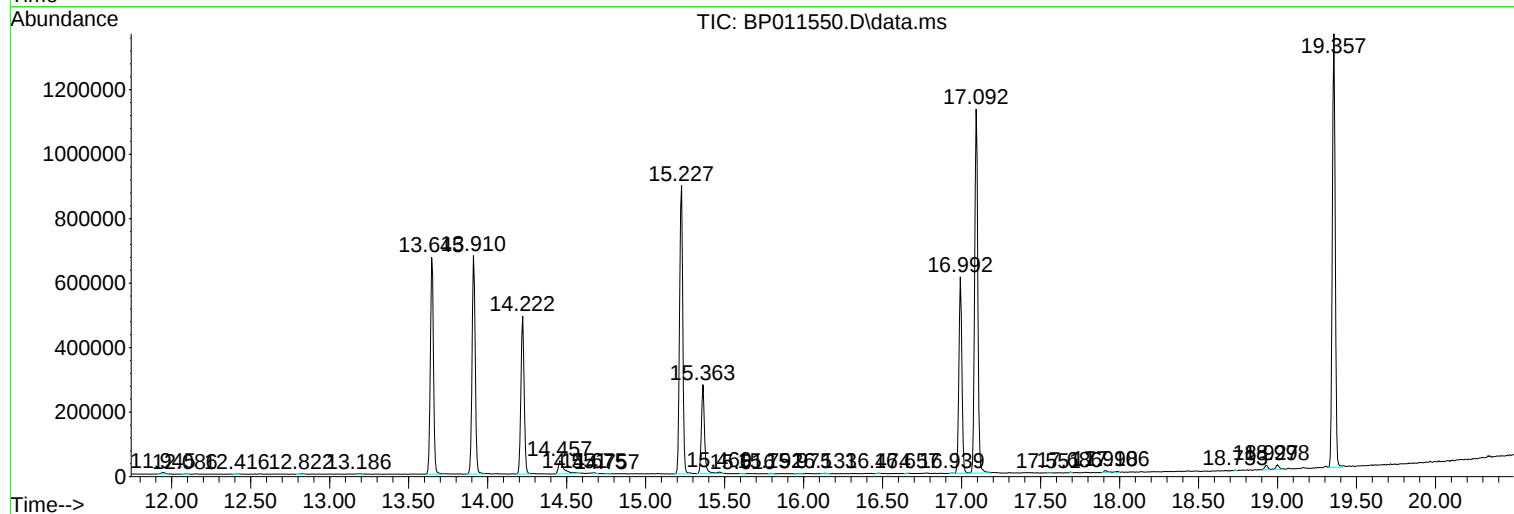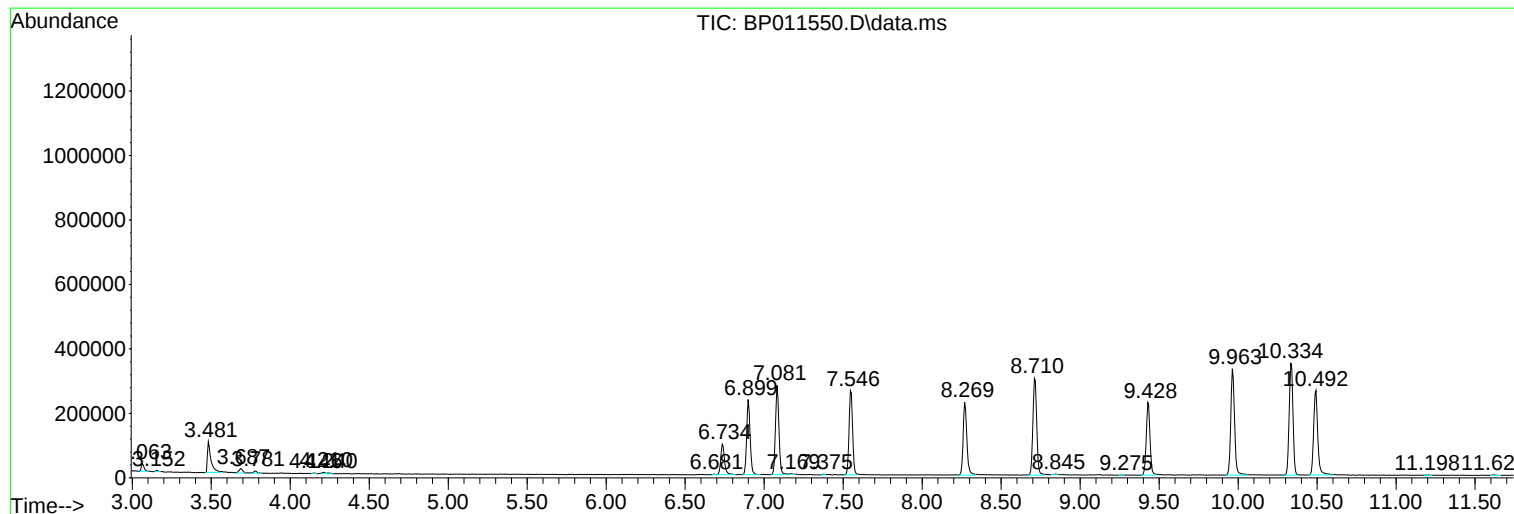

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011550.D
Acq On : 24 Aug 2022 20:45
Operator : CG/JU
Sample : N4320-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011550.D
Acq On : 24 Aug 2022 20:45
Operator : CG/JU
Sample : N4320-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc