

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011551.D
 Acq On : 24 Aug 2022 21:20
 Operator : CG/JU
 Sample : N4320-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	10	13	18	rVB	19684	24511	1.42%	0.151%
2	3.487	82	85	95	rBV	55090	87564	5.09%	0.541%
3	3.687	114	119	124	rVB2	15060	23394	1.36%	0.144%
4	3.775	129	134	138	rBV4	5948	8146	0.47%	0.050%
5	4.146	195	197	202	rBV6	1735	2860	0.17%	0.018%
6	4.211	204	208	213	rVB2	4051	5775	0.34%	0.036%
7	4.687	286	289	293	rBV6	1281	1974	0.11%	0.012%
8	4.799	301	308	310	rBV8	1464	3021	0.18%	0.019%
9	5.652	450	453	455	rBV4	1375	1860	0.11%	0.011%
10	6.681	625	628	631	rVB5	1996	2496	0.14%	0.015%
11	6.734	631	637	648	rBV	66473	114467	6.65%	0.707%
12	6.899	659	665	674	rBV	247010	367548	21.35%	2.270%
13	7.081	689	696	708	rBV	262116	401973	23.35%	2.482%
14	7.375	742	746	751	rBV5	2514	4573	0.27%	0.028%
15	7.546	769	775	784	rBV	239705	375701	21.82%	2.320%
16	8.269	891	898	914	rBV	177963	304008	17.66%	1.877%
17	8.710	966	973	984	rBV	317509	519307	30.17%	3.207%
18	8.846	993	996	1000	rVB6	2232	2201	0.13%	0.014%
19	9.116	1037	1042	1045	rBV5	2216	3628	0.21%	0.022%
20	9.428	1088	1095	1105	rBV	254052	413094	24.00%	2.551%
21	9.698	1135	1141	1147	rBV9	2598	7011	0.41%	0.043%
22	9.963	1179	1186	1197	rBV	323458	544787	31.65%	3.364%
23	10.334	1241	1249	1257	rBV	321906	520266	30.22%	3.213%
24	10.487	1266	1275	1292	rBV	249259	451863	26.25%	2.790%
25	11.063	1369	1373	1379	rVB7	1894	3358	0.20%	0.021%
26	11.616	1462	1467	1472	rVB6	1411	2756	0.16%	0.017%
27	11.940	1517	1522	1530	rBV2	5349	10568	0.61%	0.065%
28	12.163	1551	1560	1563	rBV10	1032	3199	0.19%	0.020%
29	13.187	1731	1734	1738	rVB6	1306	1890	0.11%	0.012%
30	13.645	1805	1812	1824	rBV	689972	919225	53.40%	5.676%
31	13.910	1851	1857	1871	rBV	697945	1003832	58.31%	6.199%
32	14.222	1903	1910	1919	rBV	457267	653886	37.98%	4.038%
33	14.463	1946	1951	1962	rBV	25937	63707	3.70%	0.393%
34	14.669	1983	1986	1991	rVB6	3185	4684	0.27%	0.029%
35	15.092	2055	2058	2061	rVB5	1589	1873	0.11%	0.012%
36	15.228	2074	2081	2090	rBV	875931	1251993	72.72%	7.731%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011551.D
 Acq On : 24 Aug 2022 21:20
 Operator : CG/JU
 Sample : N4320-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	15.363	2098	2104	2113	rBV	353453	478996	27.82%	2.958%
38	15.469	2119	2122	2126	rVB5	4182	5572	0.32%	0.034%
39	15.963	2202	2206	2210	rBV7	1606	2856	0.17%	0.018%
40	16.022	2213	2216	2223	rVB9	1574	2448	0.14%	0.015%
41	16.775	2339	2344	2348	rBV8	1915	3711	0.22%	0.023%
42	16.992	2375	2381	2390	rVV	563795	769349	44.69%	4.751%
43	17.092	2391	2398	2413	rVV	1169798	1601496	93.03%	9.889%
44	17.210	2416	2418	2421	rVB3	2220	2367	0.14%	0.015%
45	17.304	2428	2434	2438	rVB2	6425	9970	0.58%	0.062%
46	17.692	2498	2500	2505	rVB6	2246	2125	0.12%	0.013%
47	17.910	2534	2537	2544	rBV4	15909	22071	1.28%	0.136%
48	17.980	2545	2549	2555	rVB	57499	72648	4.22%	0.449%
49	18.933	2706	2711	2716	rBV5	12975	20939	1.22%	0.129%
50	18.998	2719	2722	2726	rVV	12483	14982	0.87%	0.093%
51	19.157	2747	2749	2752	rBV4	4241	4471	0.26%	0.028%
52	19.357	2777	2783	2791	rBV	1372405	1721550	100.00%	10.631%
53	20.857	3035	3038	3046	rBV7	22238	45148	2.62%	0.279%
54	21.121	3078	3083	3091	rBV	676164	827474	48.07%	5.110%
55	23.262	3441	3447	3454	rBV2	941169	1652228	95.97%	10.203%
56	23.410	3466	3472	3481	rVB2	433817	820614	47.67%	5.067%




Sum of corrected areas: 16194014

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011551.D
Acq On : 24 Aug 2022 21:20
Operator : CG/JU
Sample : N4320-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

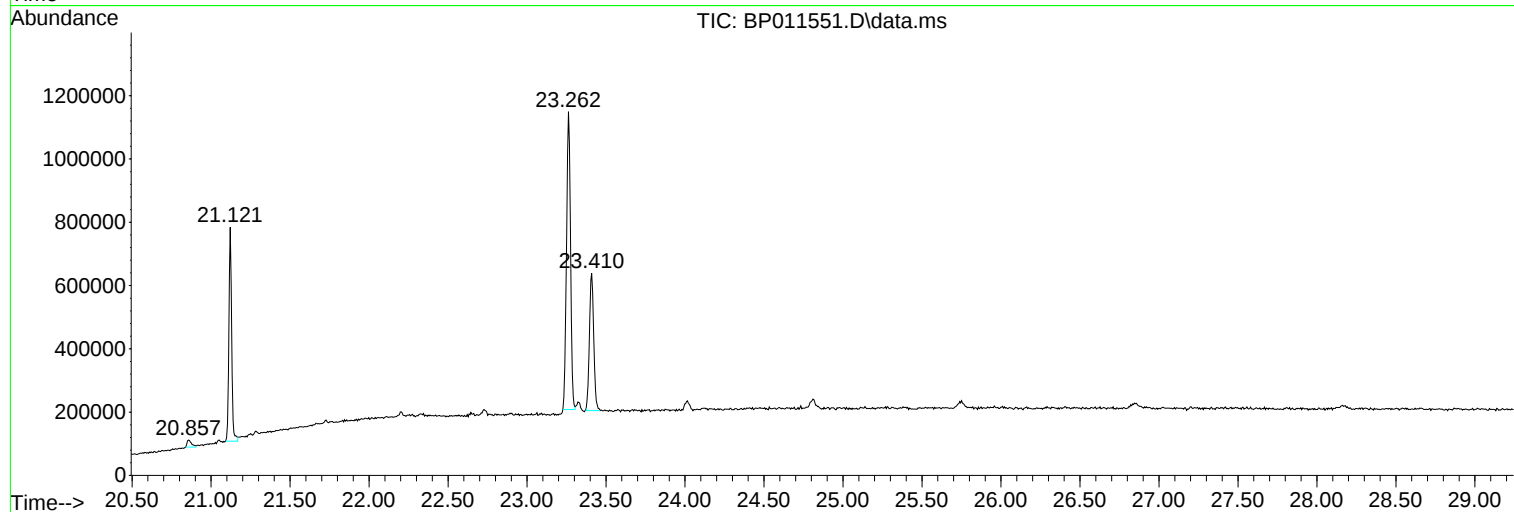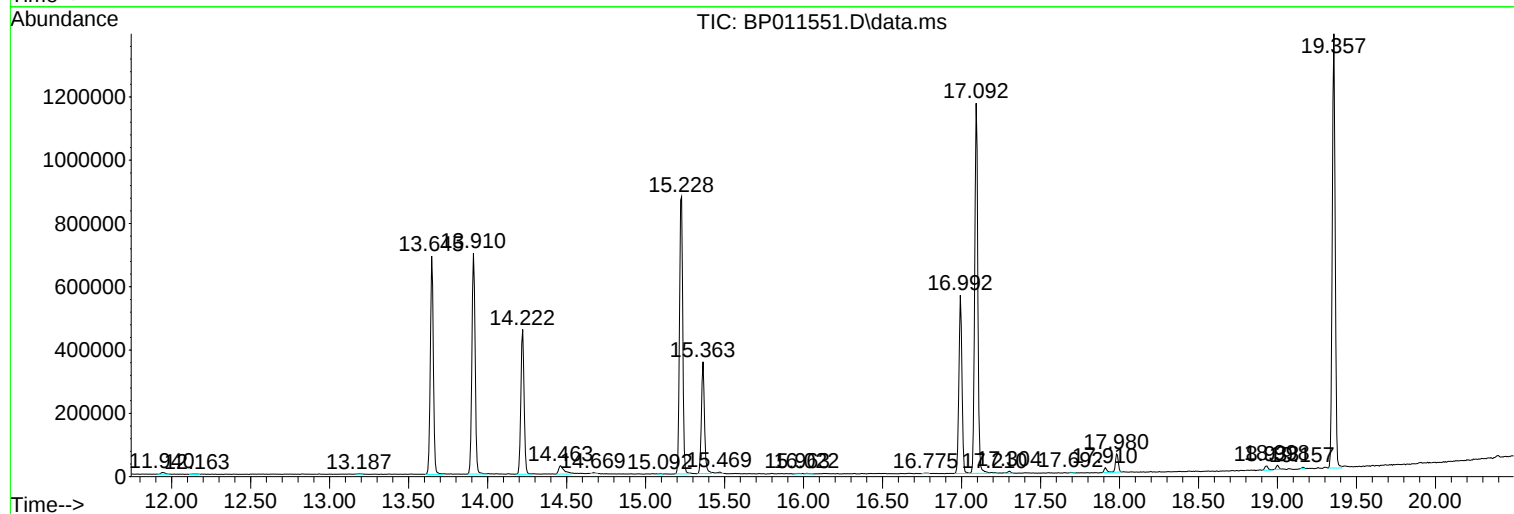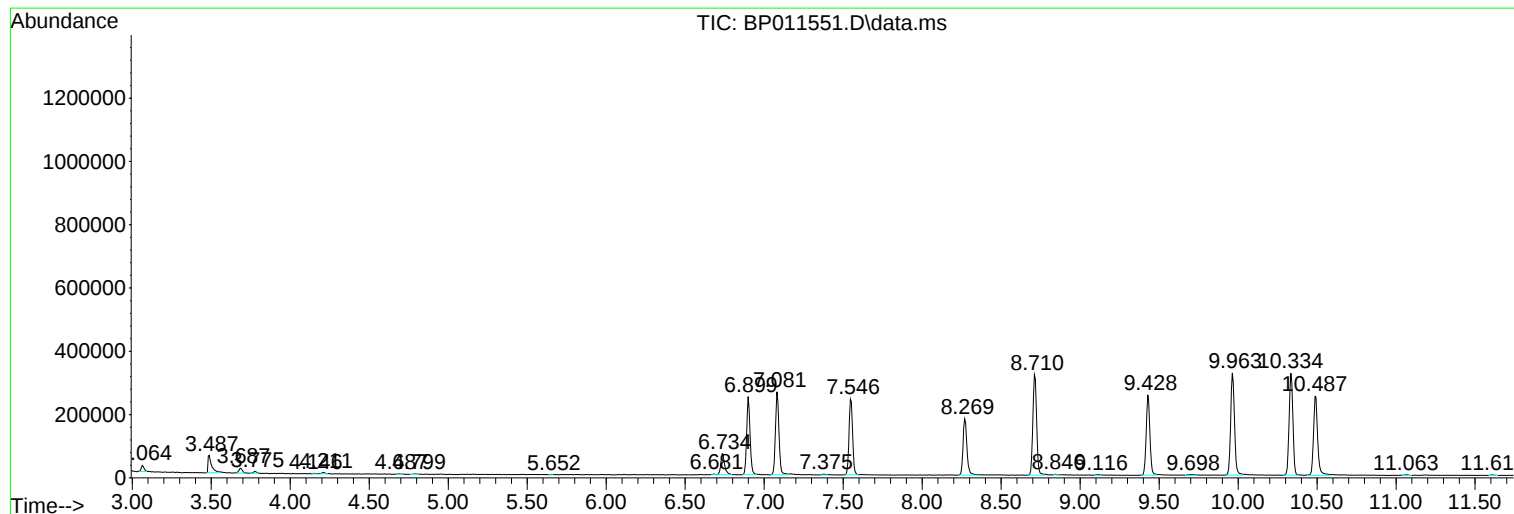

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011551.D
Acq On : 24 Aug 2022 21:20
Operator : CG/JU
Sample : N4320-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011551.D
Acq On : 24 Aug 2022 21:20
Operator : CG/JU
Sample : N4320-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc