

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011552.D
 Acq On : 24 Aug 2022 21:55
 Operator : CG/JU
 Sample : N4320-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	10	13	22	rVB	23789	31849	1.86%	0.192%
2	3.481	81	84	97	rBV	95631	152089	8.87%	0.916%
3	3.687	114	119	126	rVB	14547	21806	1.27%	0.131%
4	3.781	131	135	141	rVB2	6827	10996	0.64%	0.066%
5	4.211	204	208	215	rVB3	5063	8547	0.50%	0.051%
6	4.293	215	222	225	rBV5	5261	8782	0.51%	0.053%
7	6.593	610	613	617	rBV6	1609	2117	0.12%	0.013%
8	6.681	624	628	632	rBV4	2064	3784	0.22%	0.023%
9	6.734	632	637	649	rVB	79653	128651	7.50%	0.774%
10	6.899	659	665	677	rBV	258127	381909	22.28%	2.299%
11	7.081	689	696	707	rBV	279162	429402	25.05%	2.585%
12	7.158	707	709	714	rVB5	2295	3788	0.22%	0.023%
13	7.546	768	775	787	rBV	246567	393410	22.95%	2.368%
14	8.163	876	880	883	rBV5	1452	2047	0.12%	0.012%
15	8.269	892	898	911	rBV	214919	344504	20.09%	2.074%
16	8.710	966	973	990	rBV	334190	545010	31.79%	3.281%
17	8.840	991	995	998	rVB6	1784	2145	0.13%	0.013%
18	9.116	1040	1042	1049	rVB8	1817	2808	0.16%	0.017%
19	9.428	1088	1095	1108	rBV	270967	431898	25.19%	2.600%
20	9.705	1140	1142	1151	rVB9	1281	2756	0.16%	0.017%
21	9.963	1179	1186	1203	rBV	352784	592096	34.54%	3.564%
22	10.334	1241	1249	1260	rBV	321985	527550	30.77%	3.176%
23	10.487	1262	1275	1298	rBV	273147	499952	29.16%	3.010%
24	11.063	1370	1373	1376	rBV5	2377	3277	0.19%	0.020%
25	11.175	1386	1392	1393	rBV6	1798	2641	0.15%	0.016%
26	11.610	1462	1466	1469	rBV6	1646	1881	0.11%	0.011%
27	11.946	1517	1523	1529	rBV7	5985	11149	0.65%	0.067%
28	12.834	1669	1674	1678	rBV7	1091	1999	0.12%	0.012%
29	13.193	1729	1735	1738	rBV7	1492	1956	0.11%	0.012%
30	13.645	1806	1812	1825	rBV	698094	957196	55.83%	5.762%
31	13.910	1850	1857	1869	rBV	737404	1024853	59.78%	6.169%
32	14.222	1902	1910	1918	rBV	465273	657841	38.37%	3.960%
33	14.457	1944	1950	1963	rBV3	33010	81743	4.77%	0.492%
34	14.675	1983	1987	1992	rVB8	2237	3553	0.21%	0.021%
35	15.228	2074	2081	2094	rBV	950622	1322669	77.15%	7.962%
36	15.363	2098	2104	2118	rVV	349559	474724	27.69%	2.858%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011552.D
 Acq On : 24 Aug 2022 21:55
 Operator : CG/JU
 Sample : N4320-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	15.463	2118	2121	2129	rVB7	5171	9496	0.55%	0.057%
38	16.022	2214	2216	2223	rVB8	1568	2461	0.14%	0.015%
39	16.475	2290	2293	2297	rBV6	2079	2756	0.16%	0.017%
40	16.775	2340	2344	2348	rBV6	1797	3311	0.19%	0.020%
41	16.934	2368	2371	2374	rBV4	1487	2209	0.13%	0.013%
42	16.992	2374	2381	2390	rBV	563407	761612	44.42%	4.585%
43	17.092	2391	2398	2410	rBV	1135734	1573864	91.80%	9.474%
44	17.304	2429	2434	2438	rVB	8483	11184	0.65%	0.067%
45	17.551	2473	2476	2480	rBV5	1443	2361	0.14%	0.014%
46	17.686	2498	2499	2506	rVB6	2376	2719	0.16%	0.016%
47	17.910	2533	2537	2541	rBV6	8566	12075	0.70%	0.073%
48	17.981	2545	2549	2553	rVV	8483	10975	0.64%	0.066%
49	18.251	2591	2595	2596	rBV4	1588	2174	0.13%	0.013%
50	18.928	2706	2710	2714	rBV5	12922	18085	1.05%	0.109%
51	18.998	2718	2722	2726	rBV2	12861	17768	1.04%	0.107%
52	19.163	2747	2750	2755	rBV7	4444	7482	0.44%	0.045%
53	19.357	2777	2783	2792	rBV	1331714	1701832	99.26%	10.244%
54	21.051	3067	3071	3076	rBV	50382	60960	3.56%	0.367%
55	21.122	3078	3083	3089	rBV	657576	807330	47.09%	4.860%
56	23.263	3440	3447	3454	rBV2	948911	1714459	100.00%	10.320%
57	23.410	3466	3472	3482	rVB2	418524	813957	47.48%	4.900%




Sum of corrected areas: 16612448

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011552.D
Acq On : 24 Aug 2022 21:55
Operator : CG/JU
Sample : N4320-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

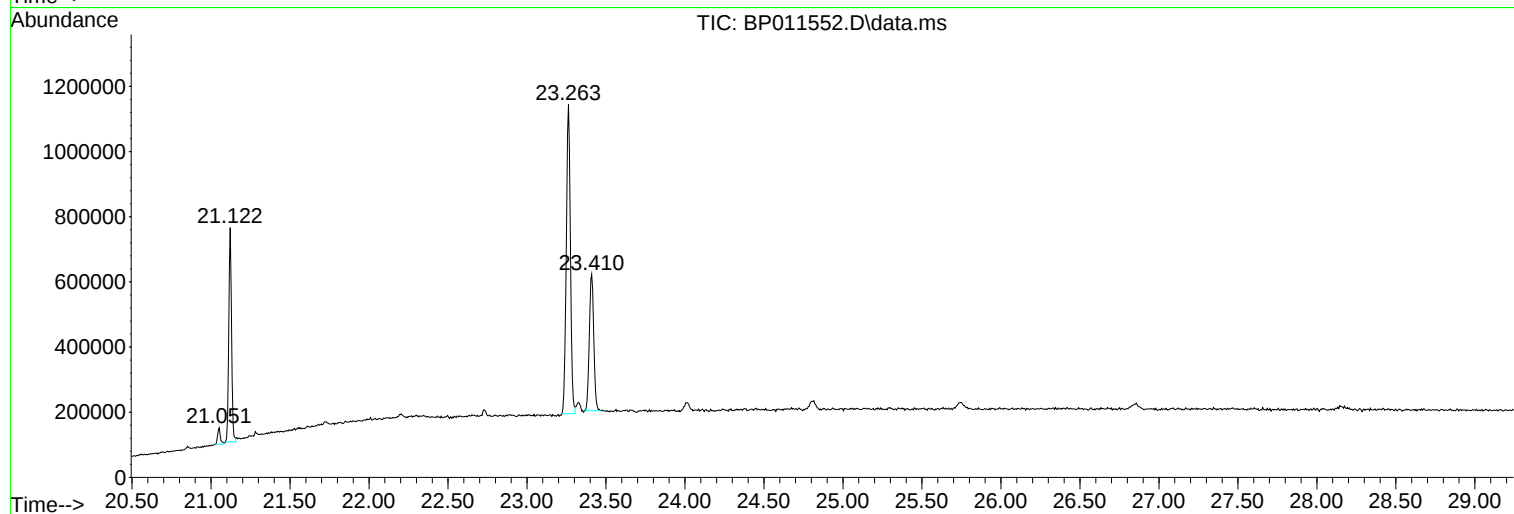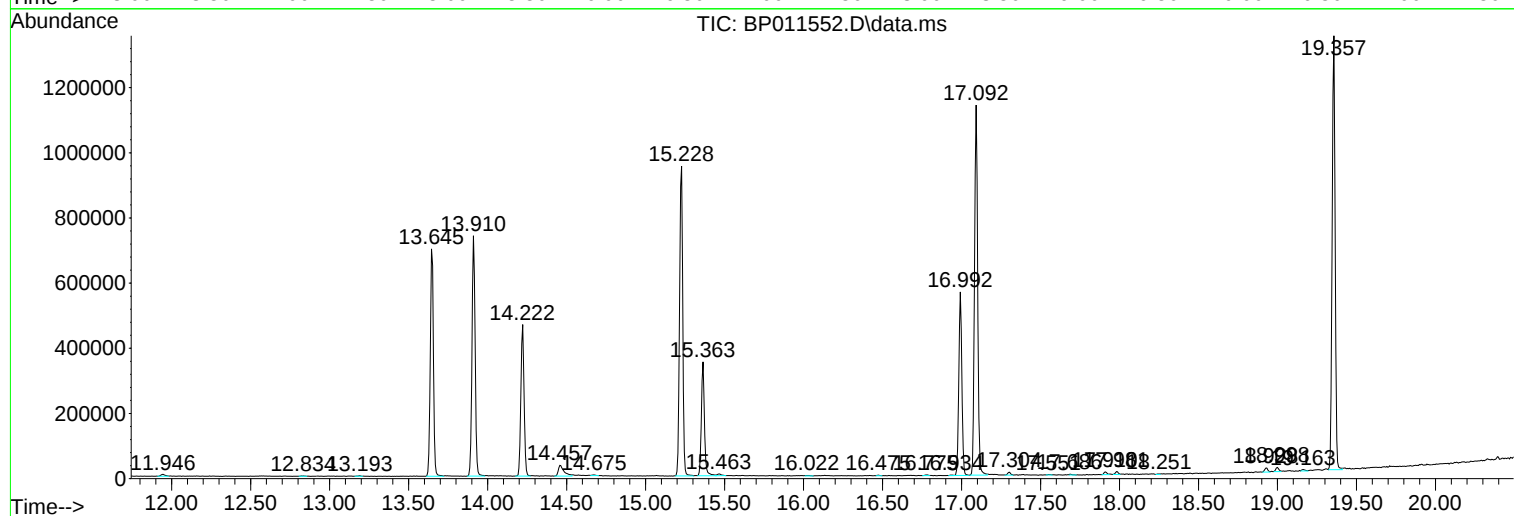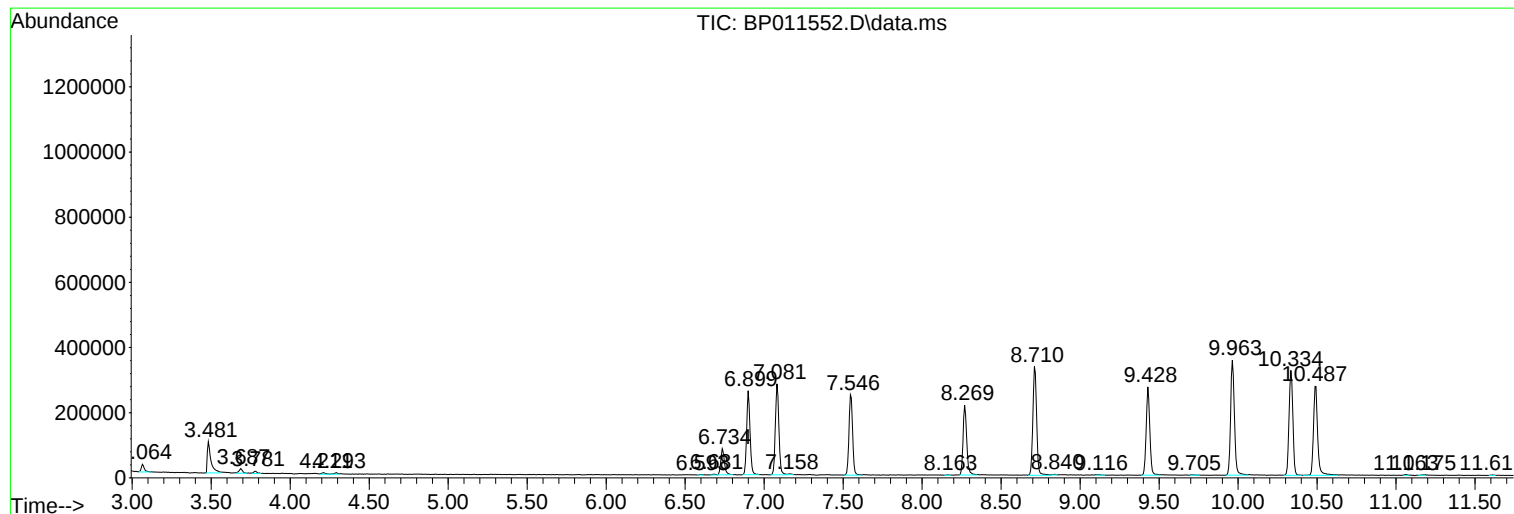

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011552.D
Acq On : 24 Aug 2022 21:55
Operator : CG/JU
Sample : N4320-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011552.D
Acq On : 24 Aug 2022 21:55
Operator : CG/JU
Sample : N4320-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc