

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011560.D
 Acq On : 25 Aug 2022 11:53
 Operator : CG/JU
 Sample : N4320-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	18	rBV	21496	25245	1.29%	0.130%
2	3.487	82	85	98	rBV	52428	92491	4.72%	0.478%
3	3.687	114	119	126	rVB	17348	27372	1.40%	0.141%
4	3.775	130	134	138	rVB	6630	8469	0.43%	0.044%
5	4.205	204	207	214	rVB3	5606	8556	0.44%	0.044%
6	6.681	623	628	631	rBV5	2549	3771	0.19%	0.019%
7	6.734	631	637	650	rVV	87469	150128	7.66%	0.776%
8	6.899	658	665	677	rBV	318848	484863	24.73%	2.506%
9	7.081	689	696	709	rBV	341939	521456	26.59%	2.695%
10	7.375	740	746	753	rBV4	4034	7382	0.38%	0.038%
11	7.546	768	775	785	rBV	284906	439982	22.44%	2.274%
12	7.622	786	788	794	rVB6	3765	5287	0.27%	0.027%
13	8.269	891	898	913	rBV	248660	403551	20.58%	2.085%
14	8.710	966	973	985	rBV	424599	674233	34.38%	3.484%
15	8.881	1000	1002	1008	rVB6	2957	4257	0.22%	0.022%
16	9.110	1038	1041	1045	rVB6	2385	3411	0.17%	0.018%
17	9.199	1052	1056	1060	rVB7	1048	2172	0.11%	0.011%
18	9.428	1086	1095	1107	rBV	344487	547581	27.92%	2.830%
19	9.699	1136	1141	1145	rBV8	2660	5887	0.30%	0.030%
20	9.963	1179	1186	1202	rBV	445712	733975	37.43%	3.793%
21	10.334	1241	1249	1260	rVB	388635	621376	31.69%	3.211%
22	10.487	1267	1275	1291	rBV	276007	490206	25.00%	2.533%
23	11.169	1387	1391	1393	rBV5	2137	2813	0.14%	0.015%
24	11.610	1463	1466	1470	rVB5	2276	3425	0.17%	0.018%
25	11.946	1517	1523	1528	rBV4	7810	14082	0.72%	0.073%
26	12.828	1668	1673	1679	rVB9	2150	3531	0.18%	0.018%
27	12.934	1685	1691	1695	rBV8	1151	2016	0.10%	0.010%
28	13.187	1731	1734	1740	rVB8	1935	3926	0.20%	0.020%
29	13.645	1805	1812	1819	rBV	902243	1202108	61.30%	6.212%
30	13.910	1848	1857	1866	rBV	957091	1337981	68.23%	6.914%
31	14.222	1902	1910	1919	rBV	541053	774050	39.47%	4.000%
32	14.292	1919	1922	1925	rVB4	1915	2294	0.12%	0.012%
33	14.457	1945	1950	1964	rBV3	32715	84050	4.29%	0.434%
34	14.669	1983	1986	1992	rVB5	5775	9335	0.48%	0.048%
35	15.222	2073	2080	2089	rBV	1163324	1650191	84.15%	8.528%
36	15.363	2097	2104	2116	rBV	433819	588761	30.02%	3.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011560.D
 Acq On : 25 Aug 2022 11:53
 Operator : CG/JU
 Sample : N4320-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	15.469	2118	2122	2126	rVB4	5454	8191	0.42%	0.042%
38	15.792	2176	2177	2183	rVB6	1711	2380	0.12%	0.012%
39	15.969	2204	2207	2209	rBV4	1662	2455	0.13%	0.013%
40	16.016	2213	2215	2221	rVB6	1775	2282	0.12%	0.012%
41	16.475	2289	2293	2297	rBV6	2153	3795	0.19%	0.020%
42	16.663	2322	2325	2329	rBV6	2035	2860	0.15%	0.015%
43	16.992	2375	2381	2392	rVV	649368	885322	45.15%	4.575%
44	17.092	2392	2398	2410	rVV2	1343251	1851883	94.44%	9.570%
45	17.686	2497	2499	2503	rVB5	3182	3448	0.18%	0.018%
46	17.910	2532	2537	2542	rBV6	8758	14929	0.76%	0.077%
47	17.986	2546	2550	2553	rVB2	4220	5170	0.26%	0.027%
48	18.928	2707	2710	2715	rVB3	15180	19633	1.00%	0.101%
49	18.998	2719	2722	2727	rVV	12229	16989	0.87%	0.088%
50	19.357	2777	2783	2790	rBV	1522617	1960922	100.00%	10.134%
51	21.122	3078	3083	3093	rBV	728396	921127	46.97%	4.760%
52	23.263	3441	3447	3455	rBV2	997386	1832019	93.43%	9.467%
53	23.410	3467	3472	3484	rVB2	469718	877051	44.73%	4.532%




Sum of corrected areas: 19350670

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011560.D
Acq On : 25 Aug 2022 11:53
Operator : CG/JU
Sample : N4320-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

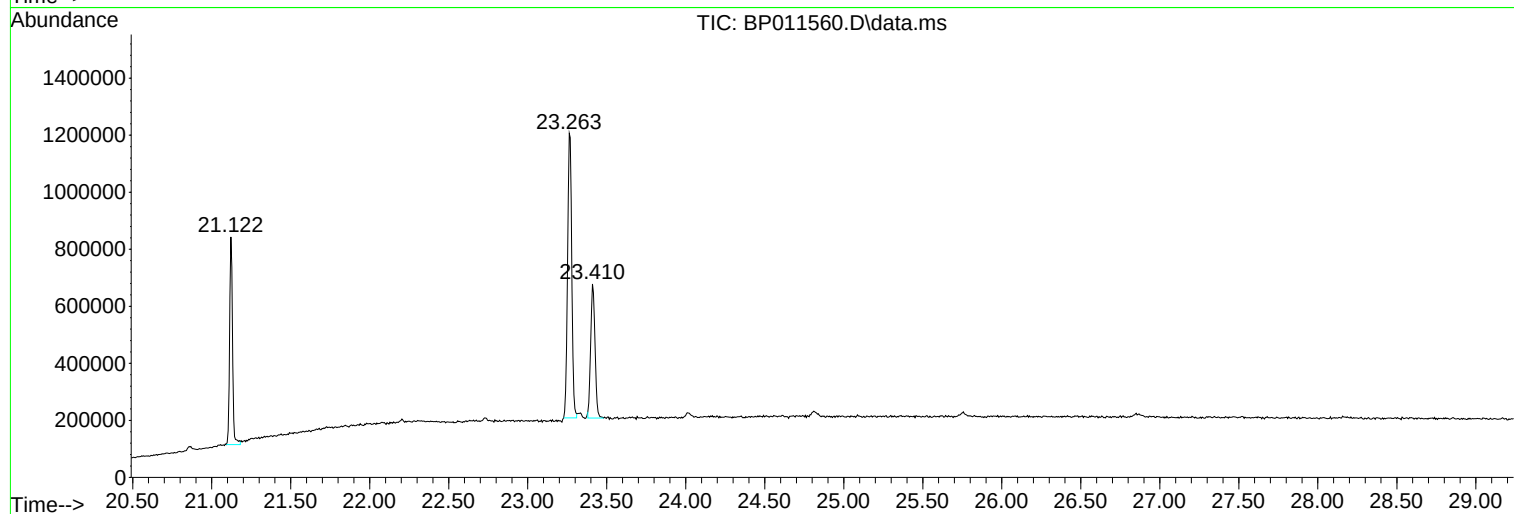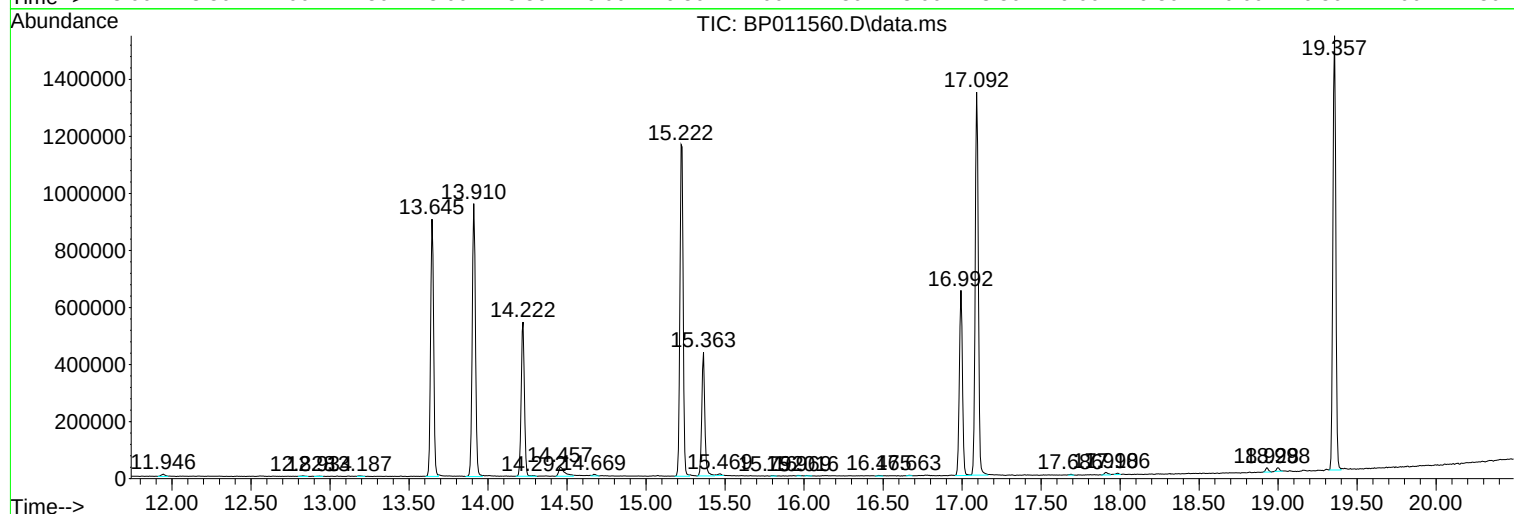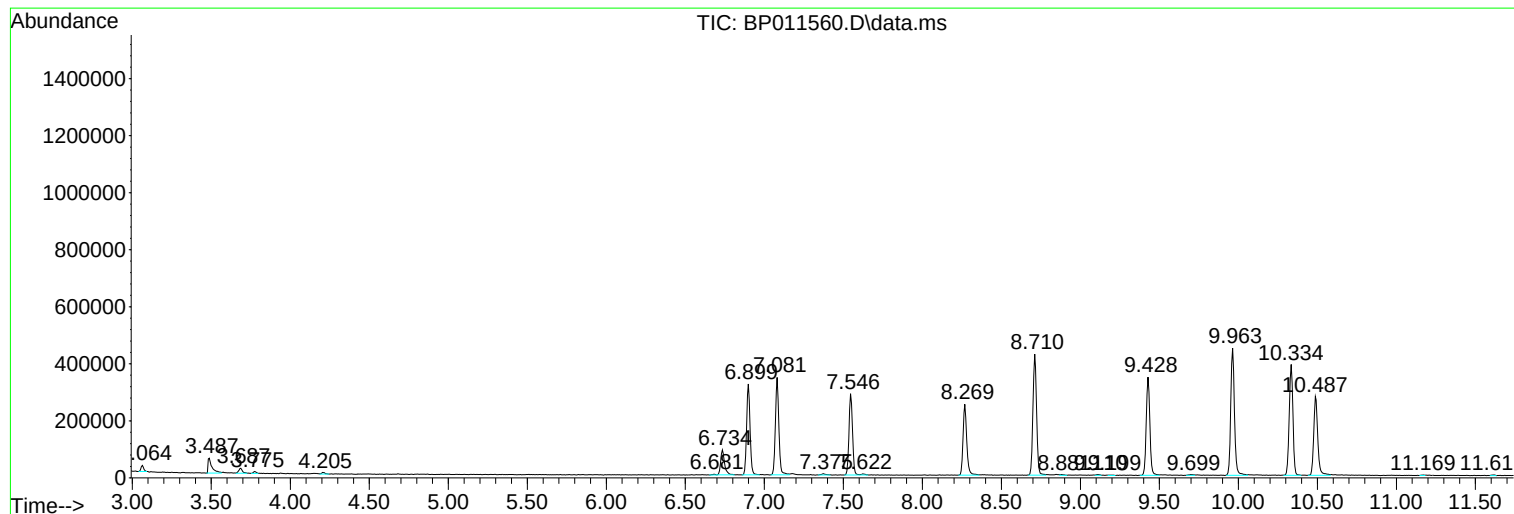

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011560.D
Acq On : 25 Aug 2022 11:53
Operator : CG/JU
Sample : N4320-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011560.D
Acq On : 25 Aug 2022 11:53
Operator : CG/JU
Sample : N4320-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc