

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011561.D
 Acq On : 25 Aug 2022 12:28
 Operator : CG/JU
 Sample : N4320-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	10	13	19	rVB	24342	27578	1.40%	0.141%
2	3.481	82	84	100	rBV	112776	177970	9.01%	0.908%
3	3.687	114	119	123	rBV2	13171	21550	1.09%	0.110%
4	3.781	131	135	140	rVB5	6954	9959	0.50%	0.051%
5	4.211	205	208	212	rVB2	4829	5924	0.30%	0.030%
6	4.287	216	221	232	rVB	142675	199149	10.08%	1.017%
7	6.111	527	531	535	rBV6	1622	2658	0.13%	0.014%
8	6.675	624	627	632	rBV7	2353	4652	0.24%	0.024%
9	6.734	632	637	650	rVB	86892	139947	7.09%	0.714%
10	6.899	659	665	674	rBV	286539	435342	22.05%	2.222%
11	7.081	686	696	709	rBV	313970	493695	25.00%	2.520%
12	7.175	709	712	718	rVB7	5147	9695	0.49%	0.049%
13	7.375	741	746	750	rVB3	3891	6822	0.35%	0.035%
14	7.546	768	775	785	rBV	290644	450145	22.80%	2.298%
15	7.622	785	788	793	rVB5	3492	4758	0.24%	0.024%
16	8.269	889	898	913	rBV	245357	391165	19.81%	1.997%
17	8.710	966	973	981	rBV	381981	617838	31.29%	3.154%
18	8.846	992	996	1002	rBV8	3722	5555	0.28%	0.028%
19	9.116	1037	1042	1050	rVB7	2609	5583	0.28%	0.028%
20	9.428	1088	1095	1105	rBV	314791	507707	25.71%	2.592%
21	9.699	1136	1141	1143	rBV6	2073	3163	0.16%	0.016%
22	9.963	1179	1186	1202	rBV	410603	678271	34.35%	3.462%
23	10.334	1242	1249	1265	rVB	385296	625725	31.69%	3.194%
24	10.487	1267	1275	1290	rBV	328617	582769	29.51%	2.975%
25	11.187	1392	1394	1402	rVB9	1782	3108	0.16%	0.016%
26	11.616	1457	1467	1471	rBV2	9650	14947	0.76%	0.076%
27	11.945	1517	1523	1529	rBV4	5967	11042	0.56%	0.056%
28	12.169	1556	1561	1567	rBV5	3360	4970	0.25%	0.025%
29	12.557	1625	1627	1635	rBV9	1466	2142	0.11%	0.011%
30	12.828	1668	1673	1678	rVB9	2075	3185	0.16%	0.016%
31	13.187	1730	1734	1739	rVV7	1530	2835	0.14%	0.014%
32	13.651	1805	1813	1823	rBV	835979	1161903	58.84%	5.931%
33	13.910	1850	1857	1868	rBV	861042	1236278	62.61%	6.311%
34	14.222	1903	1910	1918	rBV	563867	784598	39.73%	4.005%
35	14.463	1945	1951	1964	rBV	38911	91834	4.65%	0.469%
36	14.675	1984	1987	1993	rVB8	2953	5249	0.27%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011561.D
 Acq On : 25 Aug 2022 12:28
 Operator : CG/JU
 Sample : N4320-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	15.228	2074	2081	2096	rBV	1134793	1569542	79.48%	8.012%
38	15.363	2098	2104	2117	rVV	449787	595326	30.15%	3.039%
39	15.469	2117	2122	2127	rVB8	6012	10809	0.55%	0.055%
40	15.957	2201	2205	2211	rBV4	5700	9135	0.46%	0.047%
41	16.134	2231	2235	2239	rBV7	1746	2775	0.14%	0.014%
42	16.469	2290	2292	2298	rVB6	2652	4003	0.20%	0.020%
43	16.669	2323	2326	2330	rBV5	1595	2805	0.14%	0.014%
44	16.781	2340	2345	2348	rBV7	1983	2665	0.13%	0.014%
45	16.992	2375	2381	2390	rBV	657880	906363	45.90%	4.627%
46	17.092	2392	2398	2415	rVV	1355908	1844523	93.41%	9.415%
47	17.216	2415	2419	2423	rVB6	2715	5378	0.27%	0.027%
48	17.304	2432	2434	2440	rVB6	1640	2283	0.12%	0.012%
49	17.557	2473	2477	2481	rBV6	1877	3266	0.17%	0.017%
50	17.692	2496	2500	2503	rBV6	2219	2468	0.12%	0.013%
51	17.910	2533	2537	2542	rBV4	14188	19294	0.98%	0.098%
52	17.992	2547	2551	2554	rVB	3056	4866	0.25%	0.025%
53	18.186	2582	2584	2588	rBV5	1518	2102	0.11%	0.011%
54	18.933	2706	2711	2715	rBV2	14738	20855	1.06%	0.106%
55	19.004	2719	2723	2726	rBV	15051	19797	1.00%	0.101%
56	19.163	2747	2750	2753	rBV4	4179	5852	0.30%	0.030%
57	19.357	2778	2783	2792	rBV	1566167	1940472	98.27%	9.905%
58	21.127	3079	3084	3089	rBV	736807	929031	47.05%	4.742%
59	23.268	3441	3448	3456	rBV2	1117451	1974727	100.00%	10.080%
60	23.415	3467	3473	3483	rVB2	524105	982240	49.74%	5.014%




Sum of corrected areas: 19590288

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011561.D
Acq On : 25 Aug 2022 12:28
Operator : CG/JU
Sample : N4320-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

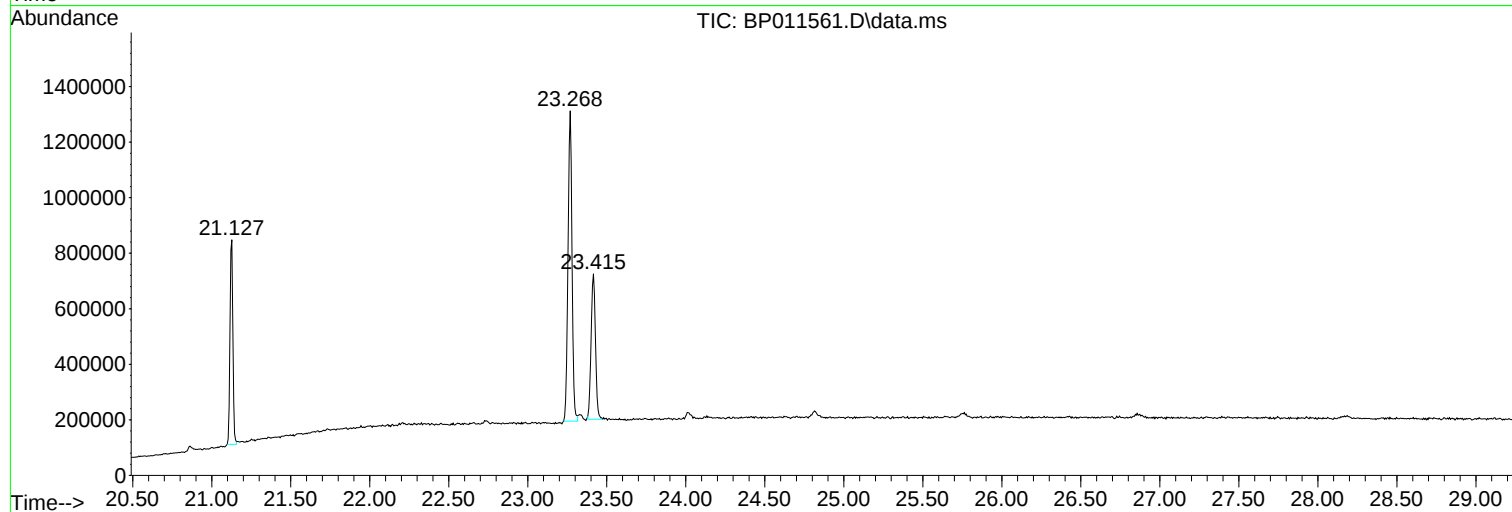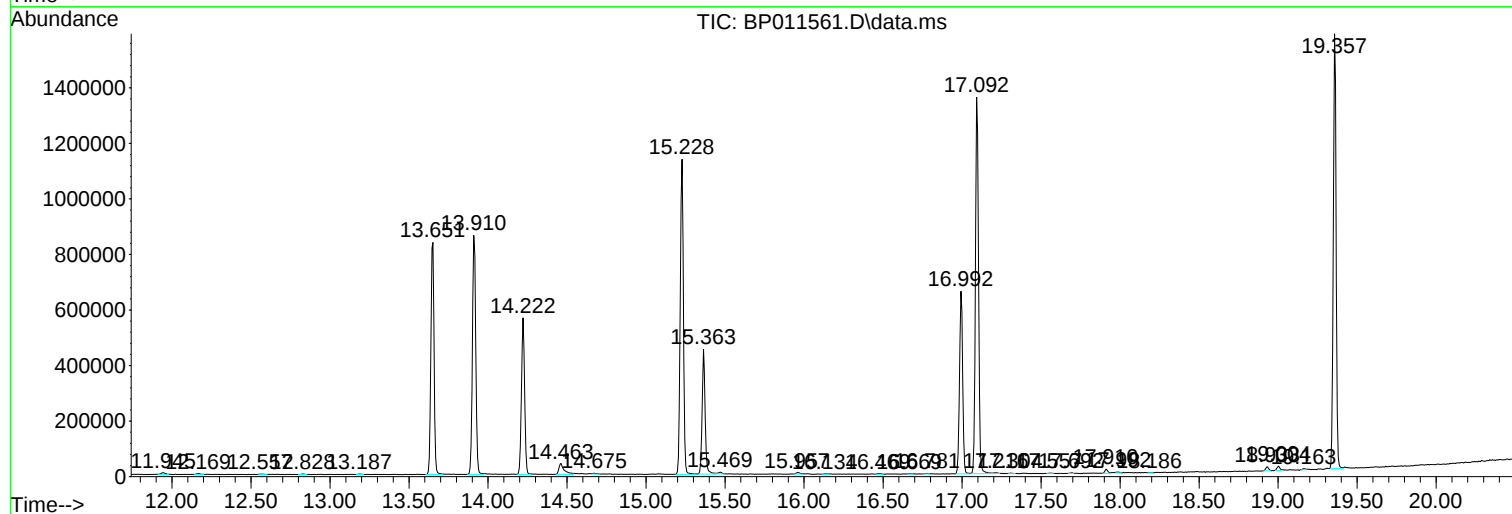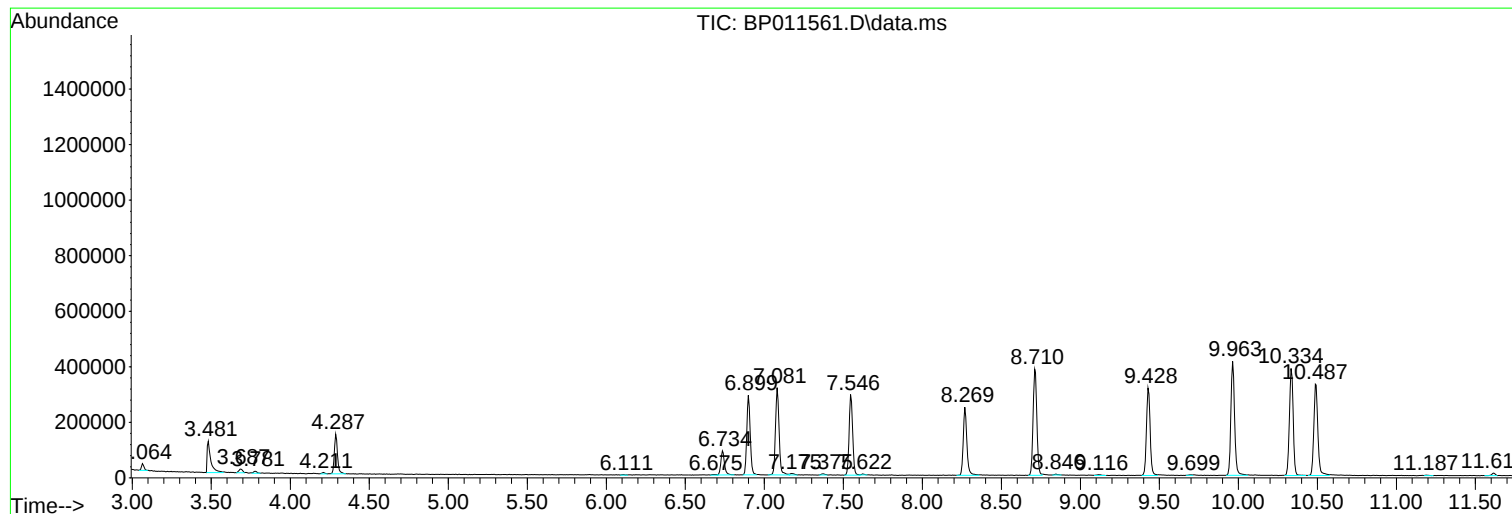

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011561.D
Acq On : 25 Aug 2022 12:28
Operator : CG/JU
Sample : N4320-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.287	8.85 ng/ul	199149	1,4-Dichlorobenzene-d4	7.546

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	12

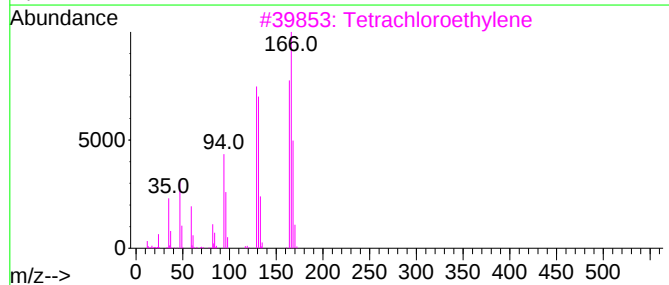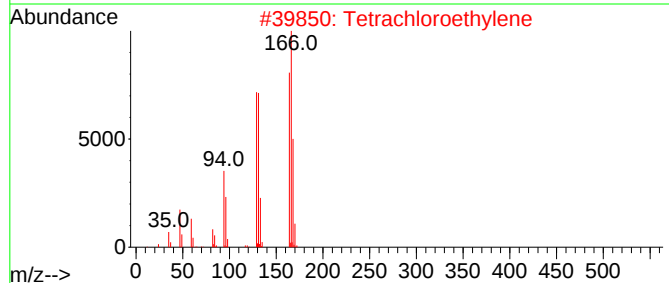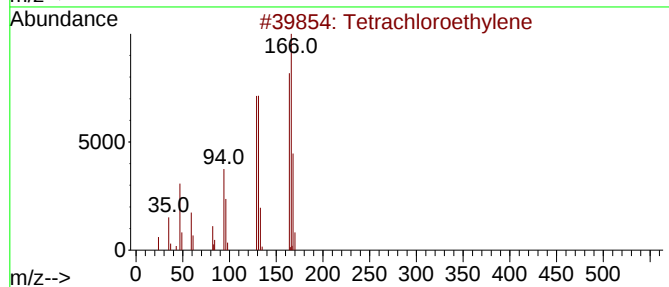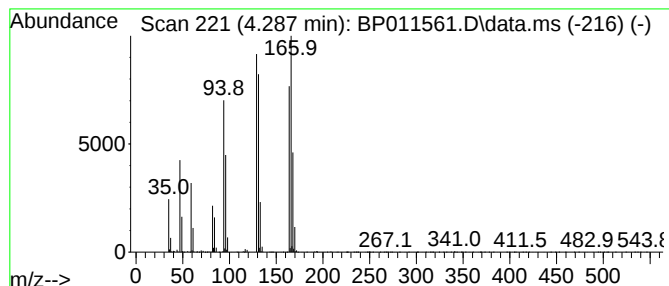

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011561.D
Acq On : 25 Aug 2022 12:28
Operator : CG/JU
Sample : N4320-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.287	8.8	ng/ul	199149	1	7.546	450145	20.0