

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011563.D
 Acq On : 25 Aug 2022 13:38
 Operator : CG/JU
 Sample : N4320-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	22	rVB	21356	27103	1.47%	0.154%
2	3.481	82	84	100	rBV	68483	110184	5.97%	0.628%
3	3.687	114	119	125	rVB	16023	24374	1.32%	0.139%
4	3.775	131	134	140	rVB3	6284	8770	0.48%	0.050%
5	4.211	204	208	215	rVB4	5083	8313	0.45%	0.047%
6	4.287	217	221	228	rVB4	11747	18333	0.99%	0.104%
7	4.793	306	307	312	rVB5	1388	1935	0.10%	0.011%
8	6.681	624	628	631	rBV5	2408	3514	0.19%	0.020%
9	6.734	631	637	648	rVV	80920	127169	6.89%	0.725%
10	6.899	658	665	677	rBV	259654	391370	21.21%	2.230%
11	7.081	689	696	708	rBV	279742	430160	23.32%	2.451%
12	7.163	708	710	716	rVB6	2245	3780	0.20%	0.022%
13	7.546	768	775	786	rBV	243737	374775	20.31%	2.135%
14	8.269	892	898	914	rBV	215211	349508	18.94%	1.991%
15	8.463	927	931	938	rVB9	885	2087	0.11%	0.012%
16	8.710	965	973	982	rBV	339177	554717	30.07%	3.161%
17	9.116	1037	1042	1051	rVB	2718	5024	0.27%	0.029%
18	9.428	1087	1095	1104	rBV	275062	450165	24.40%	2.565%
19	9.963	1179	1186	1203	rBV	362829	610925	33.11%	3.481%
20	10.334	1242	1249	1261	rVB	331792	532503	28.86%	3.034%
21	10.493	1267	1276	1293	rBV	259014	476455	25.83%	2.715%
22	11.616	1463	1467	1473	rVB7	1744	3033	0.16%	0.017%
23	11.904	1513	1516	1519	rBV4	1320	2171	0.12%	0.012%
24	11.945	1519	1523	1531	rVB4	5973	12036	0.65%	0.069%
25	12.569	1625	1629	1635	rVB8	1209	1942	0.11%	0.011%
26	13.645	1805	1812	1820	rBV	785927	1076987	58.38%	6.136%
27	13.910	1851	1857	1871	rBV	809696	1124577	60.96%	6.407%
28	14.157	1891	1899	1904	rBV6	4683	8933	0.48%	0.051%
29	14.222	1904	1910	1920	rVB	457329	679961	36.86%	3.874%
30	14.457	1945	1950	1962	rBV2	38618	89360	4.84%	0.509%
31	14.675	1985	1987	1991	rVB5	2351	2793	0.15%	0.016%
32	15.228	2073	2081	2089	rBV	1063334	1476859	80.05%	8.415%
33	15.363	2096	2104	2117	rBV	433605	571175	30.96%	3.254%
34	15.463	2118	2121	2128	rVB8	5708	9348	0.51%	0.053%
35	15.957	2199	2205	2212	rBV	38661	57431	3.11%	0.327%
36	16.475	2288	2293	2297	rBV7	1902	3067	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011563.D
 Acq On : 25 Aug 2022 13:38
 Operator : CG/JU
 Sample : N4320-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	16.775	2339	2344	2348	rBV7	2224	3813	0.21%	0.022%
38	16.992	2375	2381	2390	rBV	581812	791499	42.90%	4.510%
39	17.092	2392	2398	2416	rVV	1278065	1764538	95.65%	10.054%
40	17.304	2429	2434	2440	rVB	31802	40305	2.18%	0.230%
41	17.563	2475	2478	2482	rVB5	1533	1859	0.10%	0.011%
42	17.910	2533	2537	2544	rBV7	12464	20338	1.10%	0.116%
43	17.986	2547	2550	2555	rVB4	3031	4501	0.24%	0.026%
44	18.286	2599	2601	2605	rVB5	2244	2785	0.15%	0.016%
45	18.445	2624	2628	2630	rBV5	2355	2967	0.16%	0.017%
46	18.927	2706	2710	2715	rBV5	13141	18933	1.03%	0.108%
47	18.998	2718	2722	2728	rVV	14530	20818	1.13%	0.119%
48	19.075	2733	2735	2738	rBV3	3125	2300	0.12%	0.013%
49	19.163	2747	2750	2753	rBV4	4949	4959	0.27%	0.028%
50	19.357	2777	2783	2792	rBV	1483066	1844859	100.00%	10.511%
51	21.121	3079	3083	3092	rBV	630531	792475	42.96%	4.515%
52	23.268	3441	3448	3455	rBV	985365	1787415	96.89%	10.184%
53	23.415	3467	3473	3482	rVB2	429753	816143	44.24%	4.650%




Sum of corrected areas: 17551344

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011563.D
Acq On : 25 Aug 2022 13:38
Operator : CG/JU
Sample : N4320-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

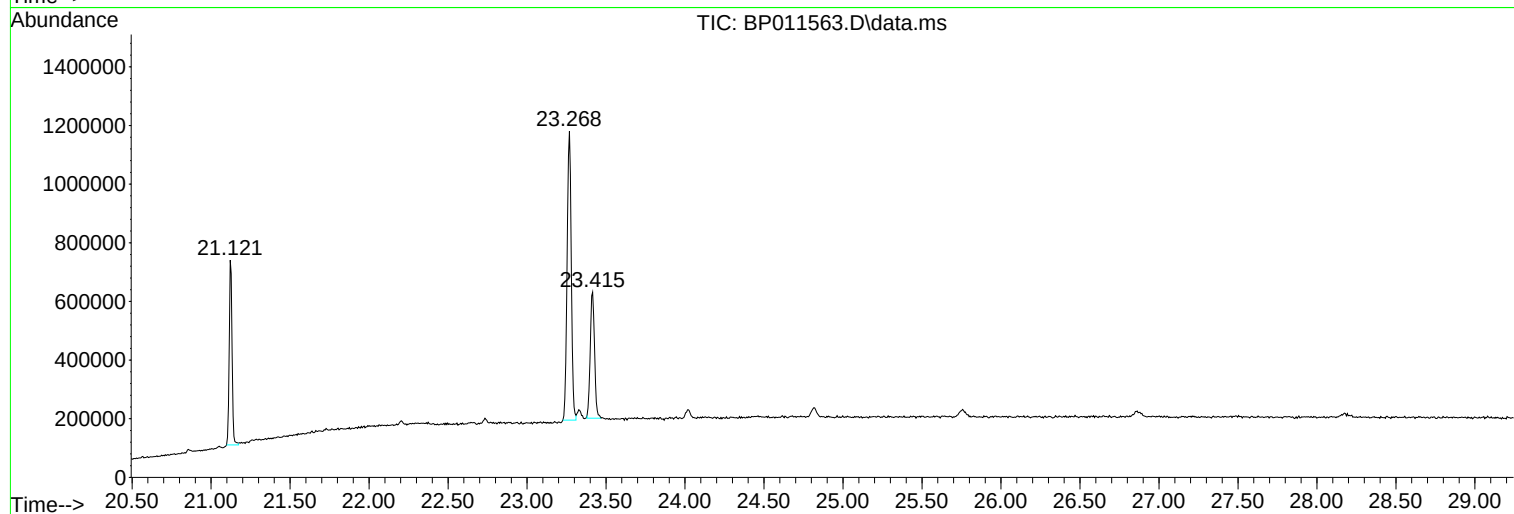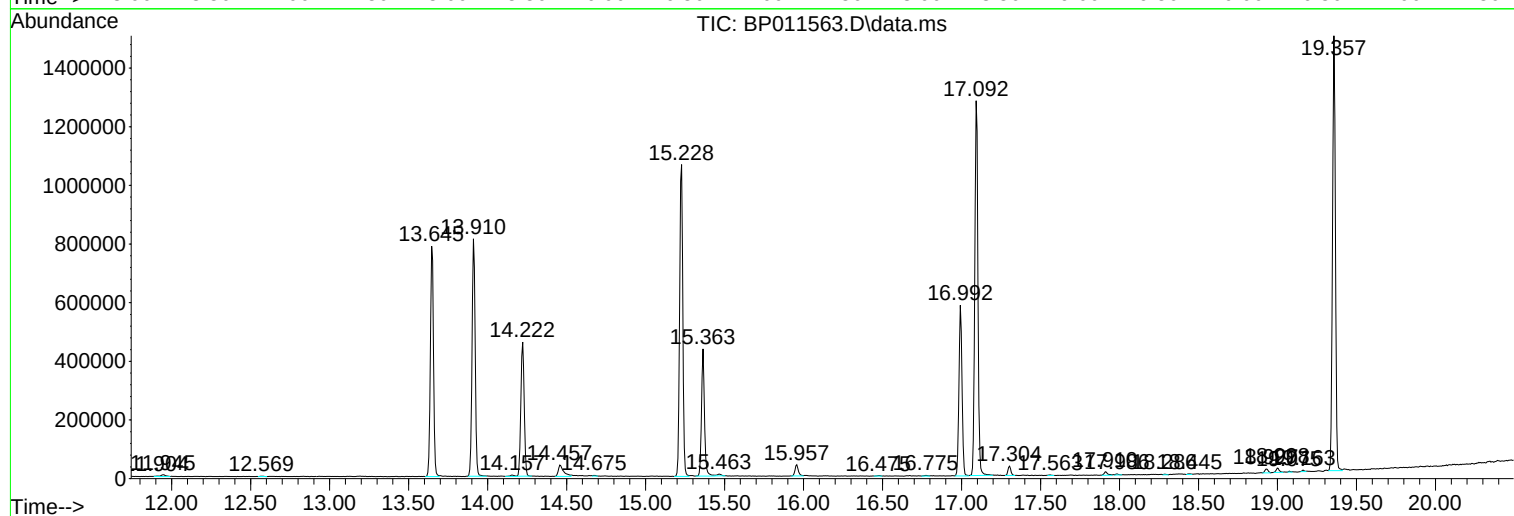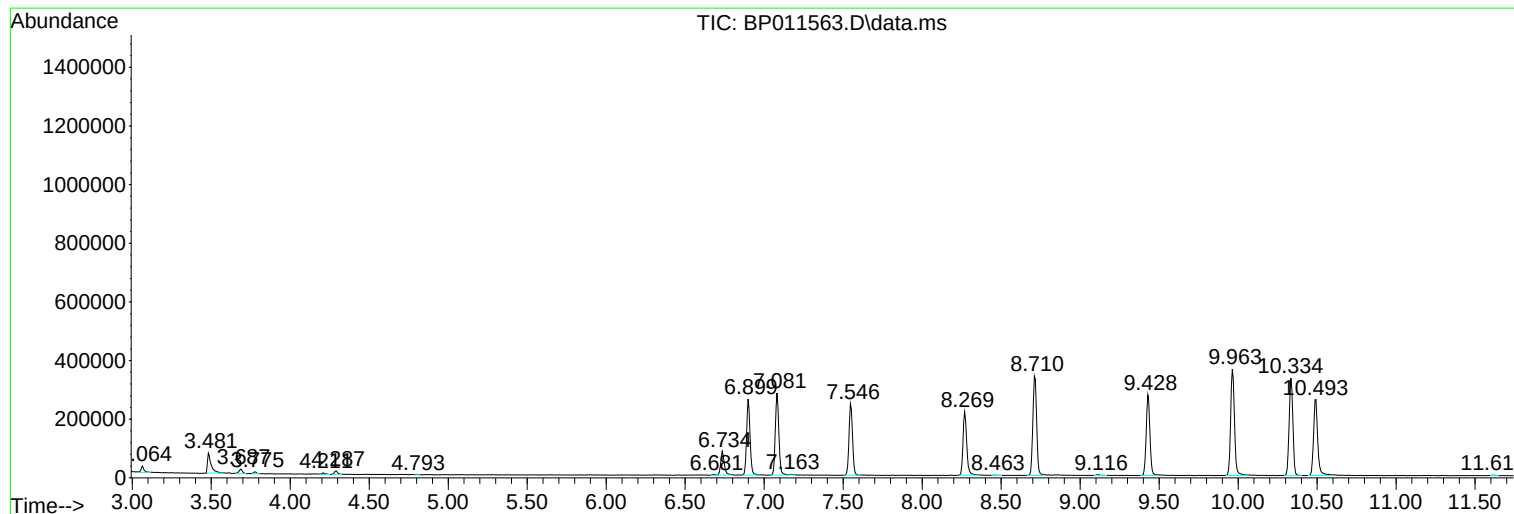

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011563.D
Acq On : 25 Aug 2022 13:38
Operator : CG/JU
Sample : N4320-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011563.D
Acq On : 25 Aug 2022 13:38
Operator : CG/JU
Sample : N4320-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc