

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
 Data File : BP011565.D
 Acq On : 25 Aug 2022 16:42
 Operator : CG/JU
 Sample : PB147282BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK282

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	23	rVB	32127	42949	2.53%	0.204%
2	3.469	79	82	108	rBV	330180	524738	30.89%	2.496%
3	3.775	130	134	141	rVB2	7698	11683	0.69%	0.056%
4	5.410	408	412	415	rBV6	1389	1776	0.10%	0.008%
5	6.734	630	637	651	rBV	413244	647019	38.09%	3.077%
6	6.899	657	665	678	rBB	311084	470023	27.67%	2.236%
7	7.081	689	696	711	rBV	423083	650379	38.28%	3.093%
8	7.546	768	775	788	rVB	360982	557071	32.79%	2.650%
9	8.269	892	898	912	rBV	472220	763970	44.97%	3.634%
10	8.463	926	931	934	rVB7	1092	2129	0.13%	0.010%
11	8.710	966	973	988	rBV	396017	640453	37.70%	3.046%
12	9.428	1088	1095	1105	rBV	339635	536438	31.58%	2.551%
13	9.963	1178	1186	1201	rBV	448172	745651	43.89%	3.546%
14	10.334	1241	1249	1261	rBV	479793	775353	45.64%	3.688%
15	10.487	1268	1275	1291	rBV	397935	698893	41.14%	3.324%
16	10.610	1294	1296	1299	rVB3	1739	1910	0.11%	0.009%
17	11.945	1518	1523	1530	rBV5	6410	11894	0.70%	0.057%
18	13.645	1806	1812	1824	rBV	819420	1115364	65.66%	5.305%
19	13.910	1848	1857	1870	rBV2	828390	1197742	70.51%	5.697%
20	14.222	1903	1910	1920	rBV	681885	950318	55.94%	4.520%
21	14.451	1942	1949	1963	rBV	286677	523639	30.82%	2.491%
22	14.645	1980	1982	1986	rVB5	2730	3422	0.20%	0.016%
23	15.228	2074	2081	2090	rBV	1076820	1476760	86.93%	7.024%
24	15.363	2097	2104	2113	rBV	386982	528808	31.13%	2.515%
25	15.463	2118	2121	2128	rVB5	5934	9461	0.56%	0.045%
26	15.804	2173	2179	2180	rBV6	1318	2206	0.13%	0.010%
27	16.010	2212	2214	2220	rBV6	1780	2334	0.14%	0.011%
28	16.633	2317	2320	2323	rBV5	1743	2548	0.15%	0.012%
29	16.780	2343	2345	2349	rVB5	1669	1998	0.12%	0.010%
30	16.992	2375	2381	2391	rBV	793073	1080849	63.62%	5.141%
31	17.092	2392	2398	2411	rVV2	1143818	1602380	94.32%	7.621%
32	18.927	2707	2710	2716	rBV5	12507	18653	1.10%	0.089%
33	18.998	2719	2722	2727	rBV	12957	17007	1.00%	0.081%
34	19.357	2777	2783	2791	rBV	1378760	1698801	100.00%	8.080%
35	21.121	3078	3083	3093	rBV	908770	1101891	64.86%	5.241%
36	23.262	3441	3447	3454	rBV	873871	1562672	91.99%	7.432%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011565.D
Acq On : 25 Aug 2022 16:42
Operator : CG/JU
Sample : PB147282BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK282

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Title : SVOA CALIBRATION

37	23.410	3466	3472	3482	rVB	571518	1045922	61.57%	4.975%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 21025104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011565.D
Acq On : 25 Aug 2022 16:42
Operator : CG/JU
Sample : PB147282BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK282

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

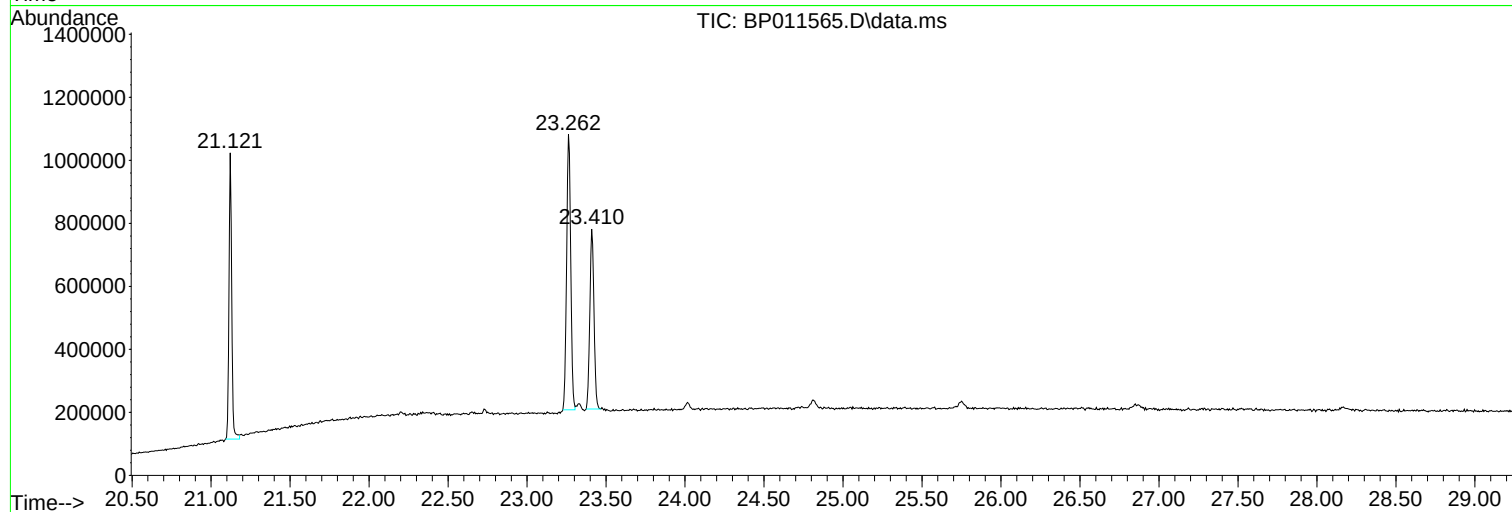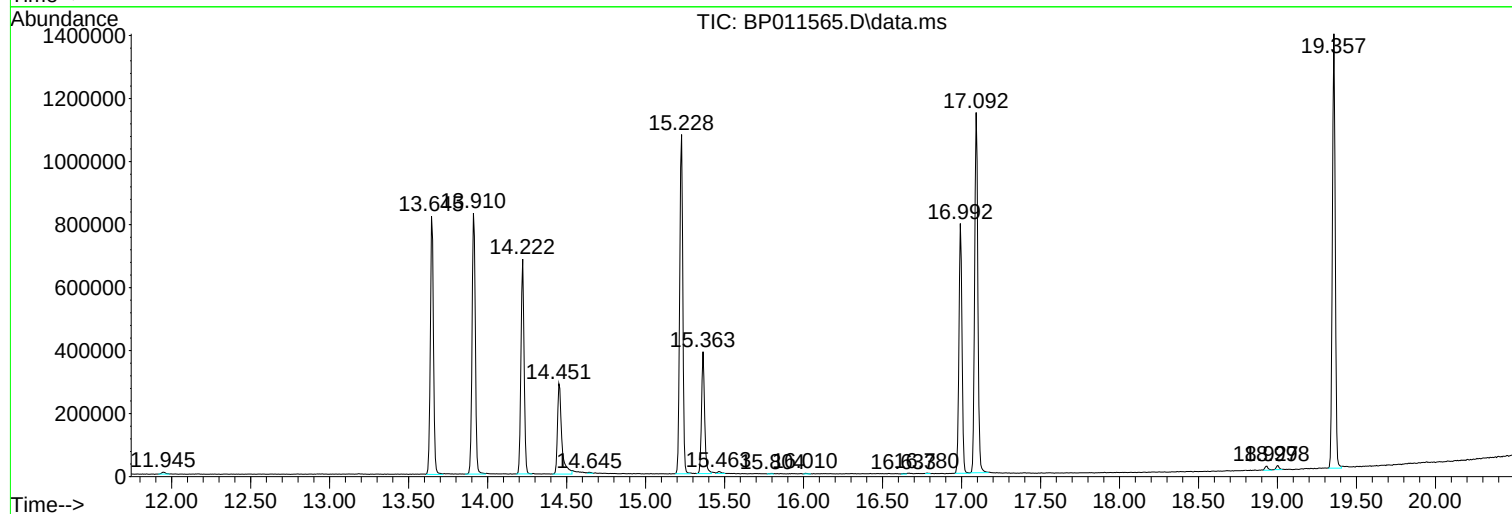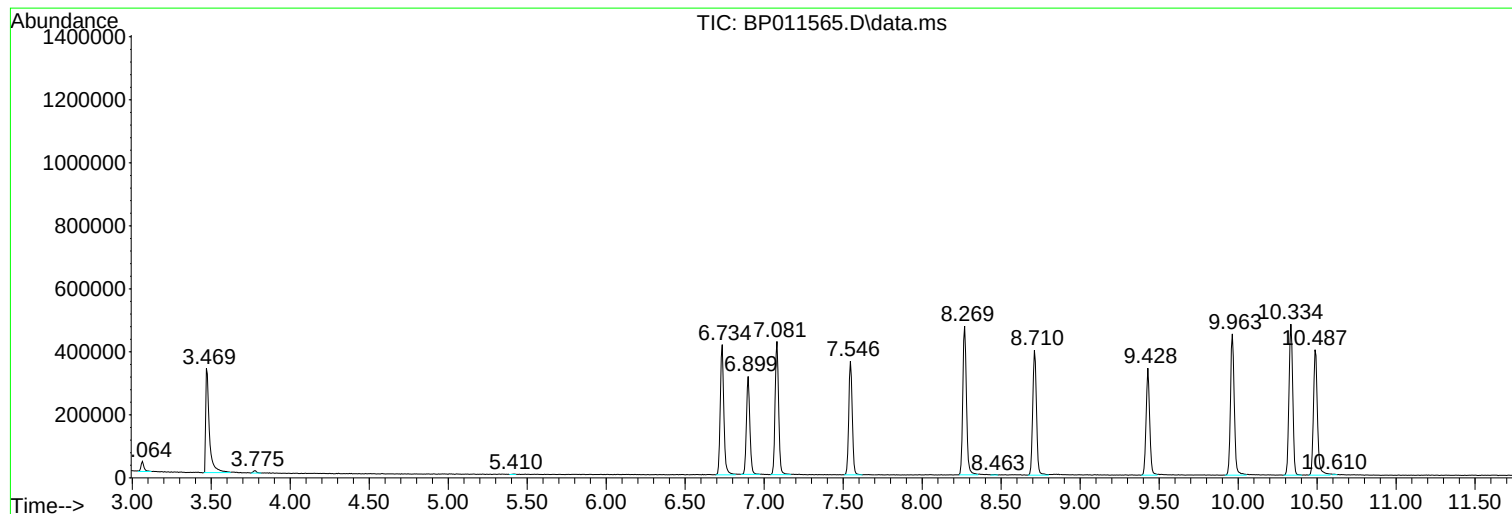

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011565.D
Acq On : 25 Aug 2022 16:42
Operator : CG/JU
Sample : PB147282BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK282

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082422\
Data File : BP011565.D
Acq On : 25 Aug 2022 16:42
Operator : CG/JU
Sample : PB147282BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK282

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc