


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP082520\
 Data File : BP003097.D
 Acq On : 25 Aug 2020 14:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 15:32:08 2020

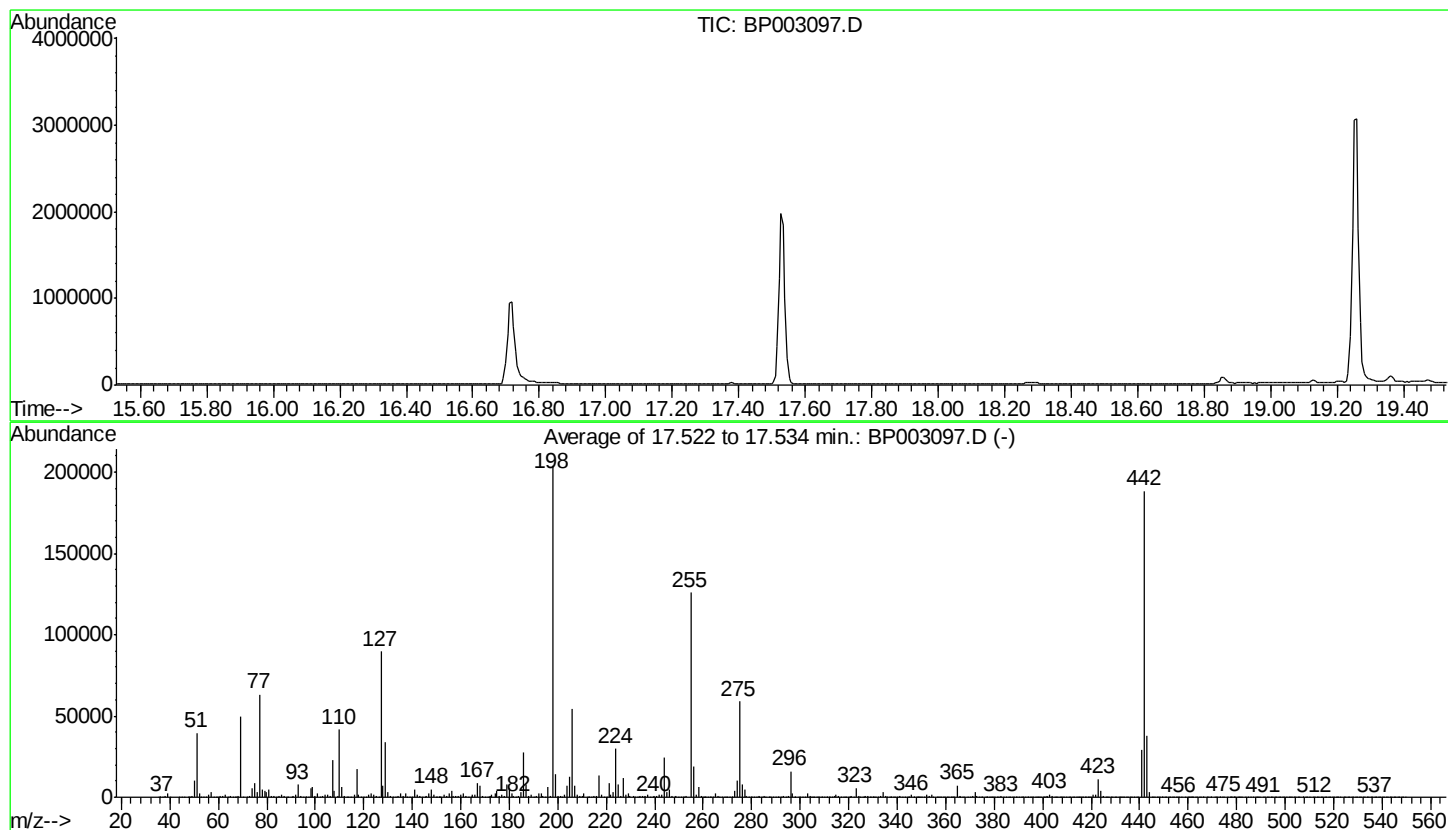

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.4	39639	PASS
68	69	0.00	2	2.0	1003	PASS
69	198	0.00	100	24.2	49298	PASS
70	69	0.00	2	0.6	286	PASS
127	198	10	80	44.0	89800	PASS
197	198	0.00	2	0.5	1078	PASS
198	198	100	100	100.0	204083	PASS
199	198	5	9	6.8	13847	PASS
275	198	10	60	28.8	58792	PASS
365	198	1	100	3.6	7312	PASS
441	198	0.01	100	14.3	29108	PASS
442	198	50	100	92.5	188679	PASS
443	442	15	24	20.0	37797	PASS