
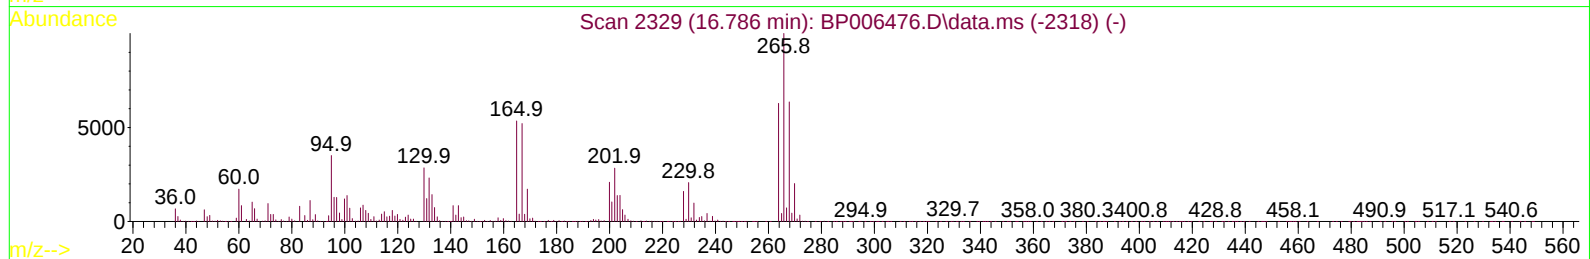
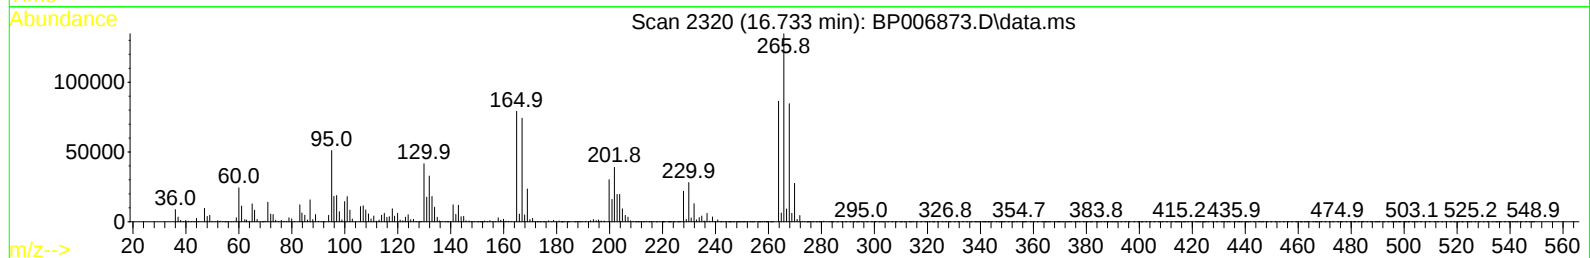


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006873.D
 Acq On : 25 Aug 2021 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 11:24:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 13:40:38 2021
 Response via : Initial Calibration

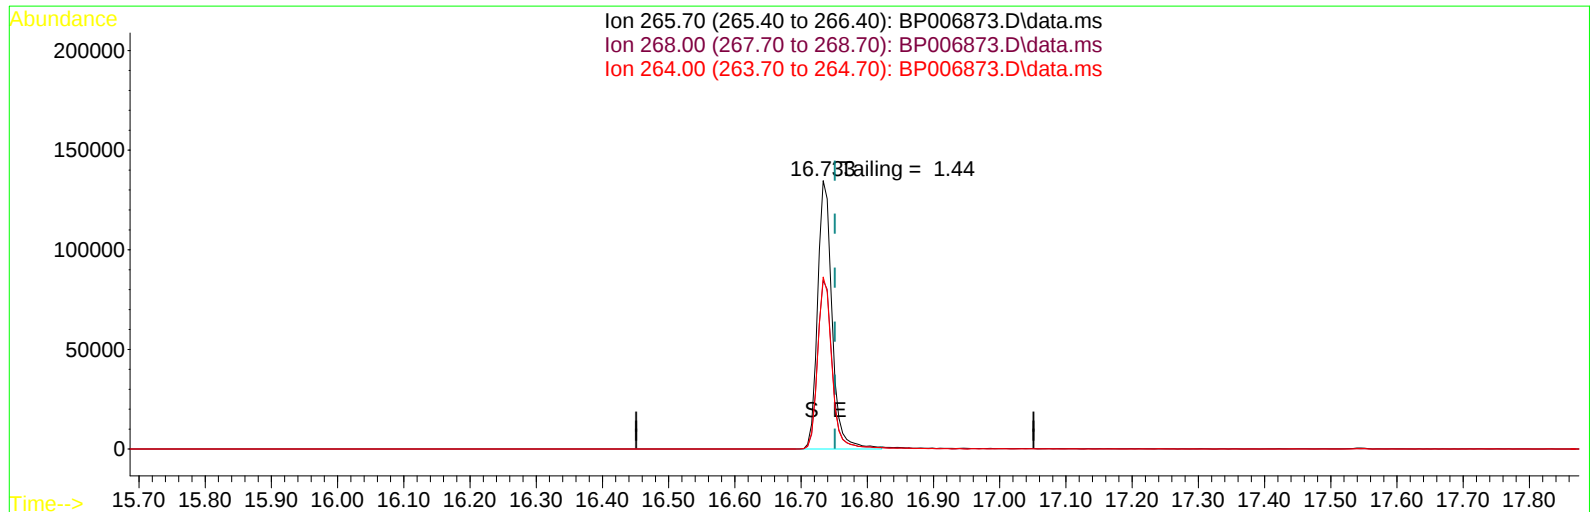

TIC: BP006873.D\data.ms

(70) Pentachlorophenol (C)




16.733min (-0.018) 780121.99 ng

response 205371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.80
264.00	62.90	64.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006873.D
 Acq On : 25 Aug 2021 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 11:24:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 13:40:38 2021
 Response via : Initial Calibration

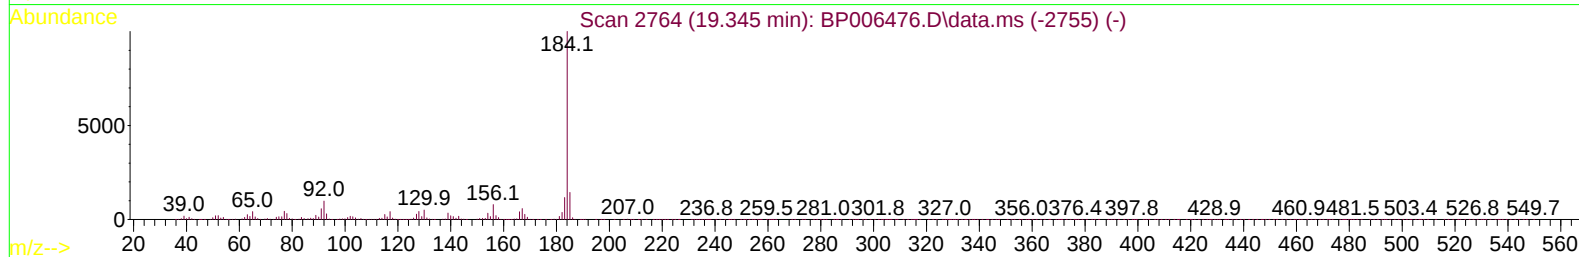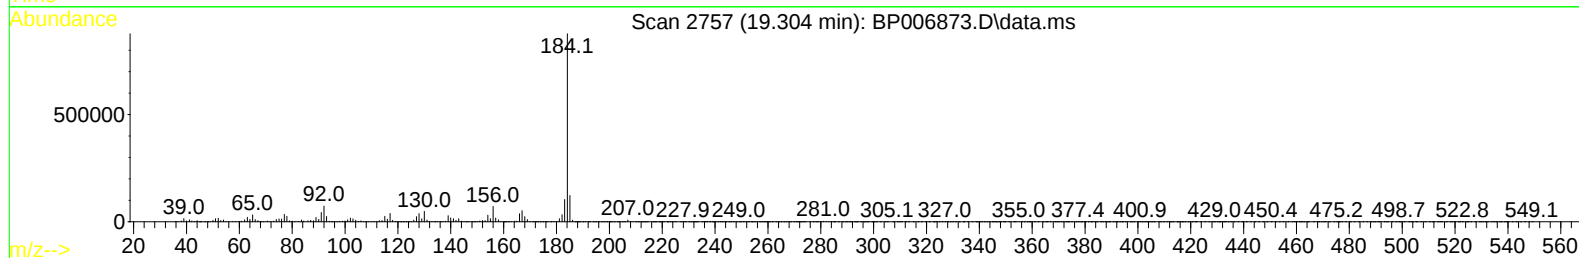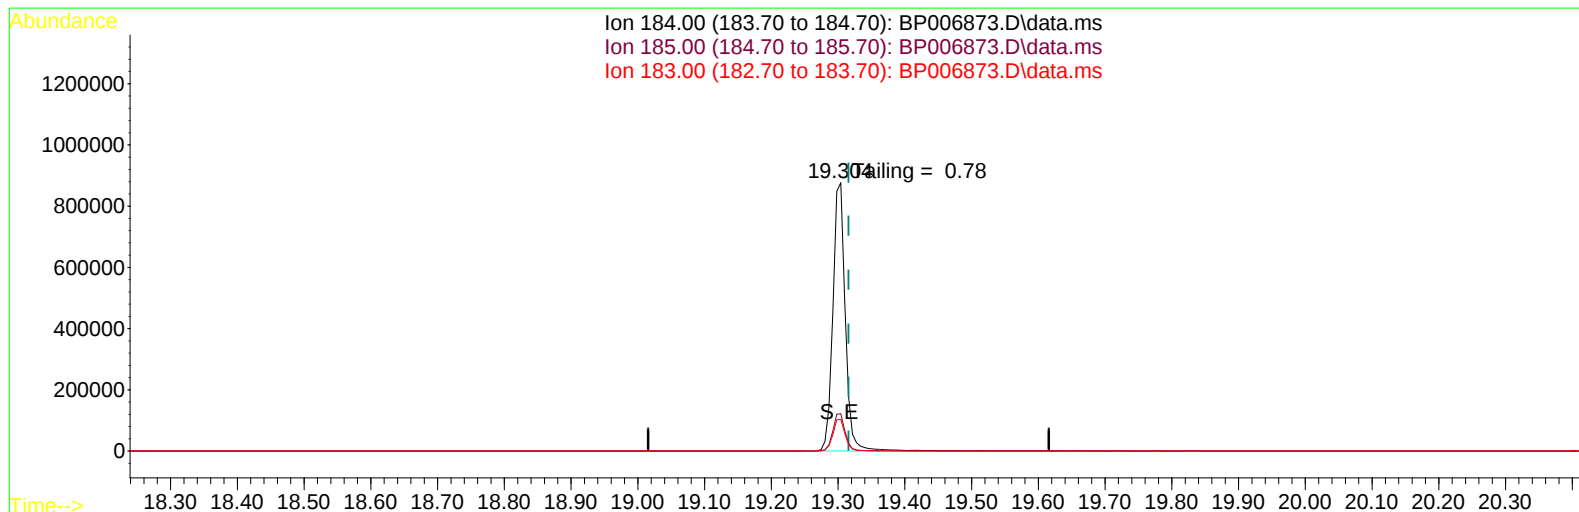

TIC: BP006873.D\data.ms

(77) Benzidine**19.304min (-0.012) 685079.60 ng****response 1131436**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.93
183.00	11.90	11.83
0.00	0.00	0.00