

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006875.D
 Acq On : 25 Aug 2021 10:34
 Operator : CG/JU
 Sample : PB138637BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB138637BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.287	368	374	388	rVB	2879616	4172102	47.66%	10.698%
2	6.875	637	644	655	rBV	2738455	4193798	47.90%	10.753%
3	7.681	775	781	788	rBV	522278	799557	9.13%	2.050%
4	8.846	972	979	993	rVB	1707408	2791749	31.89%	7.158%
5	10.463	1247	1254	1263	rBV	672327	1128016	12.88%	2.892%
6	12.946	1669	1676	1691	rBV	3884661	5845477	66.77%	14.989%
7	14.328	1904	1911	1922	rBV	917016	1393565	15.92%	3.573%
8	15.828	2159	2166	2190	rBV	3039454	4448966	50.82%	11.408%
9	17.086	2373	2380	2392	rBV	1123342	1634737	18.67%	4.192%
10	19.669	2813	2819	2824	rBV	7423179	8754799	100.00%	22.448%
11	21.192	3073	3078	3086	rBV	1446780	1856100	21.20%	4.759%
12	23.498	3463	3470	3482	rVB2	989119	1980726	22.62%	5.079%




Sum of corrected areas: 38999592

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006875.D
Acq On : 25 Aug 2021 10:34
Operator : CG/JU
Sample : PB138637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138637BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

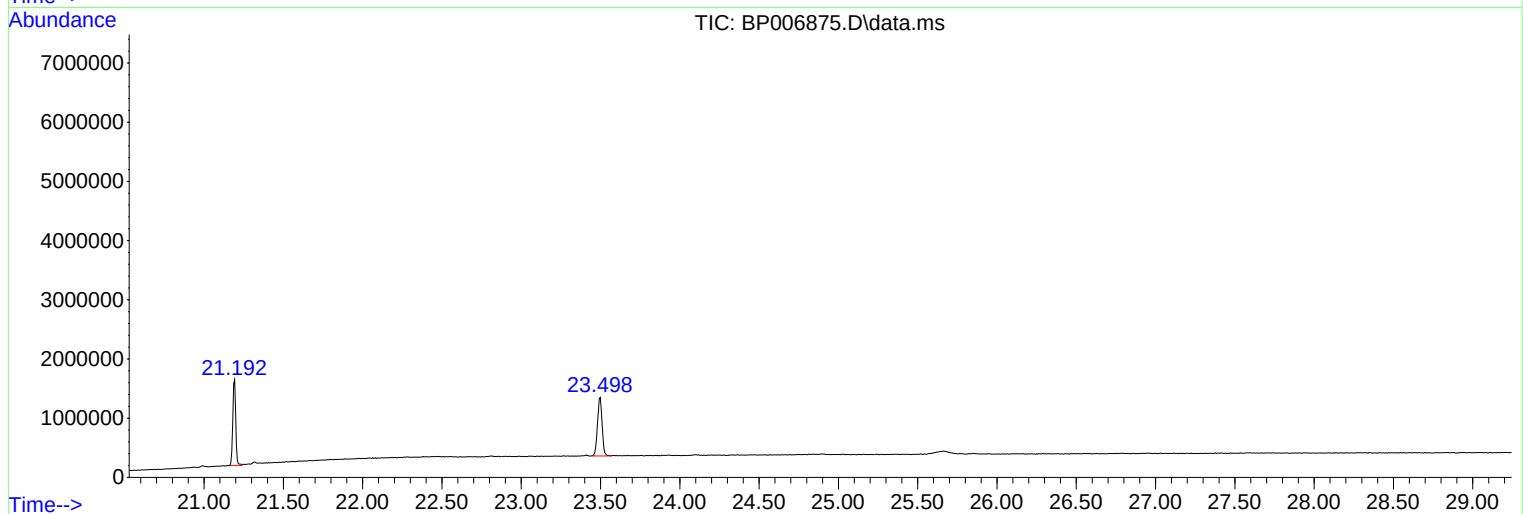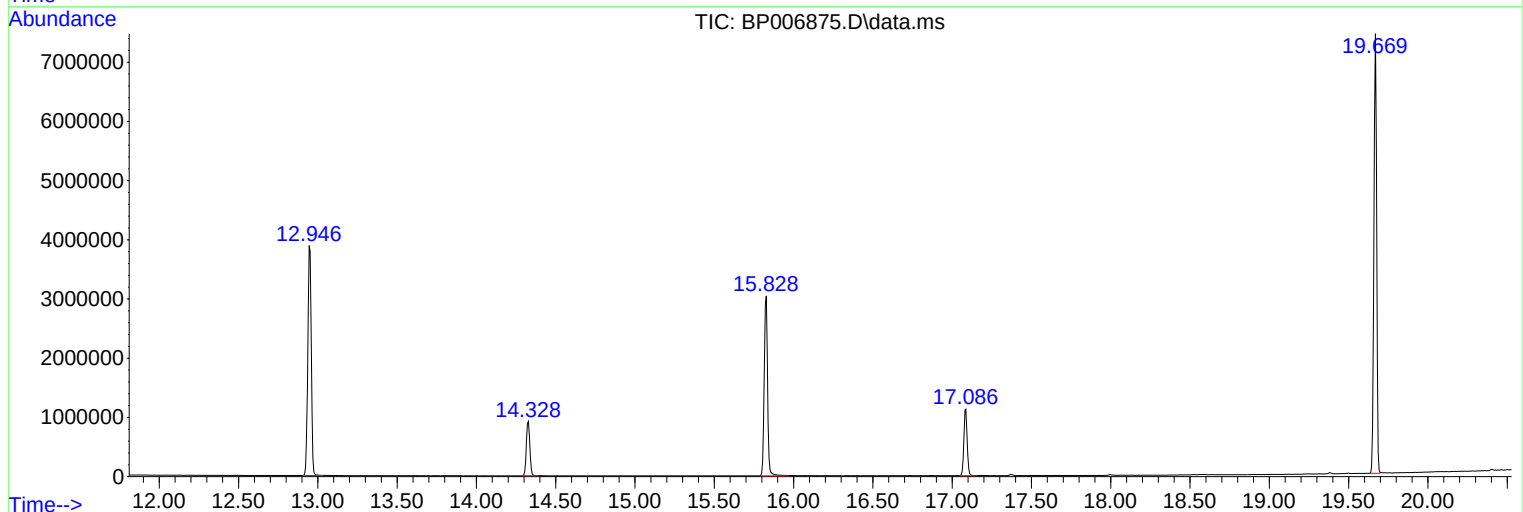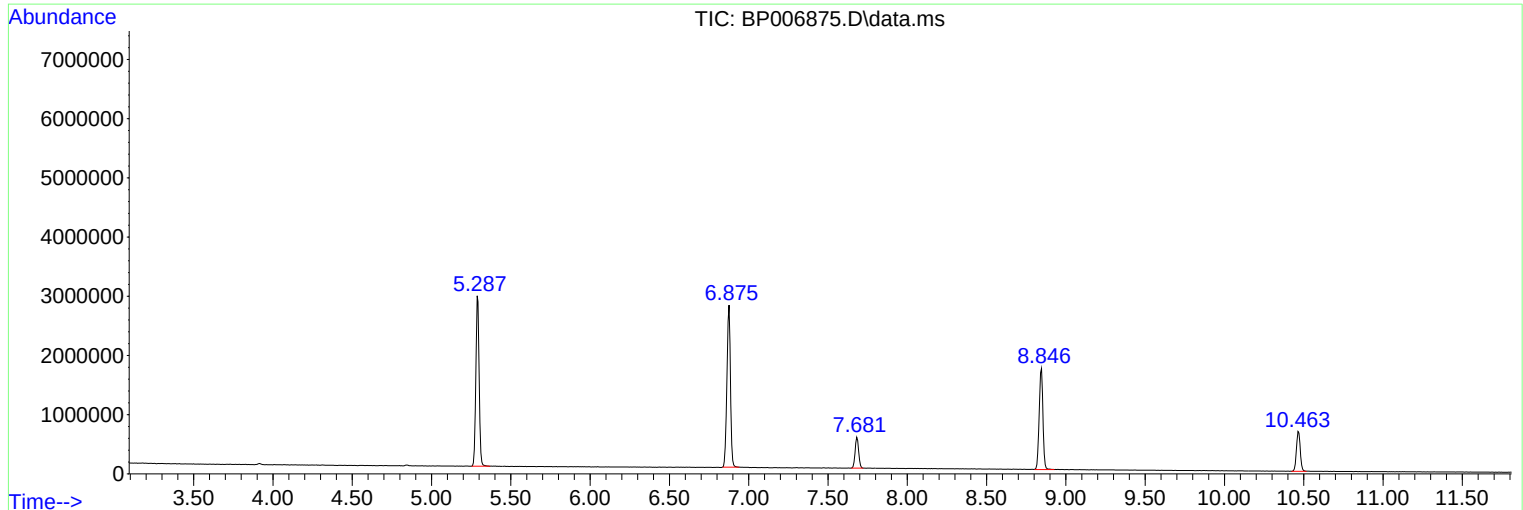

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006875.D
Acq On : 25 Aug 2021 10:34
Operator : CG/JU
Sample : PB138637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138637BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006875.D
Acq On : 25 Aug 2021 10:34
Operator : CG/JU
Sample : PB138637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138637BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------