

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006877.D
 Acq On : 25 Aug 2021 12:35
 Operator : CG/JU
 Sample : M3463-41
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 2021-08-17-EB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.287	368	374	382	rVB	1243757	1725983	19.15%	4.111%
2	5.752	450	453	456	rBV2	63019	90632	1.01%	0.216%
3	5.787	456	459	469	rVB	133232	191880	2.13%	0.457%
4	6.869	637	643	652	rVB	681125	1061667	11.78%	2.529%
5	7.681	775	781	788	rBV	551774	828848	9.20%	1.974%
6	7.934	820	824	834	rVB	48797	96563	1.07%	0.230%
7	8.781	963	968	972	rBV	176292	267450	2.97%	0.637%
8	8.846	972	979	989	rVV	1728687	2827074	31.37%	6.733%
9	9.011	1003	1007	1015	rVB	66750	117929	1.31%	0.281%
10	9.740	1123	1131	1139	rBV	324294	723301	8.02%	1.723%
11	9.975	1162	1171	1180	rBV	411974	753913	8.36%	1.796%
12	10.463	1247	1254	1261	rBV	723667	1190144	13.20%	2.835%
13	11.016	1343	1348	1354	rBV	101787	165819	1.84%	0.395%
14	11.081	1354	1359	1363	rBV	105816	155532	1.73%	0.370%
15	12.687	1625	1632	1645	rVB2	58079	119364	1.32%	0.284%
16	12.946	1669	1676	1689	rBV	3941602	5949995	66.01%	14.171%
17	13.257	1720	1729	1744	rBV	319798	501882	5.57%	1.195%
18	14.199	1883	1889	1901	rBV3	44034	103498	1.15%	0.247%
19	14.328	1904	1911	1922	rVB	1015826	1512274	16.78%	3.602%
20	15.828	2157	2166	2179	rBV	3296422	4692386	52.06%	11.176%
21	17.087	2373	2380	2389	rBV	1230294	1729234	19.19%	4.119%
22	17.769	2491	2496	2506	rBV	850419	1031777	11.45%	2.457%
23	17.998	2530	2535	2543	rBV	136890	232606	2.58%	0.554%
24	18.063	2543	2546	2555	rVB	57443	107055	1.19%	0.255%
25	19.239	2742	2746	2754	rBV	82281	129848	1.44%	0.309%
26	19.669	2814	2819	2825	rBV	7490447	9013111	100.00%	21.467%
27	21.192	3073	3078	3083	rBV	1631572	1971101	21.87%	4.695%
28	22.280	3258	3263	3276	rBV	1752069	2567617	28.49%	6.115%
29	23.498	3464	3470	3480	rVB2	1096405	2127303	23.60%	5.067%




Sum of corrected areas: 41985786

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006877.D
Acq On : 25 Aug 2021 12:35
Operator : CG/JU
Sample : M3463-41
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-17-EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

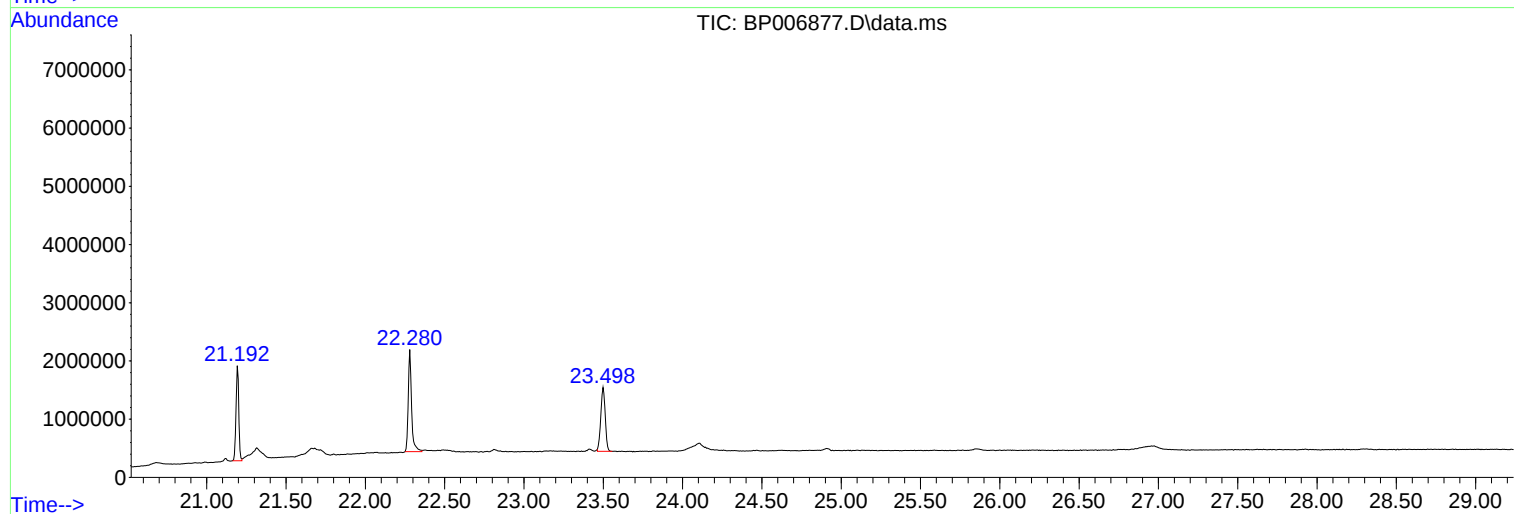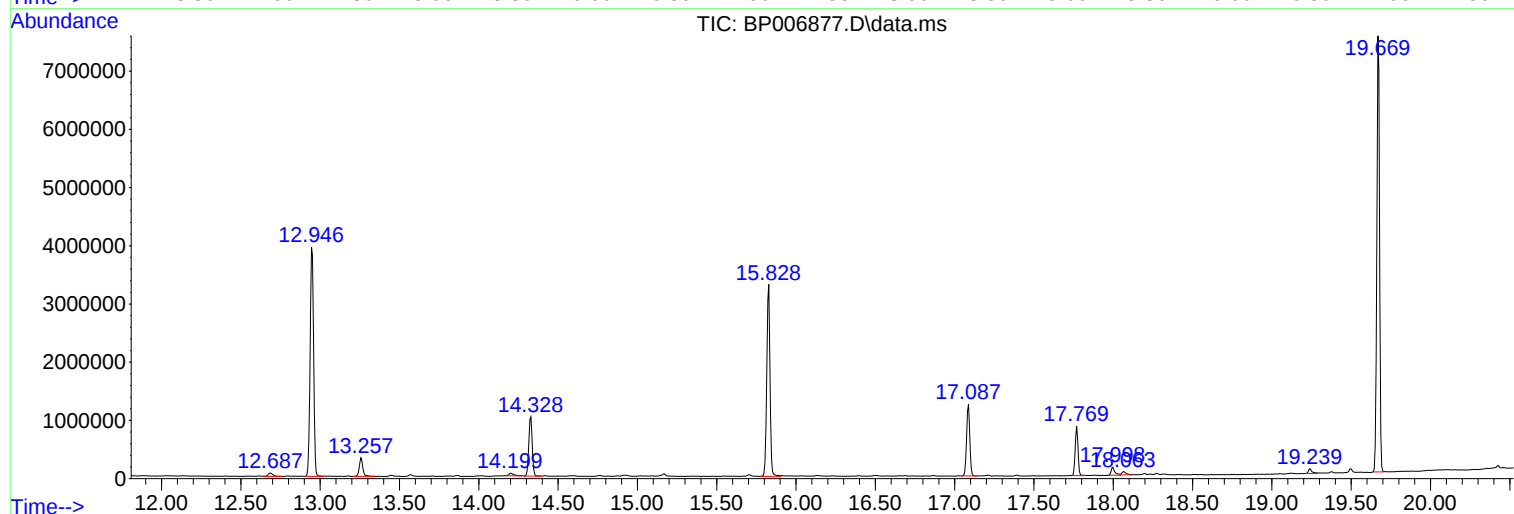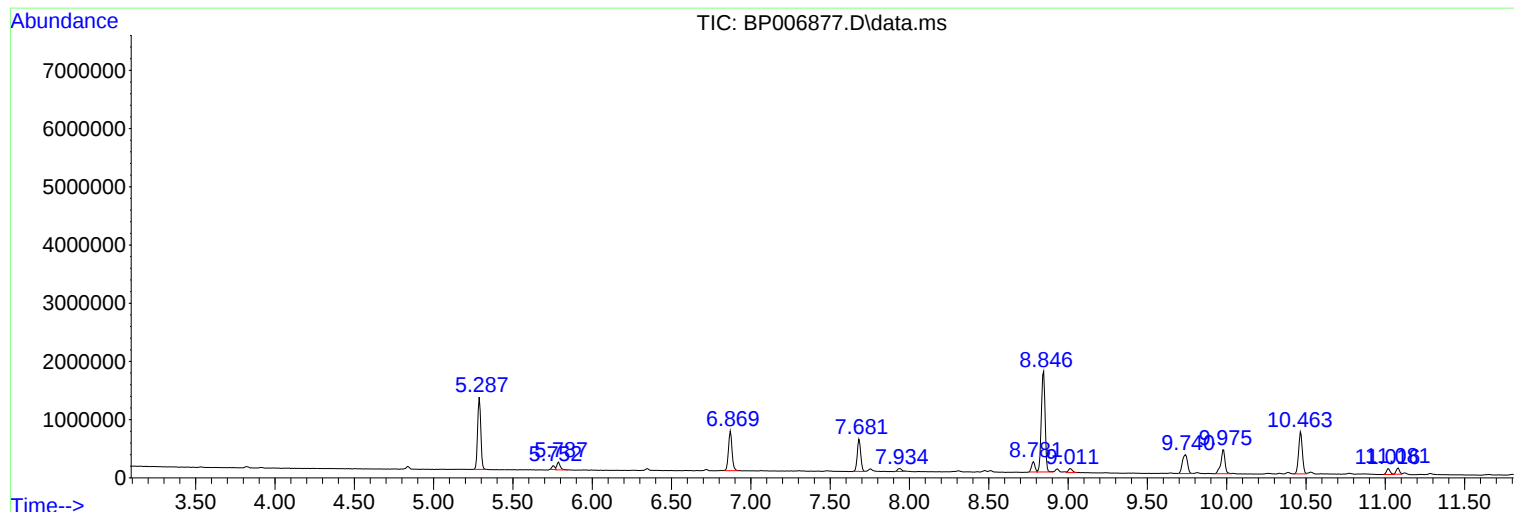

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006877.D
Acq On : 25 Aug 2021 12:35
Operator : CG/JU
Sample : M3463-41
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-17-EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006877.D
Acq On : 25 Aug 2021 12:35
Operator : CG/JU
Sample : M3463-41
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
2021-08-17-EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------