

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006881.D
 Acq On : 25 Aug 2021 15:30
 Operator : CG/JU
 Sample : M3463-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-16-0204

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.911	138	140	149	rVB	51723	73733	1.25%	0.106%
2	4.428	223	228	237	rVB	178177	283120	4.79%	0.406%
3	5.016	323	328	339	rVB	305836	477435	8.07%	0.685%
4	5.210	357	361	368	rVB2	42195	62582	1.06%	0.090%
5	5.287	368	374	379	rVV	2338222	3247793	54.89%	4.657%
6	5.340	379	383	395	rVB	168164	300318	5.08%	0.431%
7	5.705	440	445	451	rVB	122576	193492	3.27%	0.277%
8	6.869	637	643	654	rVB	2143242	3442549	58.18%	4.936%
9	7.304	713	717	726	rBV5	52779	100209	1.69%	0.144%
10	7.681	772	781	788	rVB	756999	1234499	20.86%	1.770%
11	7.993	829	834	842	rVB	263234	441728	7.47%	0.633%
12	8.228	866	874	879	rBV	197568	327762	5.54%	0.470%
13	8.334	889	892	901	rVB2	40297	72888	1.23%	0.105%
14	8.440	906	910	916	rBV4	29570	65734	1.11%	0.094%
15	8.775	959	967	971	rBV7	26094	66679	1.13%	0.096%
16	8.840	972	978	985	rVV	1564600	2624707	44.36%	3.763%
17	8.904	985	989	998	rVB	73284	134858	2.28%	0.193%
18	9.381	1065	1070	1077	rVB5	39751	70549	1.19%	0.101%
19	9.640	1110	1114	1124	rVB8	43065	81530	1.38%	0.117%
20	9.751	1124	1133	1136	rVB4	28579	61751	1.04%	0.089%
21	9.898	1149	1158	1165	rBV6	48171	102816	1.74%	0.147%
22	10.263	1213	1220	1228	rBV	597647	977773	16.53%	1.402%
23	10.463	1242	1254	1260	rBV	1037364	1792268	30.29%	2.570%
24	10.522	1260	1264	1270	rVB2	74043	155935	2.64%	0.224%
25	10.634	1279	1283	1289	rVB	96679	140539	2.38%	0.202%
26	11.157	1361	1372	1378	rBV2	144774	265689	4.49%	0.381%
27	11.310	1391	1398	1405	rVV5	27177	61189	1.03%	0.088%
28	11.387	1405	1411	1419	rVB7	35602	75574	1.28%	0.108%
29	11.498	1425	1430	1435	rBV	134106	222504	3.76%	0.319%
30	12.128	1531	1537	1544	rVB2	58481	135118	2.28%	0.194%
31	12.598	1612	1617	1624	rVB4	30821	69013	1.17%	0.099%
32	12.869	1658	1663	1666	rBV	102901	140959	2.38%	0.202%
33	12.951	1671	1677	1683	rVB	3286905	4748348	80.25%	6.808%
34	13.098	1696	1702	1705	rBV5	41060	73880	1.25%	0.106%
35	13.469	1760	1765	1769	rBV2	53524	87010	1.47%	0.125%
36	13.645	1791	1795	1799	rBV2	48113	83058	1.40%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006881.D
 Acq On : 25 Aug 2021 15:30
 Operator : CG/JU
 Sample : M3463-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SWCS-16-0204

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	13.739	1807	1811	1815	rVV2	102855	135497	2.29%	0.194%
38	13.822	1815	1825	1829	rVV4	149547	316139	5.34%	0.453%
39	13.869	1829	1833	1839	rVB7	35315	84289	1.42%	0.121%
40	14.051	1858	1864	1869	rBV	221802	367805	6.22%	0.527%
41	14.157	1877	1882	1888	rBV3	92217	194791	3.29%	0.279%
42	14.222	1888	1893	1901	rVB3	149365	338849	5.73%	0.486%
43	14.333	1901	1912	1918	rBV	1372597	2134051	36.07%	3.060%
44	14.392	1919	1922	1930	rVB2	91984	158667	2.68%	0.227%
45	14.739	1977	1981	1986	rVB3	56123	84048	1.42%	0.121%
46	14.869	1998	2003	2005	rBV3	86431	136159	2.30%	0.195%
47	15.116	2041	2045	2049	rBV3	84293	133793	2.26%	0.192%
48	15.345	2081	2084	2087	rBV	74778	89152	1.51%	0.128%
49	15.386	2087	2091	2096	rVB2	152808	207791	3.51%	0.298%
50	15.610	2124	2129	2134	rVB	115530	191634	3.24%	0.275%
51	15.686	2139	2142	2150	rVB8	56883	90259	1.53%	0.129%
52	15.833	2161	2167	2174	rVB	2443488	3437229	58.09%	4.928%
53	16.092	2203	2211	2215	rBV2	219164	443277	7.49%	0.636%
54	16.916	2347	2351	2359	rVB2	288739	474741	8.02%	0.681%
55	17.092	2376	2381	2385	rBV	1582742	2244912	37.94%	3.219%
56	17.139	2385	2389	2396	rVV	1032129	1537256	25.98%	2.204%
57	17.227	2400	2404	2409	rVB	344077	474139	8.01%	0.680%
58	18.010	2533	2537	2545	rVB2	632526	897853	15.17%	1.287%
59	18.157	2558	2562	2566	rBV2	357007	514808	8.70%	0.738%
60	19.121	2721	2726	2732	rBV	2676994	3464107	58.55%	4.967%
61	19.474	2782	2786	2789	rBV	2048506	2555432	43.19%	3.664%
62	19.504	2789	2791	2796	rVB	679576	714948	12.08%	1.025%
63	19.680	2816	2821	2831	rVB	4676563	5916749	100.00%	8.483%
64	20.057	2879	2885	2889	rBV4	530909	1169120	19.76%	1.676%
65	20.857	3018	3021	3025	rVB2	916126	1114065	18.83%	1.597%
66	20.933	3031	3034	3041	rVB3	831759	1127466	19.06%	1.617%
67	21.063	3052	3056	3060	rBV2	1360521	1752668	29.62%	2.513%
68	21.127	3064	3067	3070	rVB	979058	1105550	18.69%	1.585%
69	21.204	3075	3080	3084	rVV2	2304487	3991897	67.47%	5.724%
70	21.239	3084	3086	3090	rVB	1089478	1249423	21.12%	1.791%
71	21.845	3186	3189	3195	rVB2	1433730	2167043	36.63%	3.107%
72	21.986	3209	3213	3218	rVB	1625935	2243000	37.91%	3.216%
73	22.827	3352	3356	3361	rBV2	1167472	1892540	31.99%	2.714%
74	23.521	3471	3474	3480	rVB2	1240890	2098335	35.46%	3.009%

Sum of corrected areas: 69745071

Instrument :

BNA_P

ClientSampleId :




SWCS-16-0204

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006881.D
Acq On : 25 Aug 2021 15:30
Operator : CG/JU
Sample : M3463-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-16-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

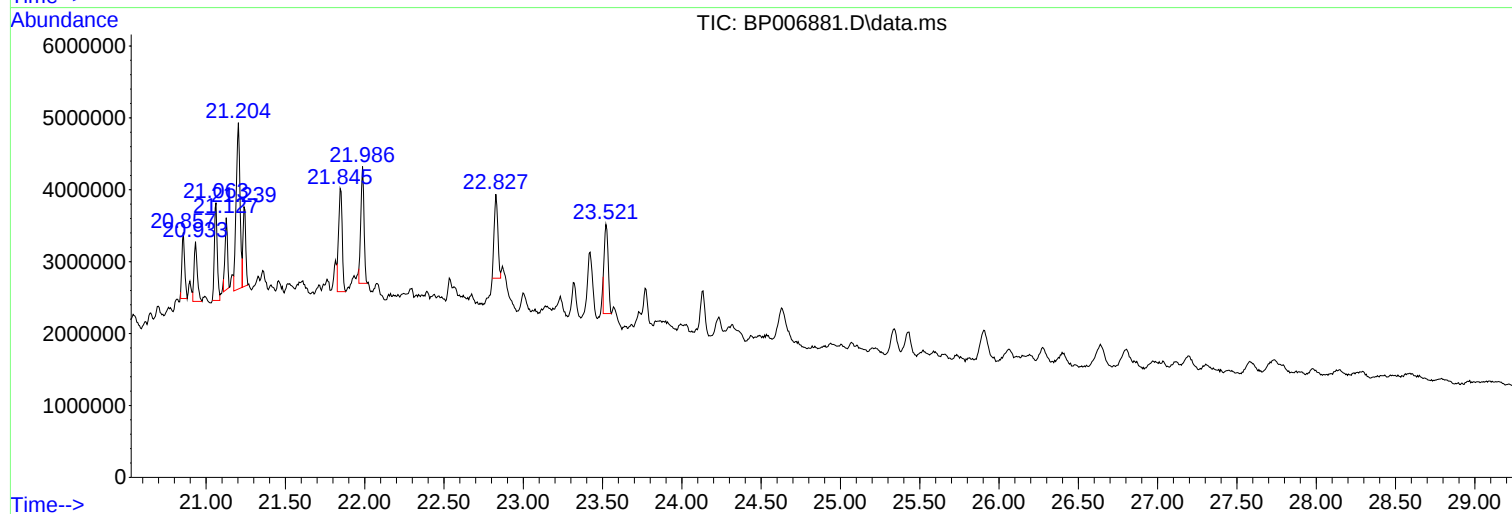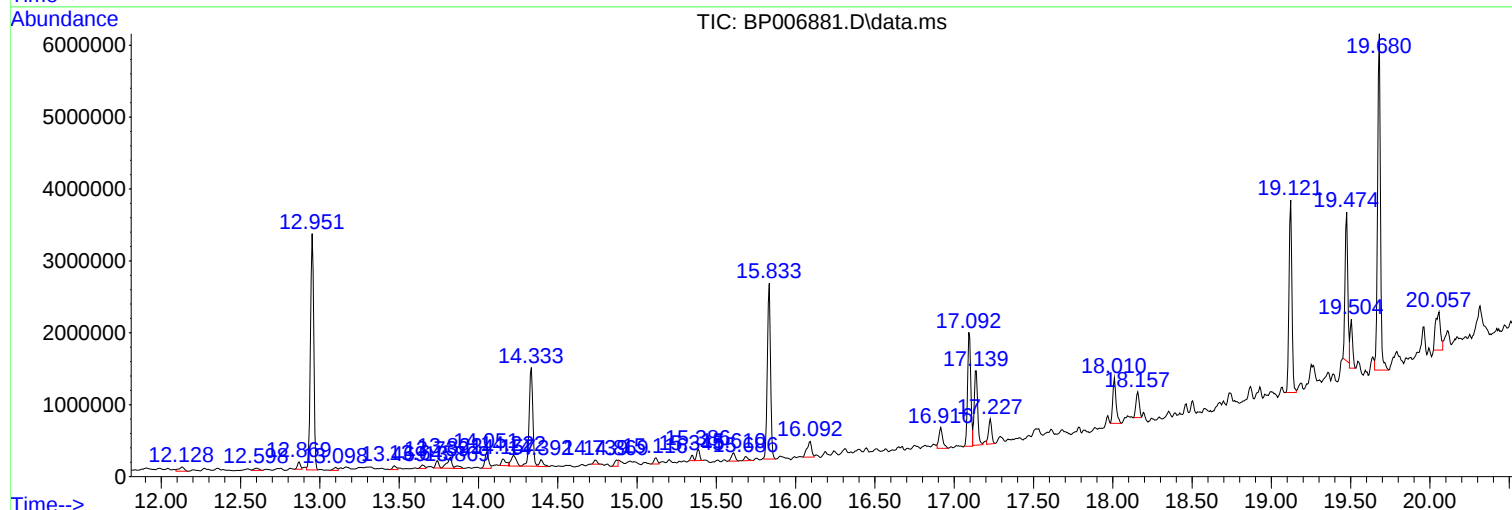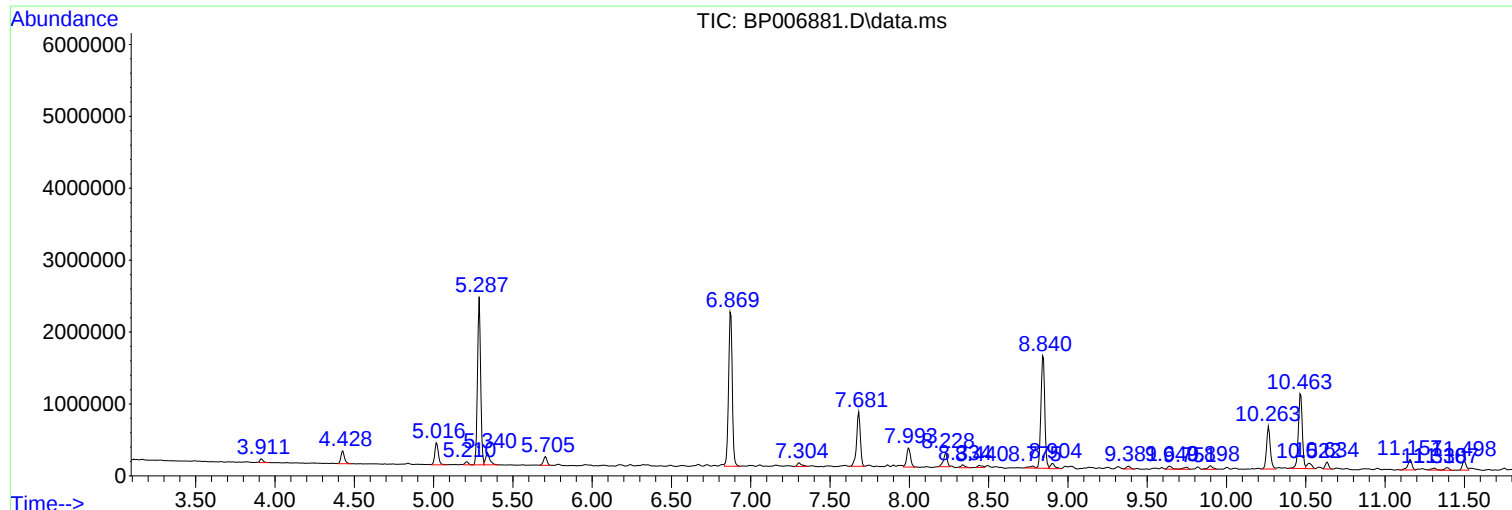

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006881.D
Acq On : 25 Aug 2021 15:30
Operator : CG/JU
Sample : M3463-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-16-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
Data File : BP006881.D
Acq On : 25 Aug 2021 15:30
Operator : CG/JU
Sample : M3463-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SWCS-16-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------