
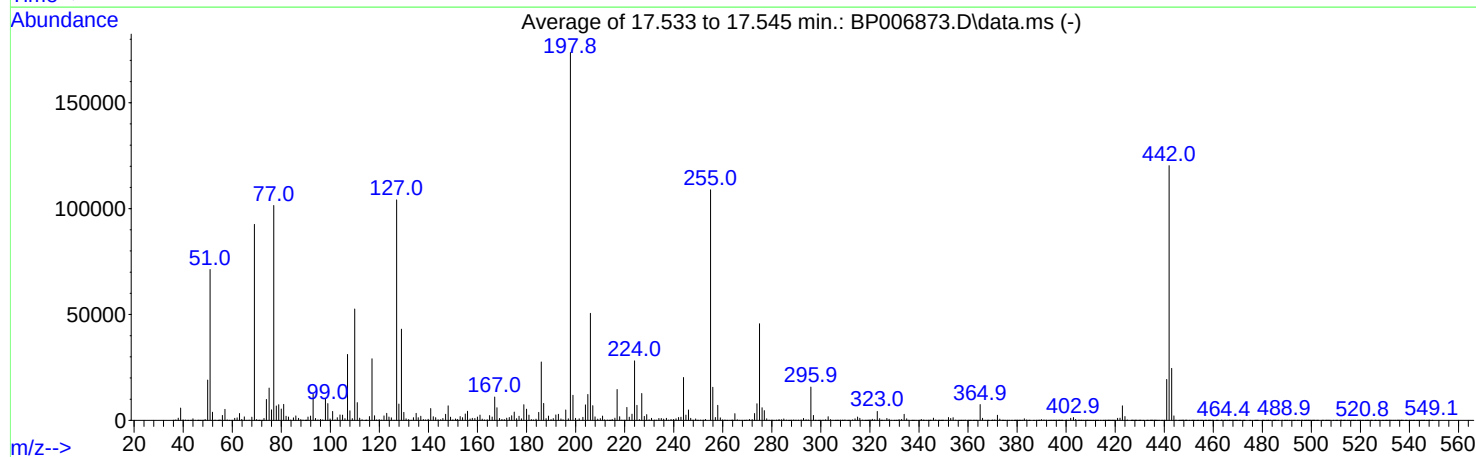


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006873.D
 Acq On : 25 Aug 2021 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 25 11:27:41 2021

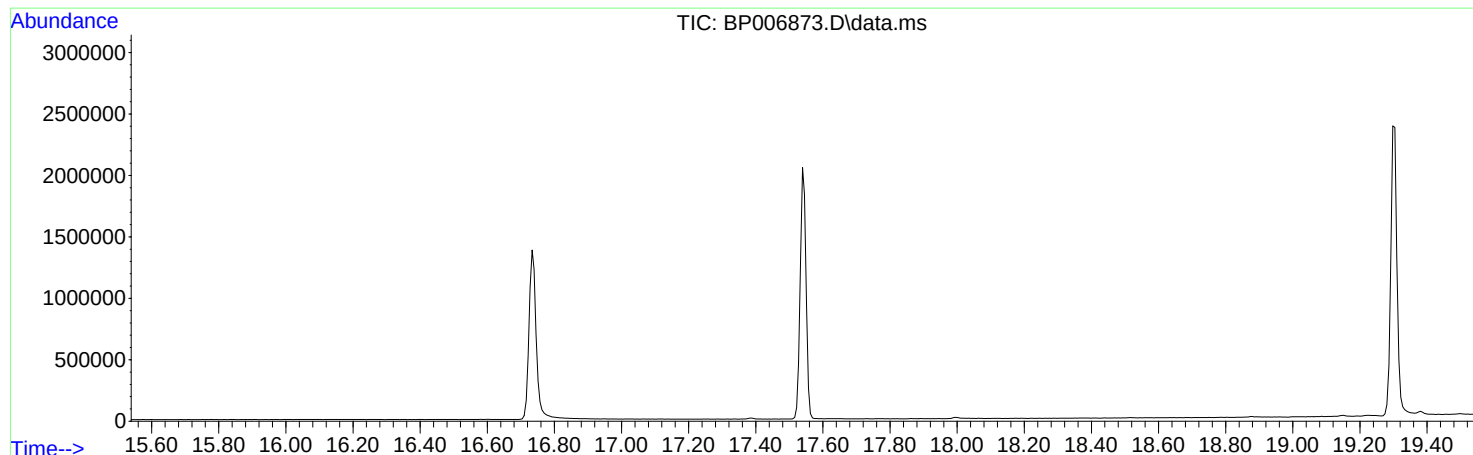




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	71247	PASS
68	69	0.00	2	1.6	1516	PASS
69	198	0.00	100	53.3	92590	PASS
70	69	0.00	2	0.4	393	PASS
127	198	10	80	59.9	104109	PASS
197	198	0.00	2	0.5	784	PASS
198	198	100	100	100.0	173725	PASS
199	198	5	9	6.8	11894	PASS
275	198	10	60	26.3	45627	PASS
365	198	1	100	4.3	7506	PASS
441	198	0.01	100	11.1	19316	PASS
442	442	100	100	100.0	120315	PASS
443	442	15	24	20.4	24565	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006873.D
 Acq On : 25 Aug 2021 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 11:24:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 13:40:38 2021
 Response via : Initial Calibration

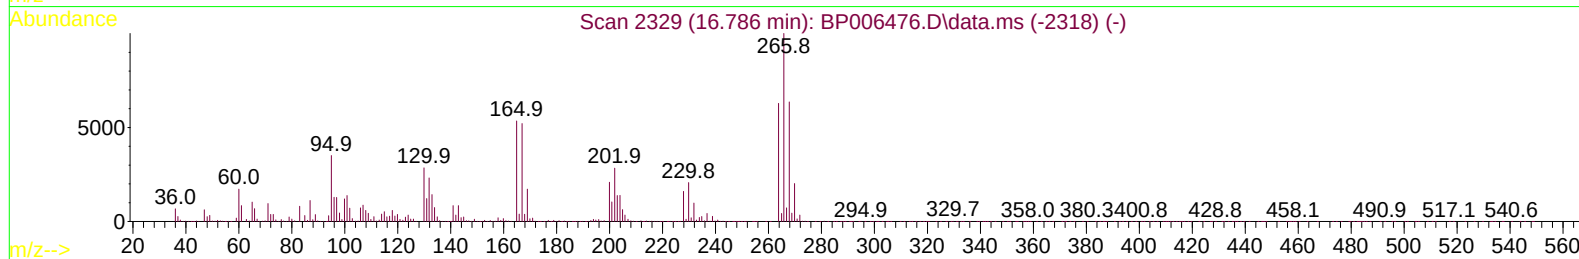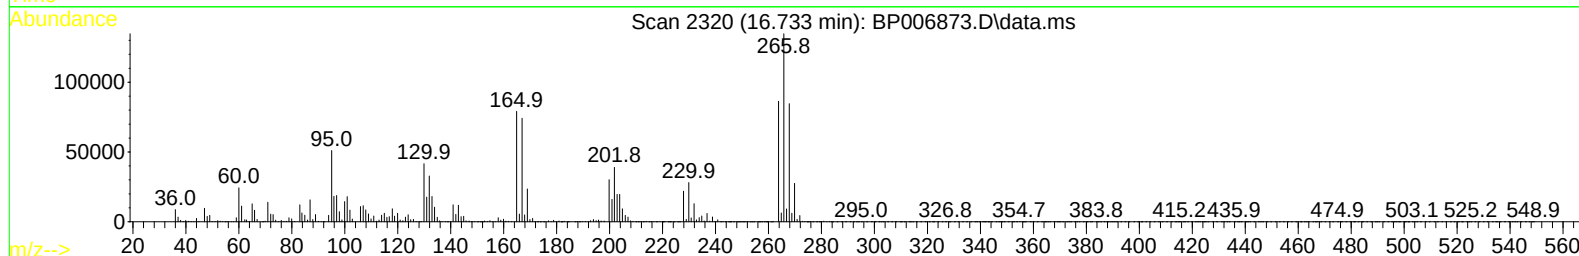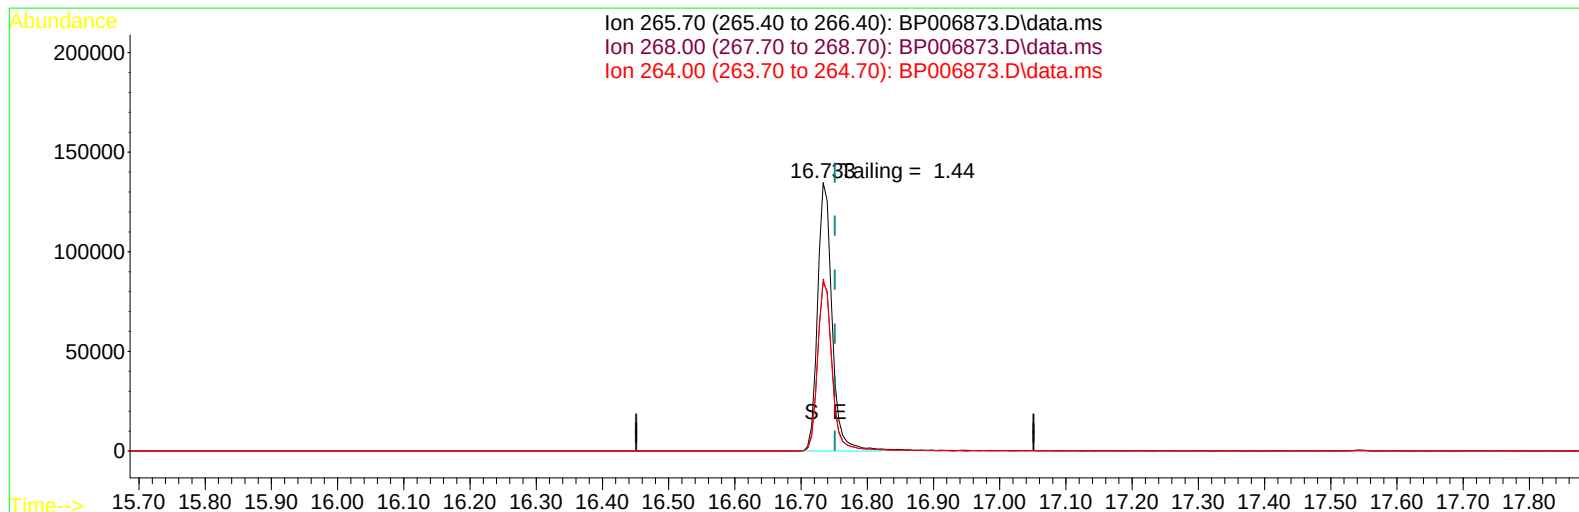

TIC: BP006873.D\data.ms

(70) Pentachlorophenol (C)

16.733min (-0.018) 780121.99 ng




response 205371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.80
264.00	62.90	64.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082521\
 Data File : BP006873.D
 Acq On : 25 Aug 2021 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 11:24:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 13:40:38 2021
 Response via : Initial Calibration

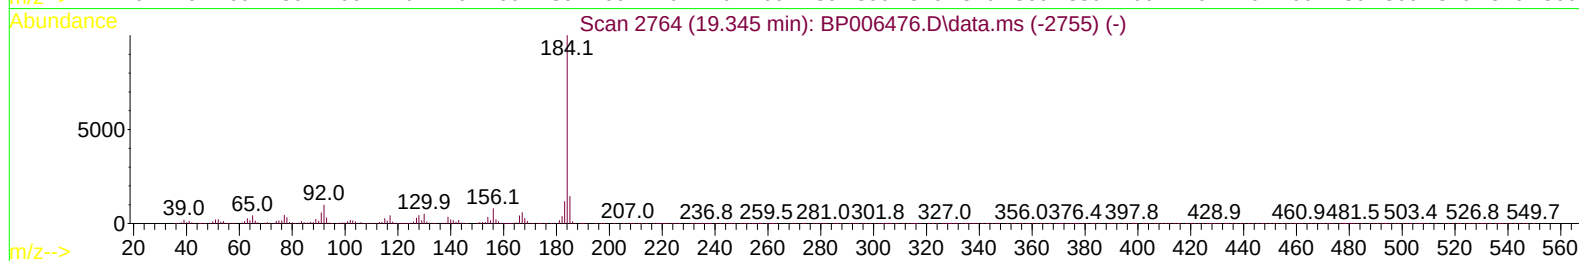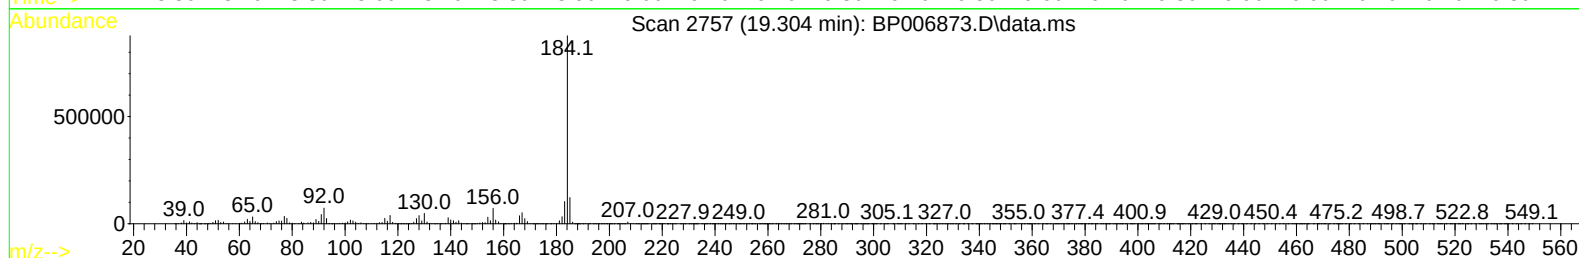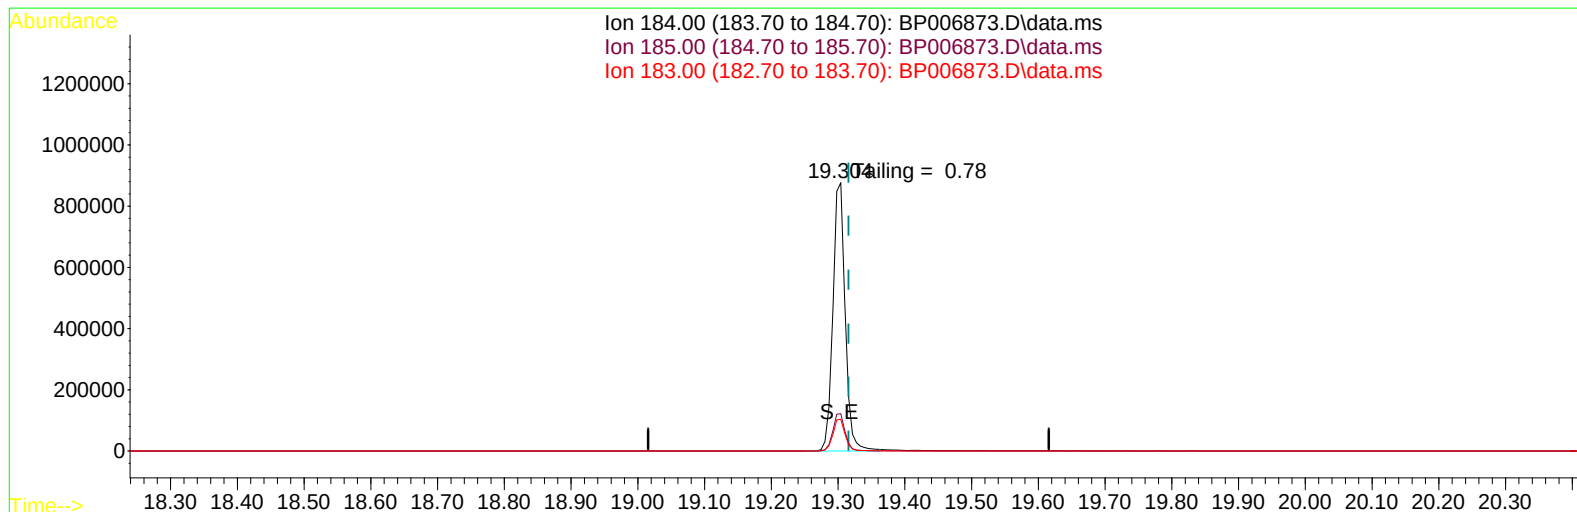

TIC: BP006873.D\data.ms

(77) Benzidine

19.304min (-0.012) 685079.60 ng

response 1131436

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.93
183.00	11.90	11.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2021	BNA_P	<u>BP006873.D</u>
Compound Name	Response	Retention Time
DDT	579305	20.5
DDD	8658	20.07
DDE	1842	19.57
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10500	589805	1.78