

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082622\
 Data File : BP011581.D
 Acq On : 26 Aug 2022 16:12
 Operator : CG/JU
 Sample : PB147286BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB147286BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP082622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP011581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.152	361	368	386	rBV	2901182	3933183	39.97%	10.278%
2	6.740	630	638	650	rBV	2593285	3952801	40.17%	10.330%
3	7.546	767	775	787	rBV	452396	691762	7.03%	1.808%
4	8.716	964	974	989	rBV	1516823	2456086	24.96%	6.418%
5	10.334	1240	1249	1262	rBV	549922	909086	9.24%	2.376%
6	12.834	1667	1674	1690	rBV	3819349	5282196	53.68%	13.804%
7	14.222	1900	1910	1918	rBV	797788	1178515	11.98%	3.080%
8	15.728	2157	2166	2182	rBV	3563041	4900611	49.80%	12.806%
9	16.992	2374	2381	2395	rBV	1034599	1481844	15.06%	3.872%
10	19.592	2817	2823	2828	rBV	8187171	9840409	100.00%	25.715%
11	21.121	3078	3083	3091	rBV	1445332	1796566	18.26%	4.695%
12	23.410	3465	3472	3485	rVB2	950110	1844003	18.74%	4.819%




Sum of corrected areas: 38267062

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082622\
Data File : BP011581.D
Acq On : 26 Aug 2022 16:12
Operator : CG/JU
Sample : PB147286BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147286BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP082622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

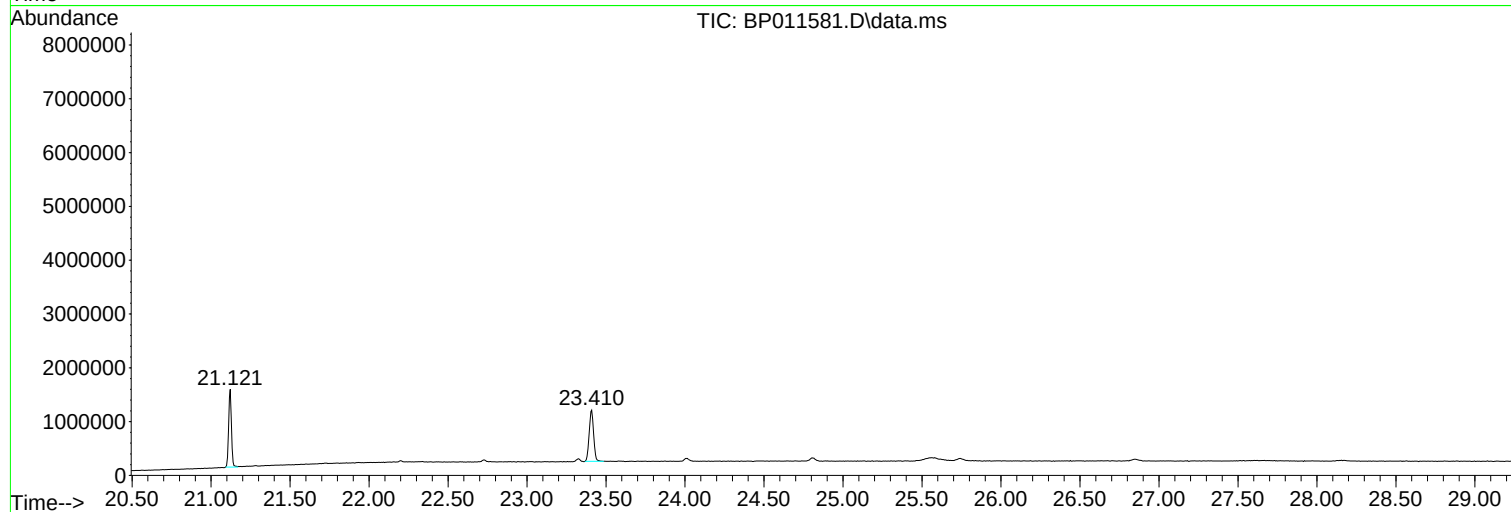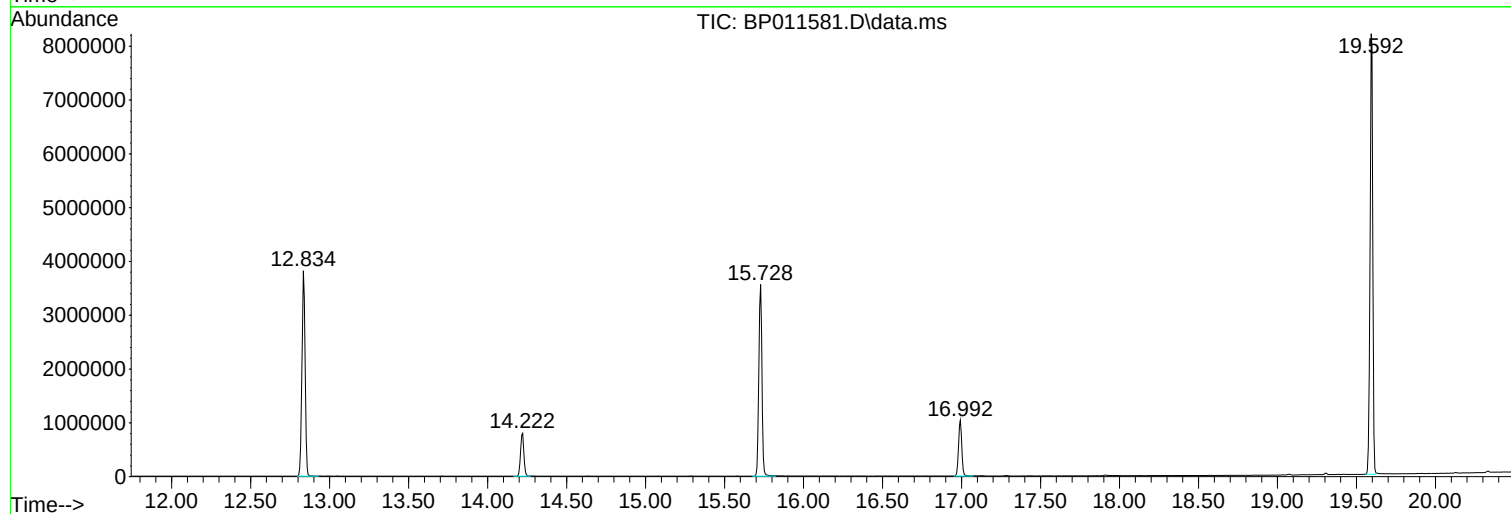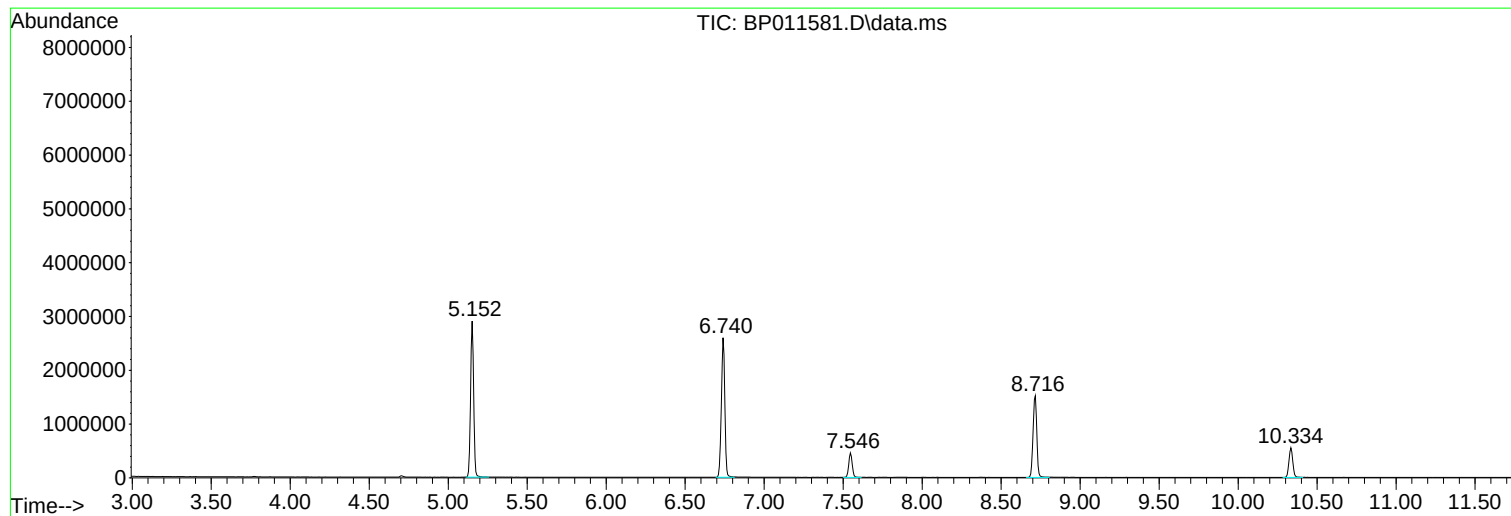

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082622\
Data File : BP011581.D
Acq On : 26 Aug 2022 16:12
Operator : CG/JU
Sample : PB147286BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147286BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP082622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082622\
Data File : BP011581.D
Acq On : 26 Aug 2022 16:12
Operator : CG/JU
Sample : PB147286BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB147286BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP082622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------