


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082622\
 Data File : BP011572.D
 Acq On : 26 Aug 2022 10:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP082622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 27 00:36:07 2022

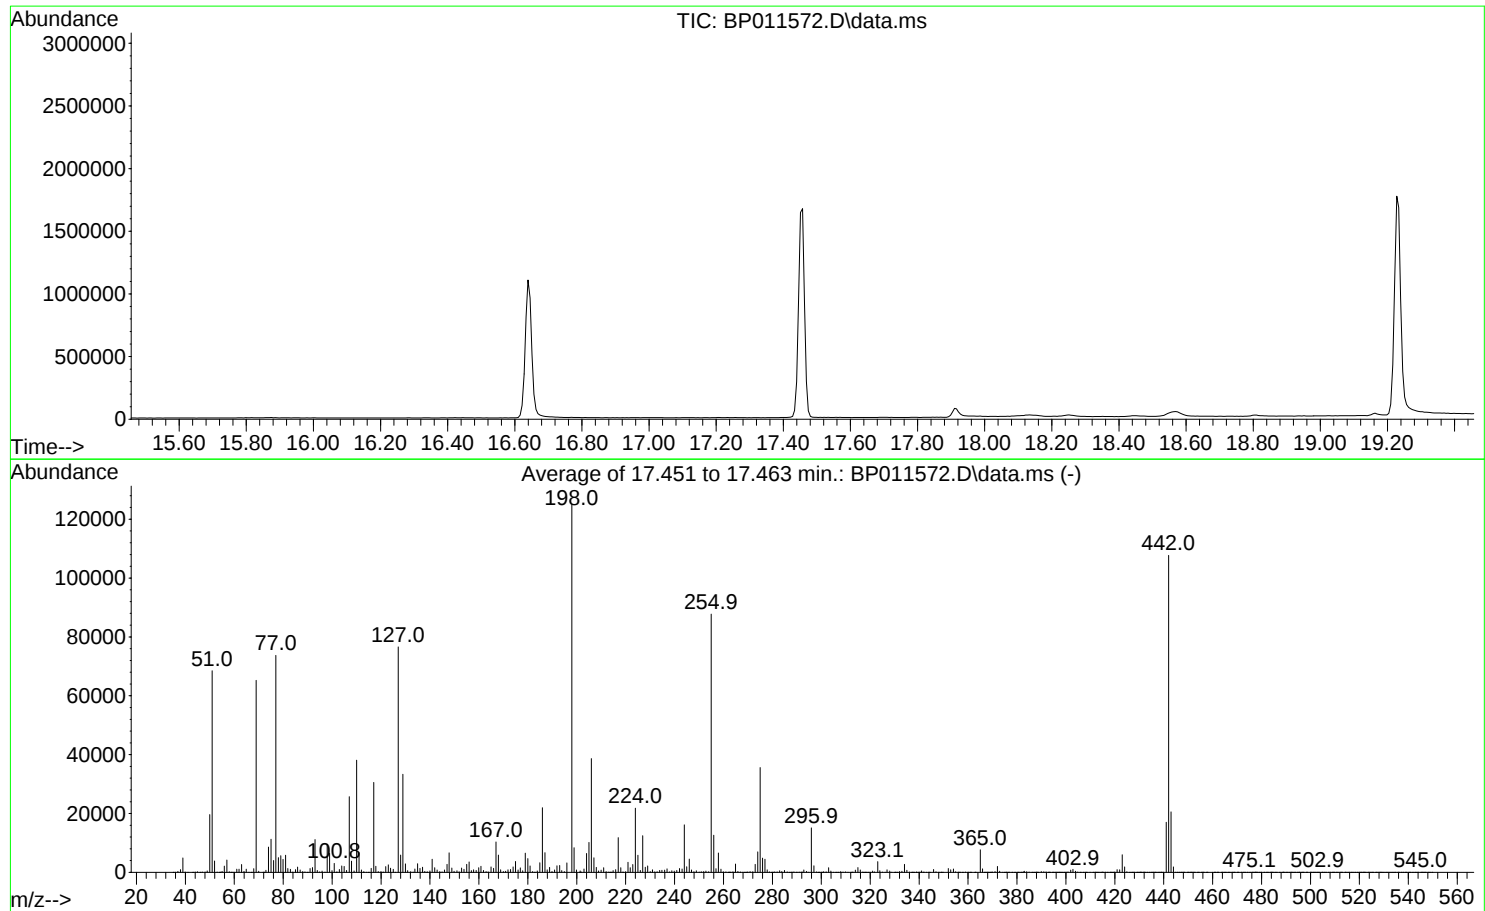

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.8	68528	PASS
68	69	0.00	2	1.9	1251	PASS
69	198	0.00	100	52.2	65253	PASS
70	69	0.00	2	0.6	412	PASS
127	198	10	80	61.3	76629	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	124992	PASS
199	198	5	9	6.7	8404	PASS
275	198	10	60	28.5	35597	PASS
365	198	1	100	6.1	7670	PASS
441	198	0.01	100	13.6	17008	PASS
442	442	100	100	100.0	107721	PASS
443	442	15	24	19.1	20533	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/26/2022	BNA_P	<u>BP011572.D</u>
Compound Name	Response	Retention Time
DDT	474514	20.43
DDD	1959	20
DDE	632	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2591	477105	0.54

Instrument :
BNA_P
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082622\  
Data File : BP011572.D  
Acq On    : 26 Aug 2022  10:05  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 26 15:23:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP082622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 26 15:22:03 2022
Response via : Initial Calibration

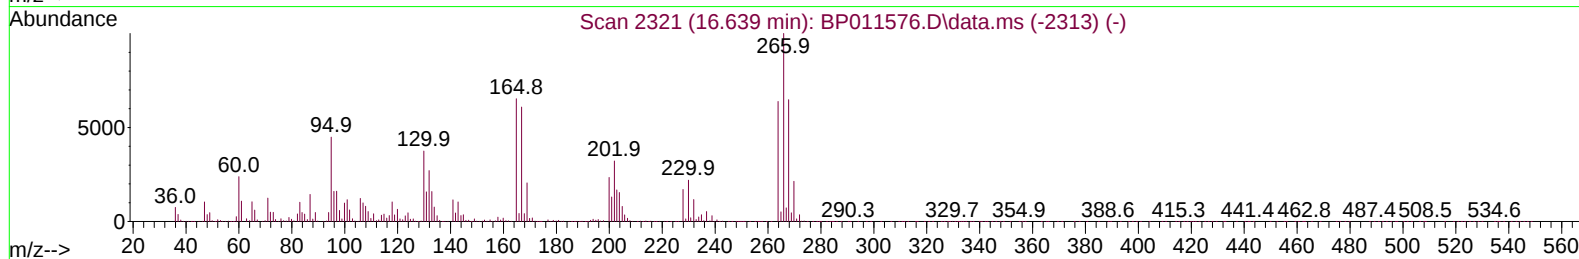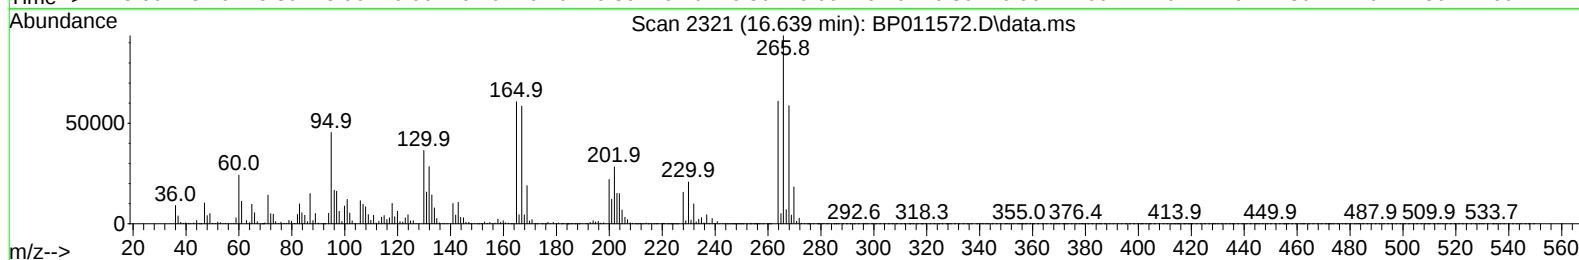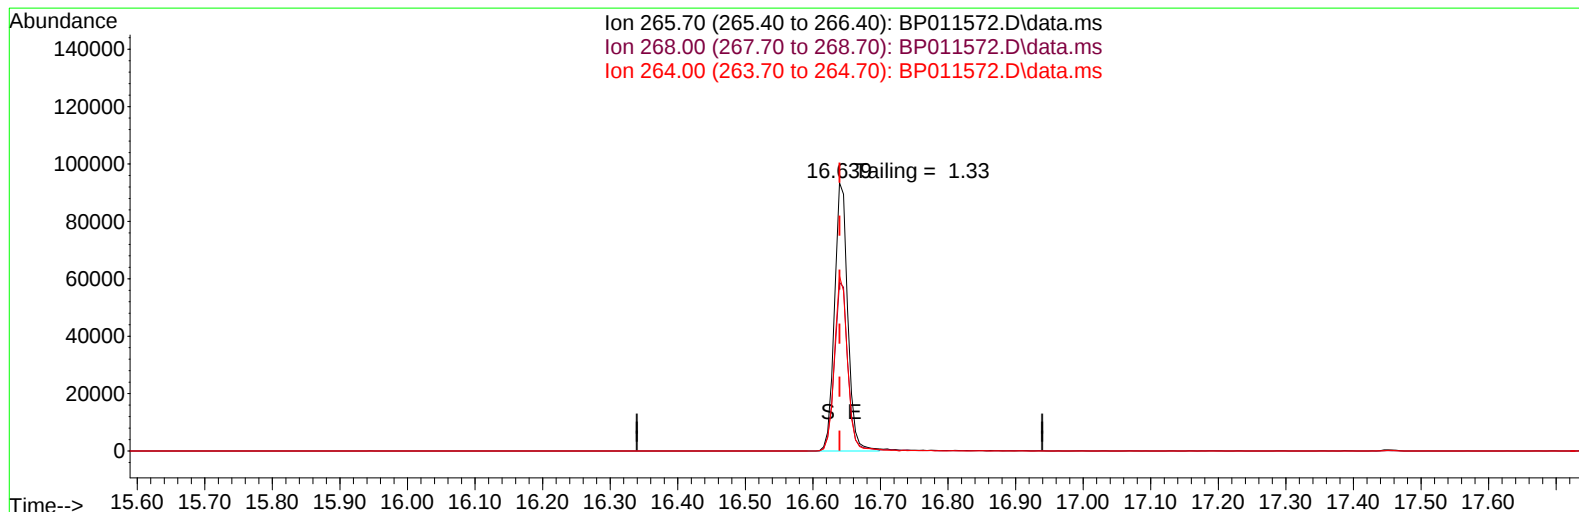

TIC: BP011572.D\data.ms

(70) Pentachlorophenol (C)

16.639min (+ 0.000) 700723.92 ng




response **128742**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.77
264.00	63.00	65.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082622\
 Data File : BP011572.D
 Acq On : 26 Aug 2022 10:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 26 15:23:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP082622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 26 15:22:03 2022
 Response via : Initial Calibration

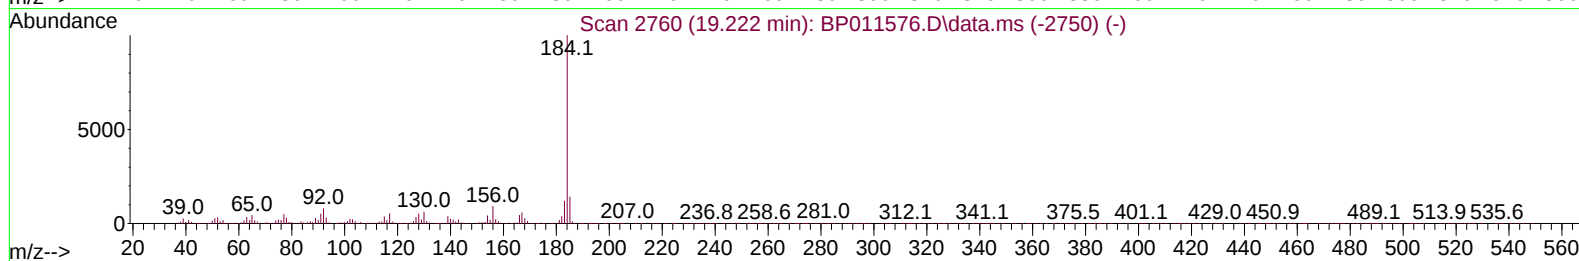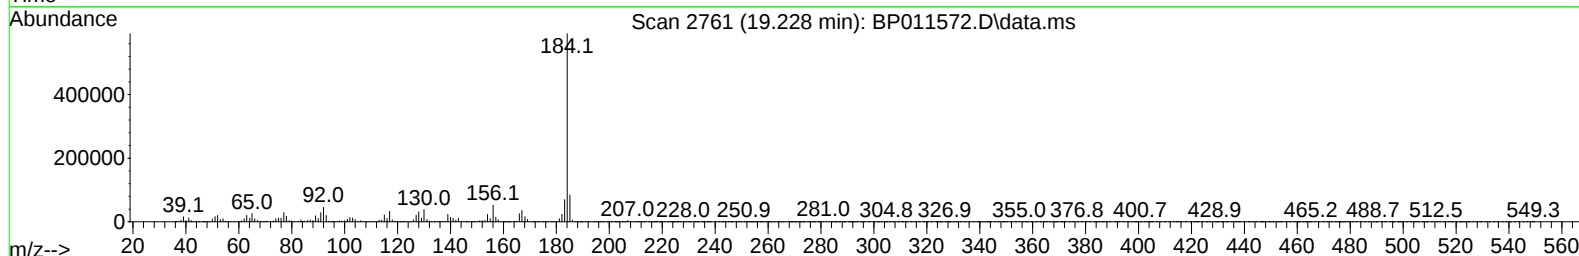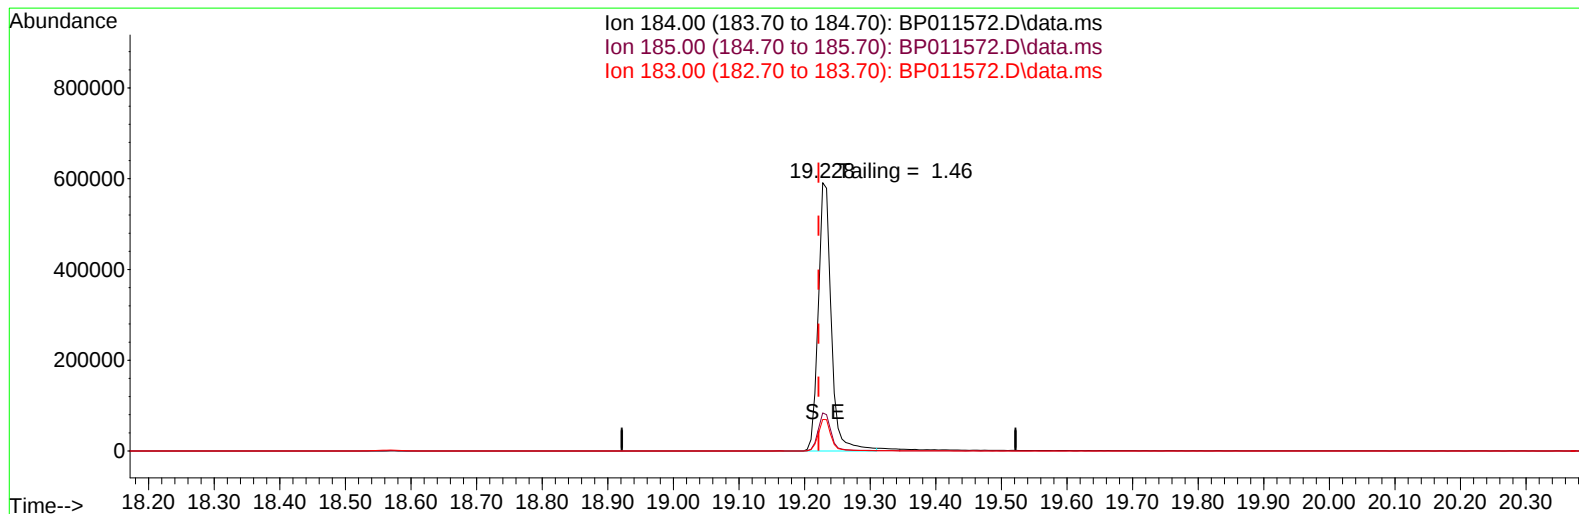

TIC: BP011572.D\data.ms

(77) Benzidine

19.228min (+ 0.006) 651149.23 ng

response 833582

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.18
183.00	11.30	11.78
0.00	0.00	0.00