

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
 Data File : BP021679.D
 Acq On : 27 Aug 2024 20:28
 Operator : RC/JU
 Sample : P3675-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCYE2

Quant Time: Aug 27 22:48:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 27 05:11:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	316102	20.000	ng/ul	0.00
20) Naphthalene-d8	10.581	136	1332571	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.434	164	898354	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	1962265	20.000	ng/ul	-0.02
79) Chrysene-d12	21.680	240	1876327	20.000	ng/ul	-0.01
88) Perylene-d12	25.086	264	2107297	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	22074	2.318	ng/uL	0.00
4) Pyridine-d5	3.687	84	332471	12.072	ng/ul	0.00
7) Phenol-d5	6.957	99	477415	14.152	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	270371	14.727	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	308984	14.187	ng/ul	0.00
15) 4-Methylphenol-d8	8.487	113	356204	13.665	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	154093	14.373	ng/ul	0.00
24) 2-Nitrophenol-d4	9.663	143	154942	14.238	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	312730	14.583	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	463792	14.865	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1080933	15.725	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	1202247	15.578	ng/ul	0.00
54) 4-Nitrophenol-d4	14.628	143	171142	13.086	ng/ul	0.00
60) Fluorene-d10	15.439	176	941538	16.292	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.551	200	87528	8.110	ng/ul	-0.02
73) Anthracene-d10	17.333	188	1492405	16.026	ng/ul	-0.02
81) Pyrene-d10	19.698	212	1844274	17.195	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.845	264	1861587	16.567	ng/ul	-0.03
Target Compounds						
					Qvalue	
55) 4-Nitrophenol	14.645	109	13090	1.093	ng/ul#	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021679.D
Acq On : 27 Aug 2024 20:28
Operator : RC/JU
Sample : P3675-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCYE2

Quant Time: Aug 27 22:48:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 27 05:11:38 2024
Response via : Initial Calibration

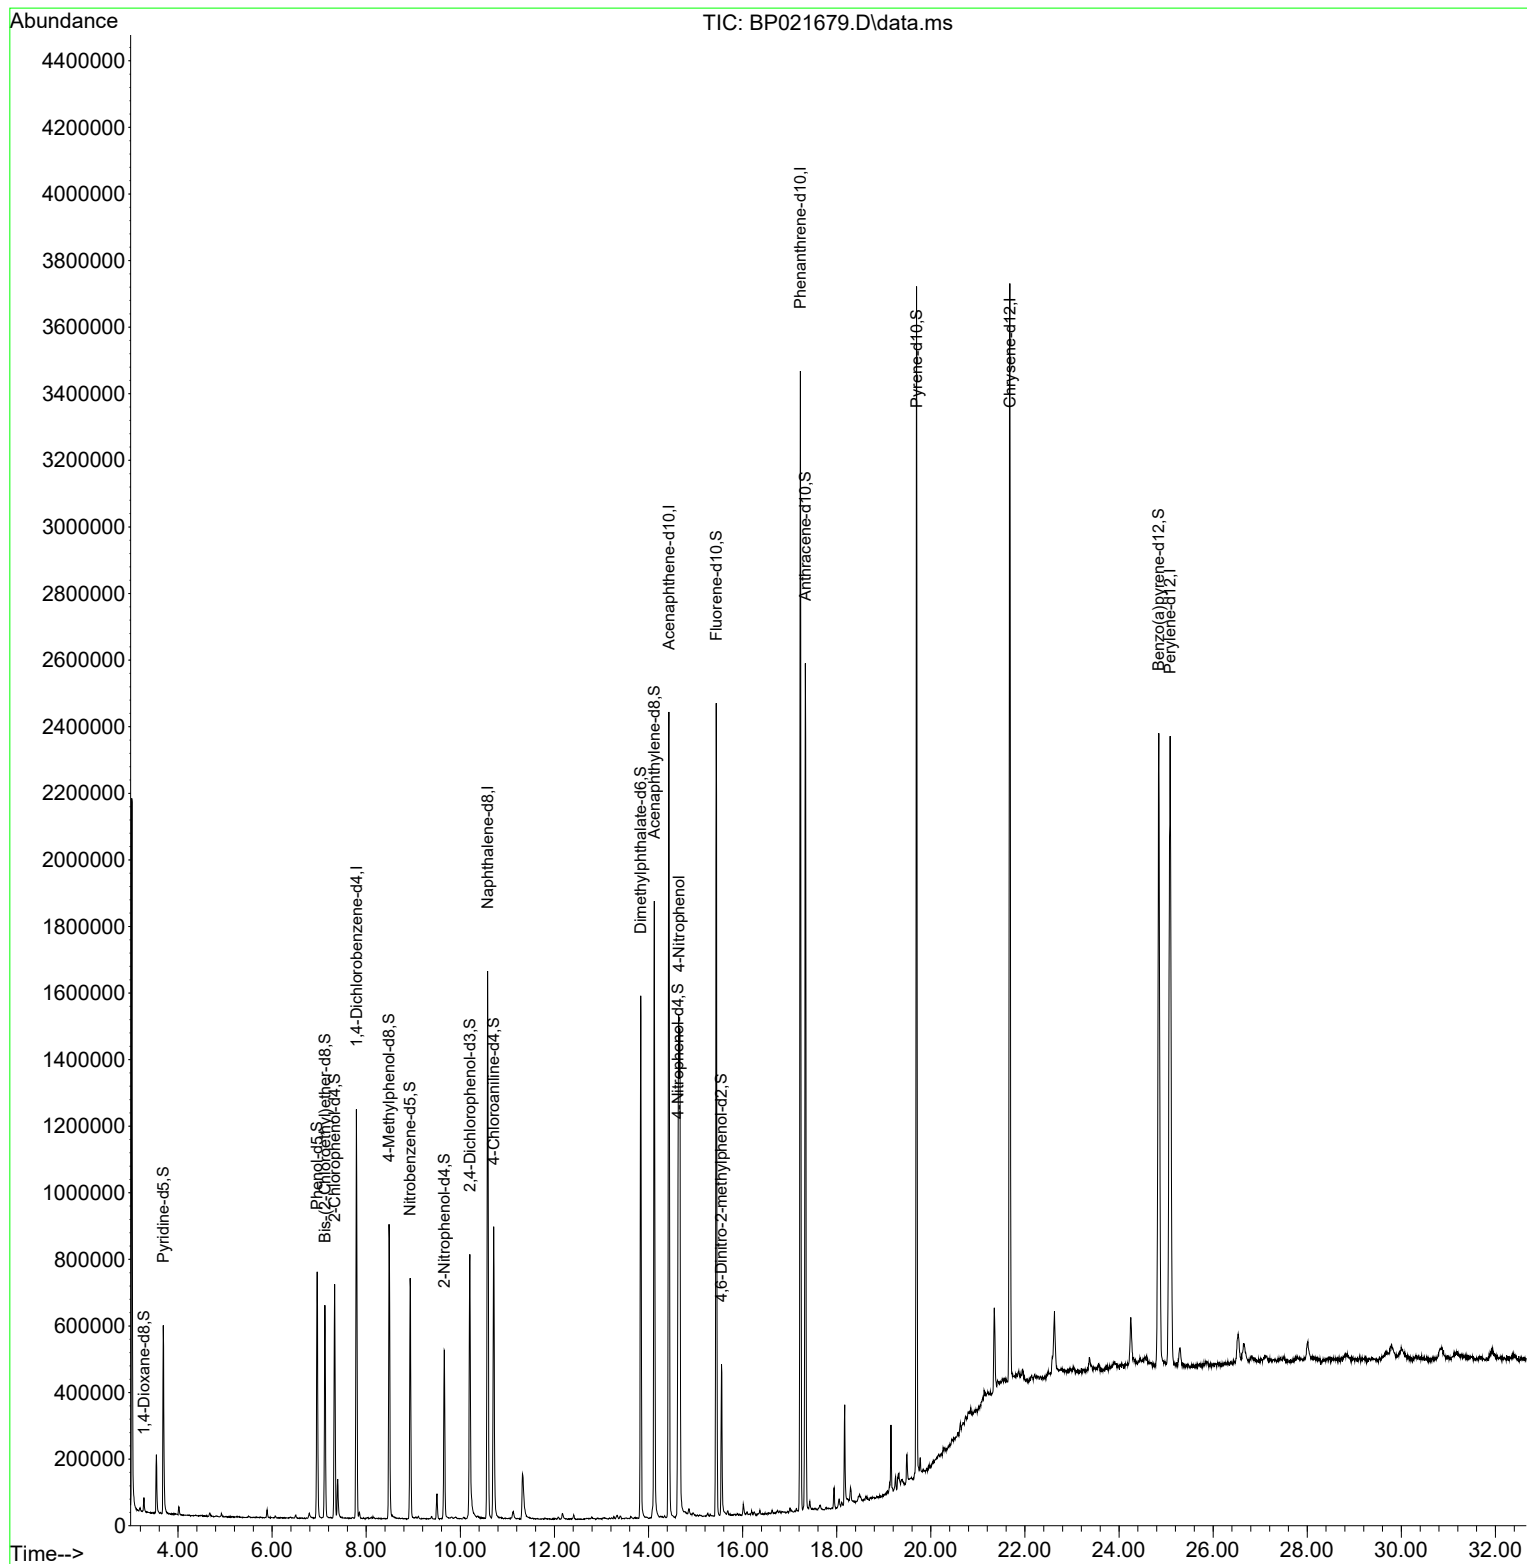

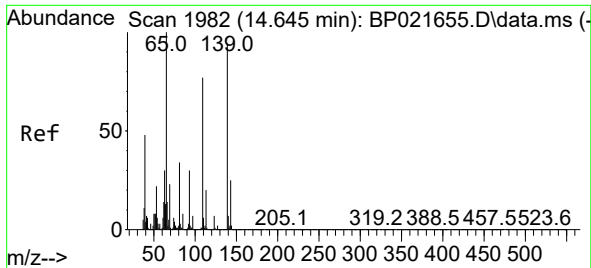

#55
 4-Nitrophenol
 Concen: 1.093 ng/ul
 RT: 14.645 min Scan# 1982
 Delta R.T. 0.000 min
 Lab File: BP021679.D
 Acq: 27 Aug 2024 20:28

Instrument :
 BNA_P
 ClientSampleId :
 DCYE2

Tgt Ion:109 Resp: 13090
 Ion Ratio Lower Upper
 109 100
 139 11.3 96.2 144.2#
 65 30.5 98.5 147.7#

