

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
 Data File : BP021681.D
 Acq On : 27 Aug 2024 21:56
 Operator : RC/JU
 Sample : P3675-18
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCXZ2

Quant Time: Aug 27 22:49:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 27 05:11:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	374314	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	1560746	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.434	164	1014781	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.222	188	2166050	20.000	ng/ul	-0.03
79) Chrysene-d12	21.675	240	2171705	20.000	ng/ul	-0.02
88) Perylene-d12	25.092	264	2463087	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	29878	2.650	ng/uL	0.00
4) Pyridine-d5	3.687	84	351432	10.776	ng/ul	0.00
7) Phenol-d5	6.958	99	554330	13.877	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	335556	15.435	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	387402	15.021	ng/ul	0.00
15) 4-Methylphenol-d8	8.487	113	299831	9.713	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	194997	15.529	ng/ul	0.00
24) 2-Nitrophenol-d4	9.658	143	193063	15.147	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.199	165	388012	15.448	ng/ul	0.00
31) 4-Chloroaniline-d4	10.705	131	413256	11.309	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1250698	16.107	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	1431231	16.417	ng/ul	0.00
54) 4-Nitrophenol-d4	14.628	143	172731	11.693	ng/ul	0.00
60) Fluorene-d10	15.440	176	1107211	16.961	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.551	200	117371	9.852	ng/ul	-0.02
73) Anthracene-d10	17.328	188	1772231	17.240	ng/ul	-0.02
81) Pyrene-d10	19.692	212	2190141	17.642	ng/ul	-0.03
92) Benzo(a)pyrene-d12	24.857	264	2319063	17.657	ng/ul	-0.02
Target Compounds						Qvalue
55) 4-Nitrophenol	14.646	109	23635	1.747	ng/ul#	9


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021681.D
Acq On : 27 Aug 2024 21:56
Operator : RC/JU
Sample : P3675-18
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCXZ2


Quant Time: Aug 27 22:49:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 27 05:11:38 2024
Response via : Initial Calibration

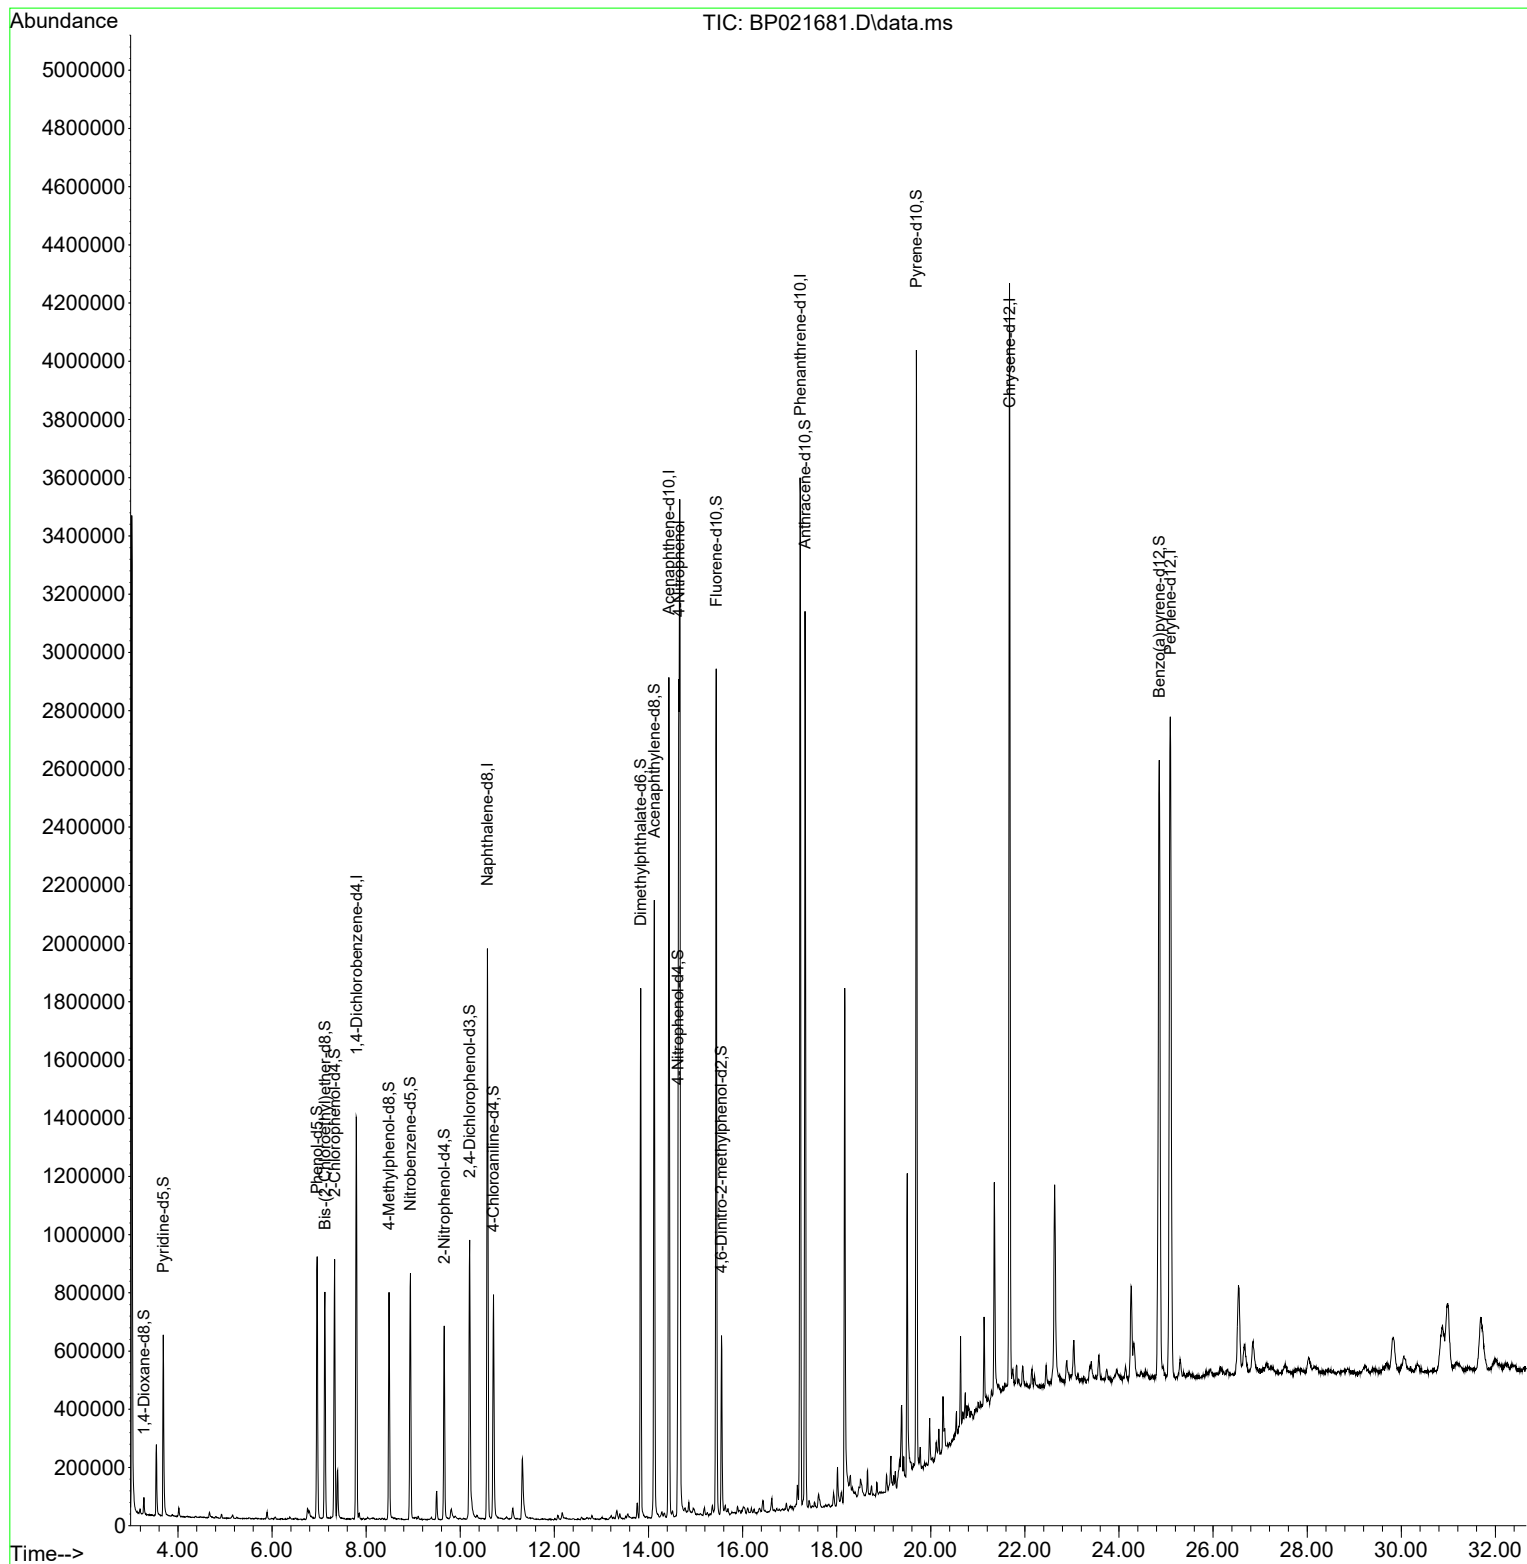

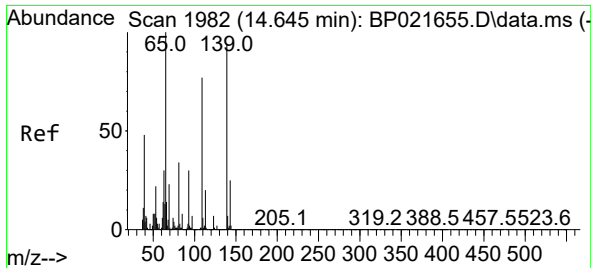

#55
4-Nitrophenol
Concen: 1.747 ng/ul
RT: 14.646 min Scan# 1982
Delta R.T. 0.000 min
Lab File: BP021681.D
Acq: 27 Aug 2024 21:56

Instrument :
BNA_P
ClientSampleId :
DCXZ2

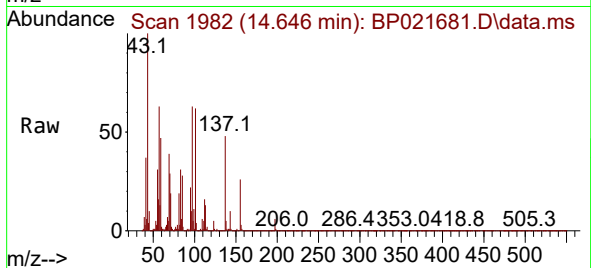

Tgt Ion:109 Resp: 23635
Ion Ratio Lower Upper
109 100
139 12.3 96.2 144.2#
65 27.3 98.5 147.7#

