

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
 Data File : BP021699.D
 Acq On : 28 Aug 2024 11:45
 Operator : RC/JU
 Sample : P3697-04DL 100X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCN88DL

Quant Time: Aug 28 12:39:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 27 05:11:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	361083	20.000	ng/u1	0.00
20) Naphthalene-d8	10.581	136	1499007	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.440	164	953889	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.234	188	2027571	20.000	ng/u1	-0.02
79) Chrysene-d12	21.686	240	1979139	20.000	ng/u1	0.00
88) Perylene-d12	25.098	264	2226282	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	5613	0.516	ng/uL	0.00
4) Pyridine-d5	3.693	84	22197	0.706	ng/u1	0.00
7) Phenol-d5	6.964	99	60999	1.583	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	74376	3.547	ng/u1	0.00
11) 2-Chlorophenol-d4	7.328	132	87830	3.530	ng/u1	0.00
15) 4-Methylphenol-d8	8.505	113	86791	2.915	ng/u1	0.01
21) Nitrobenzene-d5	8.940	128	39503	3.276	ng/u1	0.00
24) 2-Nitrophenol-d4	9.658	143	40336	3.295	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	84616	3.508	ng/u1	0.02
31) 4-Chloroaniline-d4	10.710	131	46808	1.334	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	273019	3.741	ng/u1	0.00
49) Acenaphthylene-d8	14.128	160	295553	3.607	ng/u1	0.00
54) 4-Nitrophenol-d4	14.651	143	15729	1.133	ng/u1	0.02
60) Fluorene-d10	15.440	176	241935	3.943	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.563	200	22243	1.995	ng/u1	0.00
73) Anthracene-d10	17.328	188	375948	3.907	ng/u1	-0.02
81) Pyrene-d10	19.698	212	486882	4.304	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.851	264	445845	3.756	ng/u1	-0.02
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.881	266	2051707	120.643	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021699.D
Acq On : 28 Aug 2024 11:45
Operator : RC/JU
Sample : P3697-04DL 100X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCN88DL

Quant Time: Aug 28 12:39:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 27 05:11:38 2024
Response via : Initial Calibration

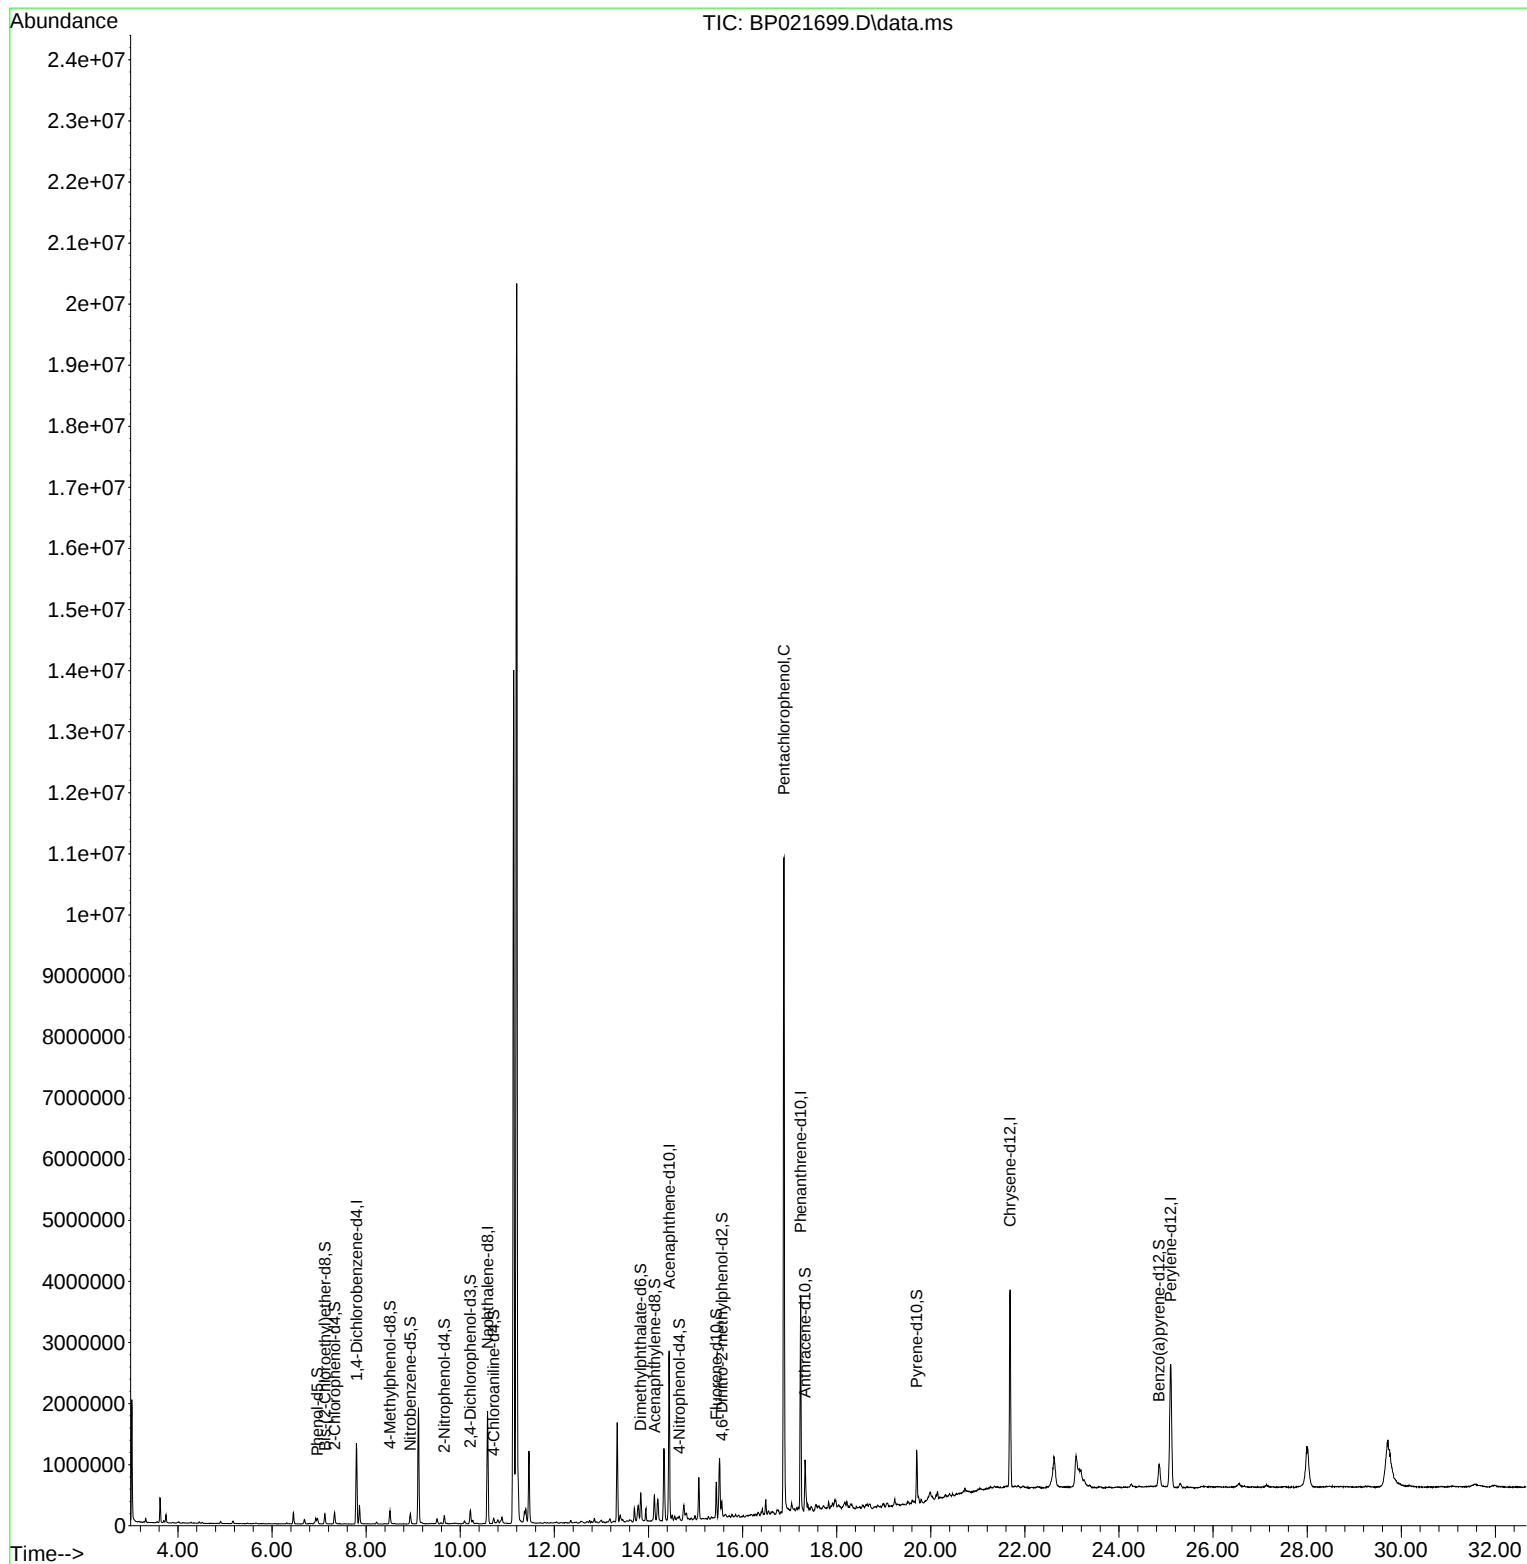

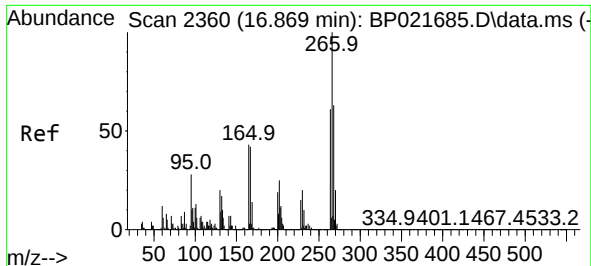

#71
 Pentachlorophenol
 Concen: 120.643 ng/ul
 RT: 16.881 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP021699.D
 Acq: 28 Aug 2024 11:45

Instrument :
 BNA_P
 ClientSampleId :
 GCN88DL

Tgt Ion:266 Resp: 2051707
 Ion Ratio Lower Upper
 266 100
 264 63.9 51.4 77.0
 268 64.1 50.6 75.8

