

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
 Data File : BP021643.D
 Acq On : 26 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3336-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.023	3	6	24	rVB	10739844	13282326	100.00%	21.199%
2	3.276	45	49	55	rVB	28920	38402	0.29%	0.061%
3	3.546	90	95	105	rBV	30366	50466	0.38%	0.081%
4	3.699	117	121	128	rBV2	19298	27840	0.21%	0.044%
5	3.793	133	137	142	rVB	35529	50022	0.38%	0.080%
6	4.017	172	175	183	rVB	18469	27180	0.20%	0.043%
7	4.928	324	330	335	rBV	25828	40378	0.30%	0.064%
8	5.028	340	347	352	rVB5	11821	23758	0.18%	0.038%
9	6.081	518	526	532	rBV5	8163	19931	0.15%	0.032%
10	6.793	640	647	654	rBV5	8613	21149	0.16%	0.034%
11	6.958	668	675	685	rBV	334049	572305	4.31%	0.913%
12	7.122	692	703	711	rBV	353589	563279	4.24%	0.899%
13	7.328	732	738	747	rBV	348229	568531	4.28%	0.907%
14	7.793	810	817	824	rBV	895837	1457178	10.97%	2.326%
15	8.487	928	935	946	rBV	390886	657834	4.95%	1.050%
16	8.611	950	956	961	rVB	43743	79687	0.60%	0.127%
17	8.940	1004	1012	1020	rVV	349750	624841	4.70%	0.997%
18	9.022	1023	1026	1037	rVB6	11577	27238	0.21%	0.043%
19	9.505	1099	1108	1116	rBV5	38894	74885	0.56%	0.120%
20	9.658	1128	1134	1142	rBV	242158	423574	3.19%	0.676%
21	10.205	1219	1227	1246	rVB	331295	715480	5.39%	1.142%
22	10.581	1282	1291	1298	rBV	1175740	2162905	16.28%	3.452%
23	10.710	1305	1313	1321	rBV	282246	544980	4.10%	0.870%
24	11.122	1375	1383	1388	rBV	11951	22246	0.17%	0.036%
25	11.322	1411	1417	1429	rBV2	44740	117947	0.89%	0.188%
26	11.487	1440	1445	1456	rVB9	17516	47565	0.36%	0.076%
27	11.622	1463	1468	1473	rBV5	18521	39301	0.30%	0.063%
28	12.022	1530	1536	1541	rBV2	20813	40397	0.30%	0.064%
29	12.246	1569	1574	1582	rVB3	22481	45447	0.34%	0.073%
30	12.463	1605	1611	1615	rBV3	12623	20412	0.15%	0.033%
31	12.840	1670	1675	1680	rBV7	11235	22218	0.17%	0.035%
32	12.981	1694	1699	1704	rVV5	22074	33603	0.25%	0.054%
33	13.269	1743	1748	1753	rBV2	36984	53471	0.40%	0.085%
34	13.616	1801	1807	1814	rVB9	10349	21048	0.16%	0.034%
35	13.751	1825	1830	1834	rVV3	17840	28470	0.21%	0.045%
36	13.840	1835	1845	1856	rVV	881091	1272134	9.58%	2.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
 Data File : BP021643.D
 Acq On : 26 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3336-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

37	13.934	1857	1861	1865	rVV2	40303	54919	0.41%	0.088%
38	13.993	1865	1871	1878	rVB8	16411	40718	0.31%	0.065%
39	14.128	1885	1894	1906	rBV	911739	1528005	11.50%	2.439%
40	14.351	1927	1932	1937	rBV2	39859	54568	0.41%	0.087%
41	14.440	1939	1947	1955	rBV	1951198	2970346	22.36%	4.741%
42	14.634	1974	1980	1991	rBV3	205399	477008	3.59%	0.761%
43	14.734	1993	1997	2001	rVV	33523	62381	0.47%	0.100%
44	14.787	2001	2006	2010	rVV6	20551	42644	0.32%	0.068%
45	14.846	2011	2016	2024	rVV	43695	106119	0.80%	0.169%
46	14.916	2026	2028	2032	rVV4	14928	22992	0.17%	0.037%
47	14.981	2034	2039	2047	rVV10	19060	46874	0.35%	0.075%
48	15.069	2049	2054	2059	rVV5	14075	27254	0.21%	0.043%
49	15.245	2078	2084	2087	rBV4	23526	47151	0.35%	0.075%
50	15.316	2092	2096	2101	rVV	34963	43846	0.33%	0.070%
51	15.445	2111	2118	2124	rBV	1313760	1900491	14.31%	3.033%
52	15.504	2124	2128	2132	rVB4	32486	54126	0.41%	0.086%
53	15.563	2132	2138	2146	rBV	277842	393433	2.96%	0.628%
54	15.734	2163	2167	2173	rVB4	32954	53854	0.41%	0.086%
55	15.816	2175	2181	2188	rVV6	20904	40719	0.31%	0.065%
56	15.893	2190	2194	2198	rBV7	13445	24102	0.18%	0.038%
57	15.951	2201	2204	2212	rVV3	32487	63586	0.48%	0.101%
58	16.022	2214	2216	2223	rVB7	15067	26909	0.20%	0.043%
59	16.151	2234	2238	2241	rBV5	13406	22699	0.17%	0.036%
60	16.198	2242	2246	2248	rVV4	57995	88140	0.66%	0.141%
61	16.234	2248	2252	2258	rVB	146997	246117	1.85%	0.393%
62	16.334	2265	2269	2273	rBV7	12130	23239	0.17%	0.037%
63	16.781	2338	2345	2349	rBV3	33442	85312	0.64%	0.136%
64	16.887	2359	2363	2371	rVB2	33803	56416	0.42%	0.090%
65	16.969	2373	2377	2381	rBV4	25245	47333	0.36%	0.076%
66	17.016	2381	2385	2388	rVB	46816	57912	0.44%	0.092%
67	17.239	2417	2423	2428	rBV	2451997	3679090	27.70%	5.872%
68	17.287	2428	2431	2435	rVV	217316	291608	2.20%	0.465%
69	17.345	2435	2441	2445	rVV2	1316020	2224206	16.75%	3.550%
70	17.381	2445	2447	2453	rVV	285447	340498	2.56%	0.543%
71	17.439	2453	2457	2463	rVB6	29809	50734	0.38%	0.081%
72	17.569	2474	2479	2484	rBV7	24281	40729	0.31%	0.065%
73	17.657	2488	2494	2498	rBV	75029	123652	0.93%	0.197%
74	17.781	2512	2515	2522	rVB3	54192	74771	0.56%	0.119%
75	18.145	2575	2577	2579	rBV	20462	23102	0.17%	0.037%
76	18.181	2579	2583	2592	rVB2	203372	352148	2.65%	0.562%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
 Data File : BP021643.D
 Acq On : 26 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3336-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

77	18.281	2597	2600	2606	rVV	54186	80749	0.61%	0.129%
78	18.339	2606	2610	2614	rVV2	62014	115163	0.87%	0.184%
79	18.381	2615	2617	2622	rVB2	48707	55918	0.42%	0.089%
80	18.498	2634	2637	2642	rVB	49831	53820	0.41%	0.086%
81	18.657	2662	2664	2667	rVV2	24678	30755	0.23%	0.049%
82	18.692	2667	2670	2677	rVB2	58118	100230	0.75%	0.160%
83	19.092	2733	2738	2744	rBV4	70361	137699	1.04%	0.220%
84	19.151	2745	2748	2753	rBV4	69906	116611	0.88%	0.186%
85	19.239	2760	2763	2766	rBV	69410	101856	0.77%	0.163%
86	19.363	2779	2784	2793	rVB	1019958	1411745	10.63%	2.253%
87	19.504	2805	2808	2816	rBV4	87412	154785	1.17%	0.247%
88	19.710	2837	2843	2846	rBV	1717090	2474768	18.63%	3.950%
89	19.928	2877	2880	2886	rBV	82423	127484	0.96%	0.203%
90	20.092	2903	2908	2918	rBV5	135505	360366	2.71%	0.575%
91	20.222	2926	2930	2931	rBV2	114817	152013	1.14%	0.243%
92	20.369	2951	2955	2958	rBV	107747	152993	1.15%	0.244%
93	20.428	2961	2965	2970	rVB3	183144	298424	2.25%	0.476%
94	20.845	3032	3036	3045	rBV10	116997	297052	2.24%	0.474%
95	21.057	3068	3072	3079	rVB	202947	332165	2.50%	0.530%
96	21.339	3117	3120	3122	rBV	125772	173995	1.31%	0.278%
97	21.692	3171	3180	3185	rBV3	2762704	6265904	47.17%	10.001%
98	21.739	3185	3188	3198	rVB	1101968	1923387	14.48%	3.070%
99	24.021	3568	3576	3585	rBV2	968634	3281958	24.71%	5.238%
100	25.104	3752	3760	3771	rVB	1699653	4726626	35.59%	7.544%




Sum of corrected areas: 62654645

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021643.D
Acq On : 26 Aug 2024 18:04
Operator : RC/JU
Sample : P3336-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

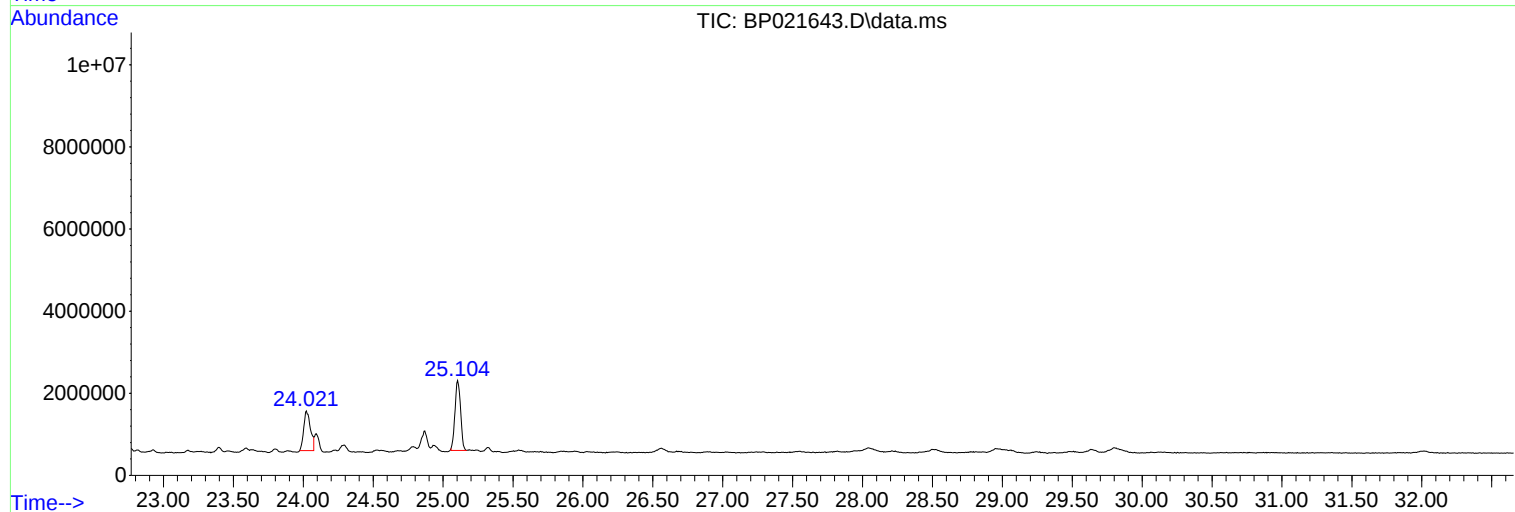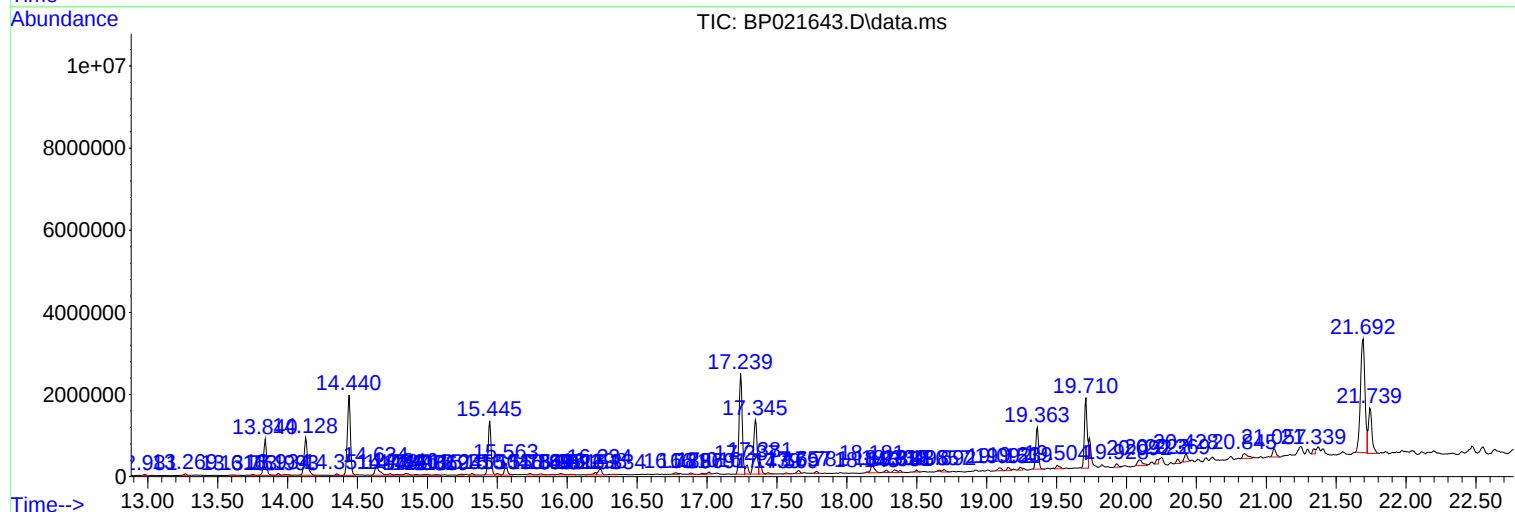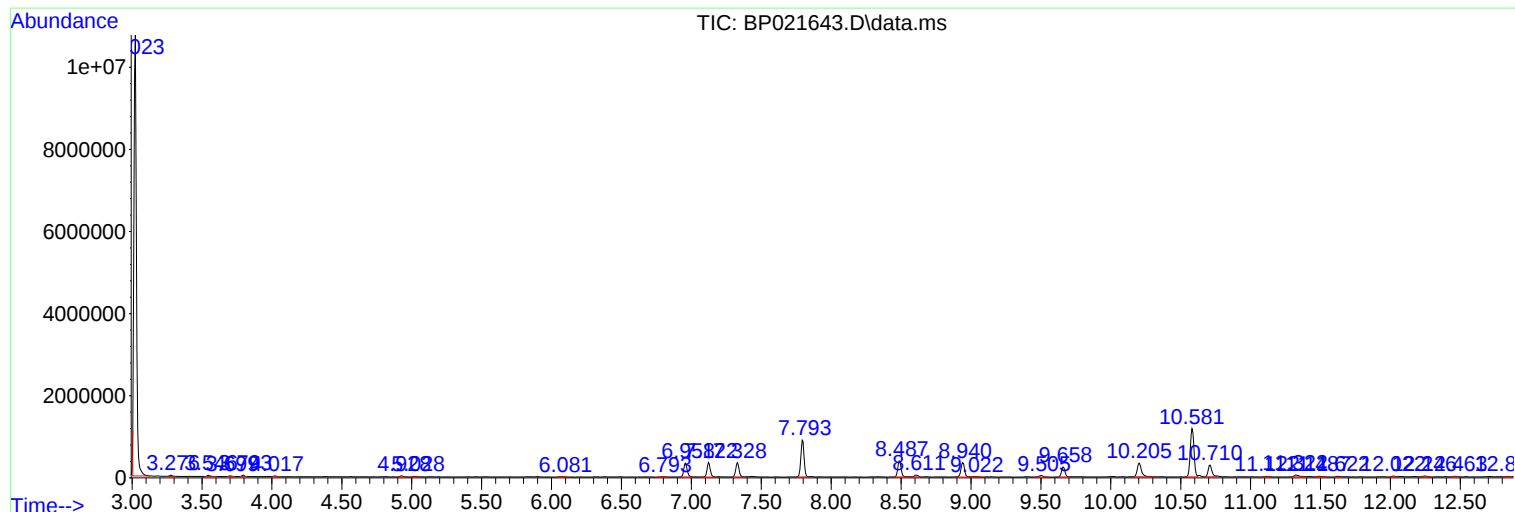

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021643.D
Acq On : 26 Aug 2024 18:04
Operator : RC/JU
Sample : P3336-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E43










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.023	182.30 ng/ul	13282300	1,4-Dichlorobenzene-d4	7.793

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

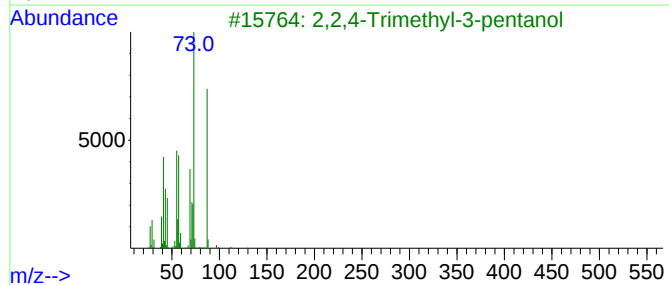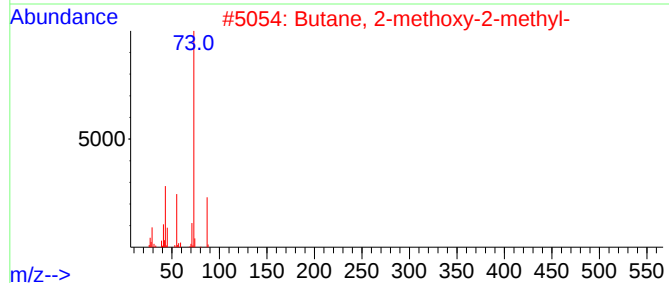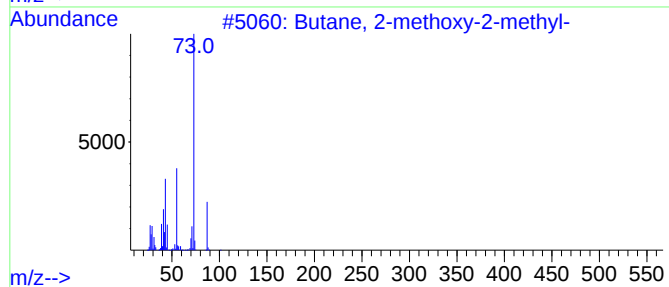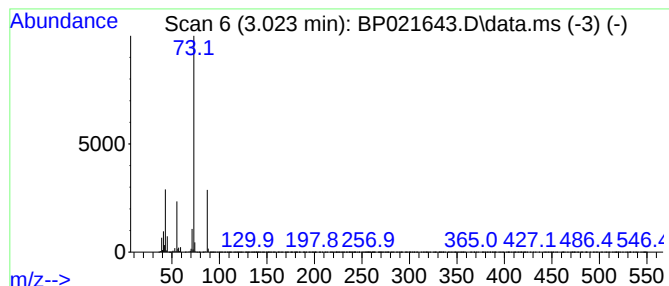

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021643.D
Acq On : 26 Aug 2024 18:04
Operator : RC/JU
Sample : P3336-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.023	182.3	ng/ul	13282300	1	7.793	1457180	20.0