

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
 Data File : BP021666.D
 Acq On : 27 Aug 2024 11:05
 Operator : RC/JU
 Sample : P3711-12
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E24A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.023	3	6	30	rVB	12643629	16091140	100.00%	15.230%
2	3.281	45	50	61	rVB	71885	106437	0.66%	0.101%
3	3.693	116	120	135	rBV	434971	635766	3.95%	0.602%
4	4.022	173	176	185	rVB	24016	31897	0.20%	0.030%
5	4.811	306	310	317	rVB2	15575	24951	0.16%	0.024%
6	4.934	326	331	338	rVB2	24850	42689	0.27%	0.040%
7	6.069	519	524	532	rVB2	36904	58551	0.36%	0.055%
8	6.958	667	675	685	rBV	442243	711348	4.42%	0.673%
9	7.122	692	703	714	rBV	1084395	1782885	11.08%	1.687%
10	7.328	730	738	751	rBV	1130708	1872728	11.64%	1.772%
11	7.793	810	817	826	rBV	1273349	2094669	13.02%	1.983%
12	8.158	874	879	887	rBV6	11765	22039	0.14%	0.021%
13	8.493	928	936	944	rBV	1132659	1970895	12.25%	1.865%
14	8.940	1004	1012	1022	rBV	1260752	2049961	12.74%	1.940%
15	9.657	1125	1134	1146	rBV	977848	1590398	9.88%	1.505%
16	10.204	1216	1227	1254	rBV	1333513	2578340	16.02%	2.440%
17	10.581	1283	1291	1300	rBV	1756460	3063967	19.04%	2.900%
18	10.704	1304	1312	1334	rBV	1400800	2556385	15.89%	2.420%
19	11.381	1420	1427	1434	rBV	7418	19422	0.12%	0.018%
20	11.716	1475	1484	1493	rBV3	12392	31191	0.19%	0.030%
21	12.175	1551	1562	1570	rBV3	25105	59819	0.37%	0.057%
22	12.410	1595	1602	1609	rVB	20360	32674	0.20%	0.031%
23	13.840	1838	1845	1858	rBV	2882691	4400163	27.35%	4.165%
24	14.122	1883	1893	1910	rBV	3042507	4752319	29.53%	4.498%
25	14.434	1937	1946	1970	rBV	2799285	4440667	27.60%	4.203%
26	14.628	1973	1979	1995	rBV	338720	671007	4.17%	0.635%
27	14.857	2014	2018	2024	rBV9	15309	27122	0.17%	0.026%
28	15.445	2110	2118	2131	rBV	4238414	6652461	41.34%	6.296%
29	15.563	2131	2138	2155	rVV	1416352	2029591	12.61%	1.921%
30	15.687	2155	2159	2166	rVB4	23768	43302	0.27%	0.041%
31	17.245	2416	2424	2433	rBV	3721181	5465170	33.96%	5.173%
32	17.345	2434	2441	2452	rVV2	5010456	7928338	49.27%	7.504%
33	17.628	2485	2489	2497	rBV8	7879	16738	0.10%	0.016%
34	18.181	2578	2583	2591	rBV2	65943	113635	0.71%	0.108%
35	19.263	2763	2767	2773	rVB3	65045	94232	0.59%	0.089%
36	19.339	2775	2780	2784	rBV	80662	117844	0.73%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021666.D
Acq On : 27 Aug 2024 11:05
Operator : RC/JU
Sample : P3711-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Title : SVOA CALIBRATION

37	19.510	2805	2809	2814	rBV2	71059	88040	0.55%	0.083%
38	19.716	2838	2844	2853	rVB2	6220358	9534576	59.25%	9.024%
39	21.692	3174	3180	3188	rVB2	3770583	6037052	37.52%	5.714%
40	24.880	3711	3722	3736	rVB	3017559	9557690	59.40%	9.046%
41	25.110	3751	3761	3776	rVB	2051439	6257345	38.89%	5.922%




Sum of corrected areas: 105655444

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021666.D
Acq On : 27 Aug 2024 11:05
Operator : RC/JU
Sample : P3711-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

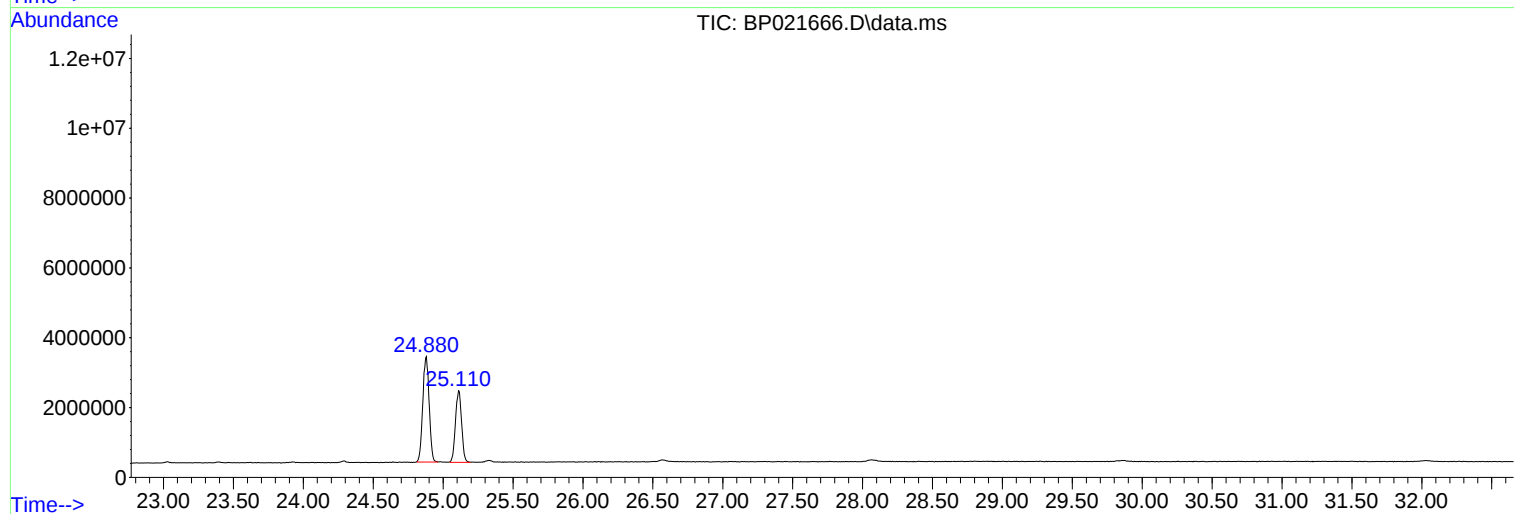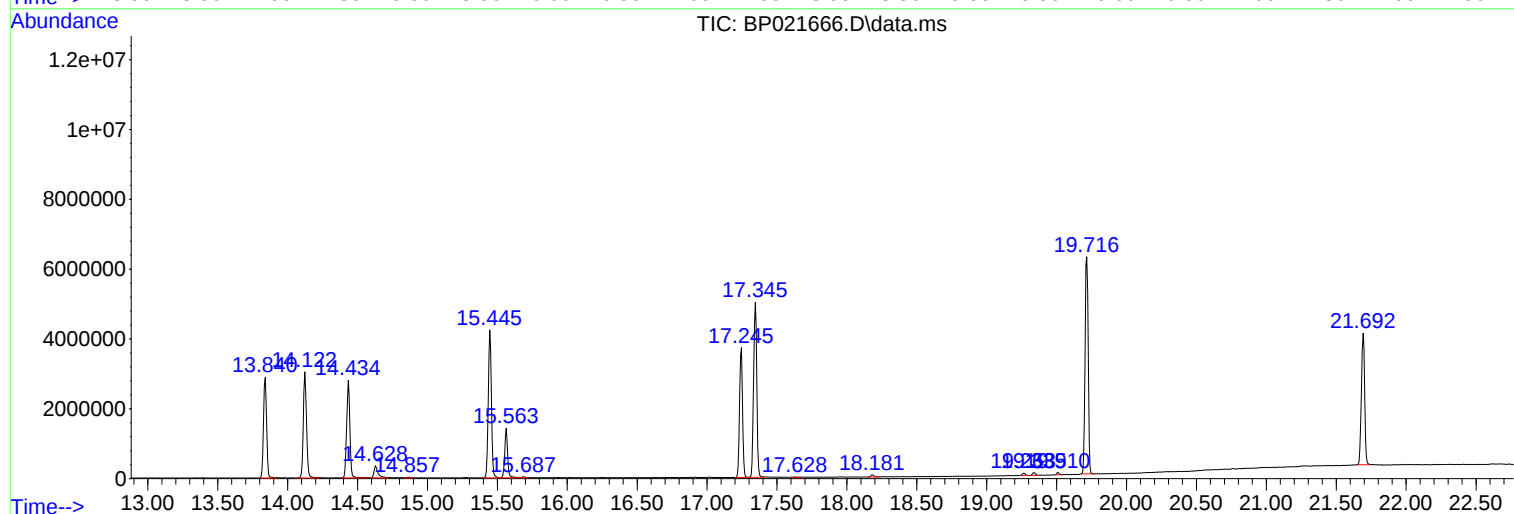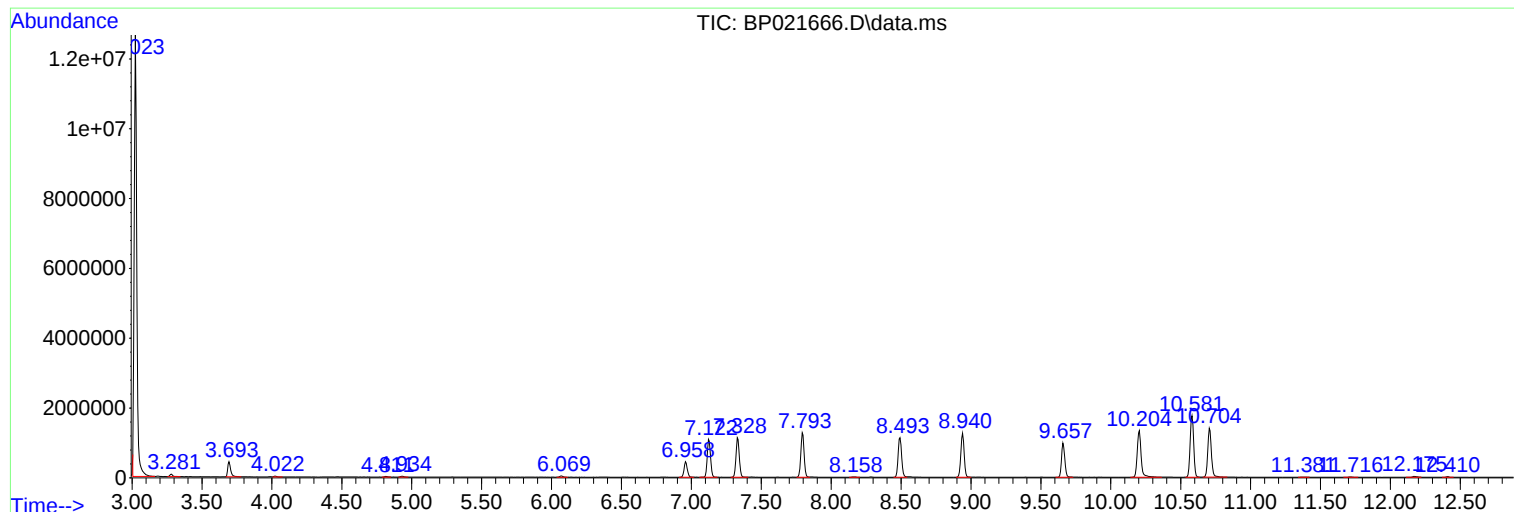

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021666.D
Acq On : 27 Aug 2024 11:05
Operator : RC/JU
Sample : P3711-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.023	153.64 ng/ul	16091100	1,4-Dichlorobenzene-d4	7.793

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	74		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23		
5	Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9		

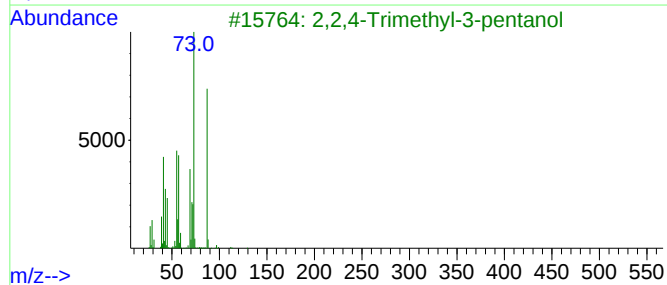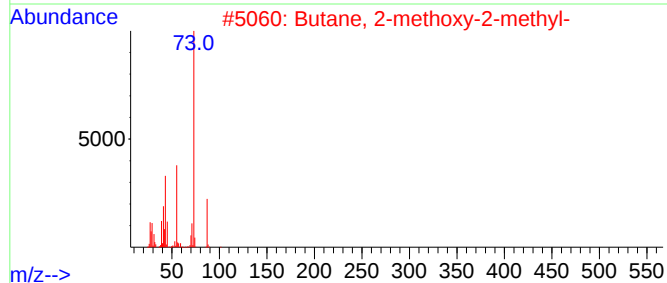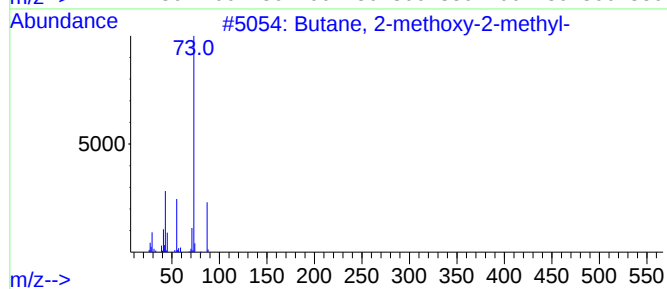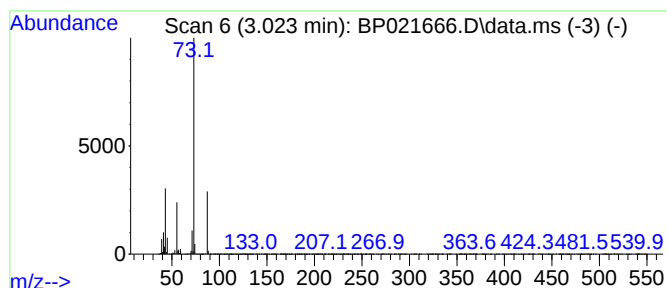

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082624\
Data File : BP021666.D
Acq On : 27 Aug 2024 11:05
Operator : RC/JU
Sample : P3711-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.023	153.6	ng/ul	16091100	1	7.793	2094670	20.0