




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021741.D
Acq On : 30 Aug 2024 05:02
Operator : RC/JU
Sample : P3711-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A7

Manual IntegrationsAPPROVED

Quant Time: Aug 30 05:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/30/2024
Supervised By :mohammad ahmed 09/02/2024

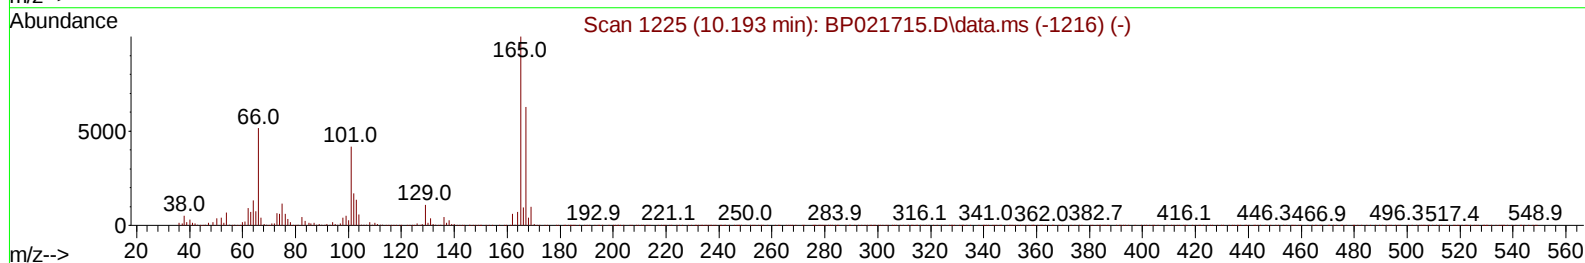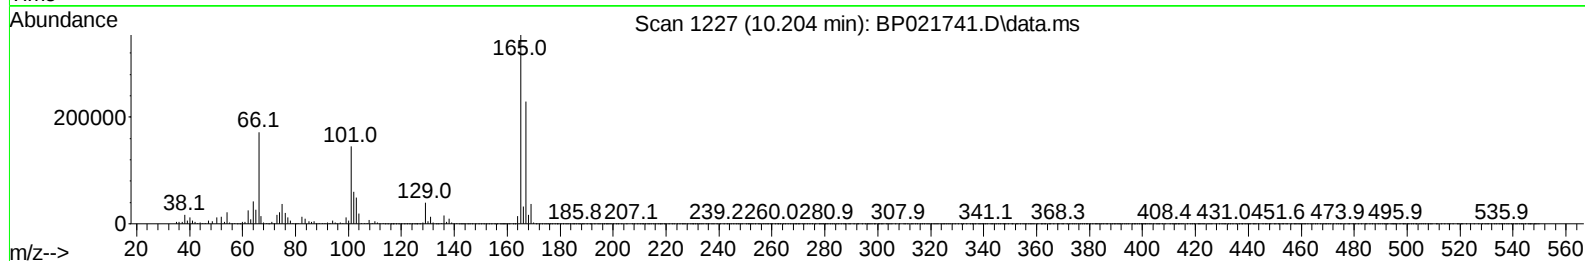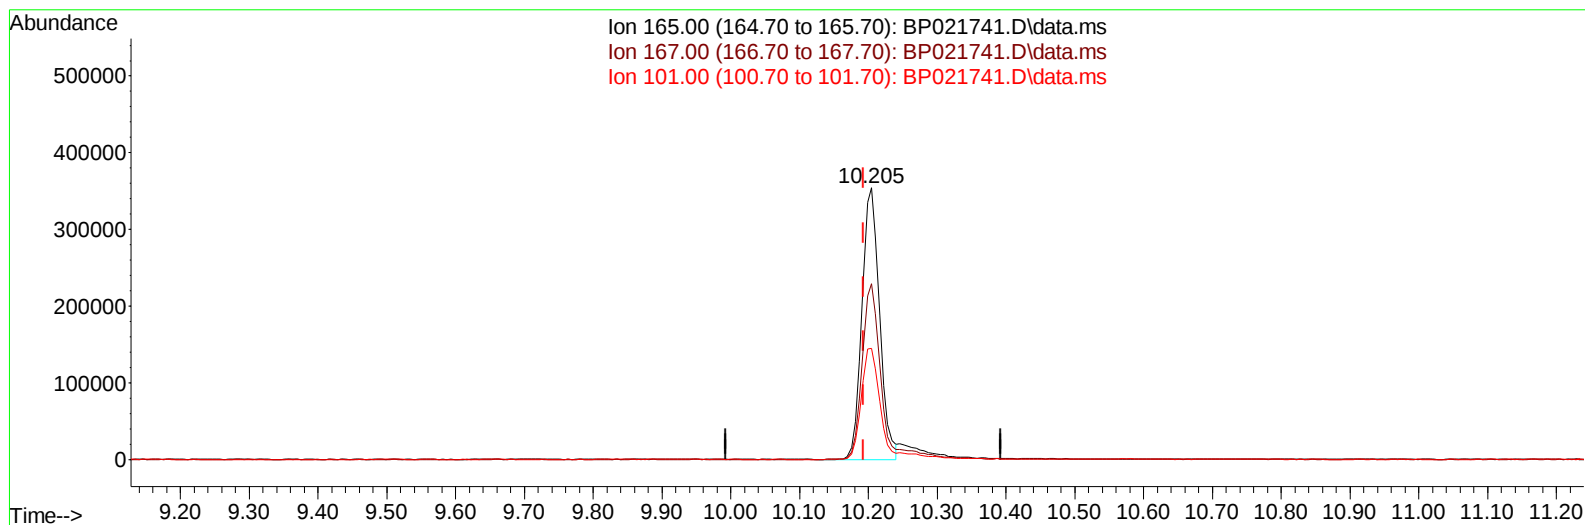

TIC: BP021741.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.204min (+ 0.012) 28.93 ng/u1

response 629528

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	64.62
101.00	41.40	41.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021741.D
Acq On : 30 Aug 2024 05:02
Operator : RC/JU
Sample : P3711-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A7

Manual IntegrationsAPPROVED

Quant Time: Aug 30 05:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/30/2024
Supervised By :mohammad ahmed 09/02/2024

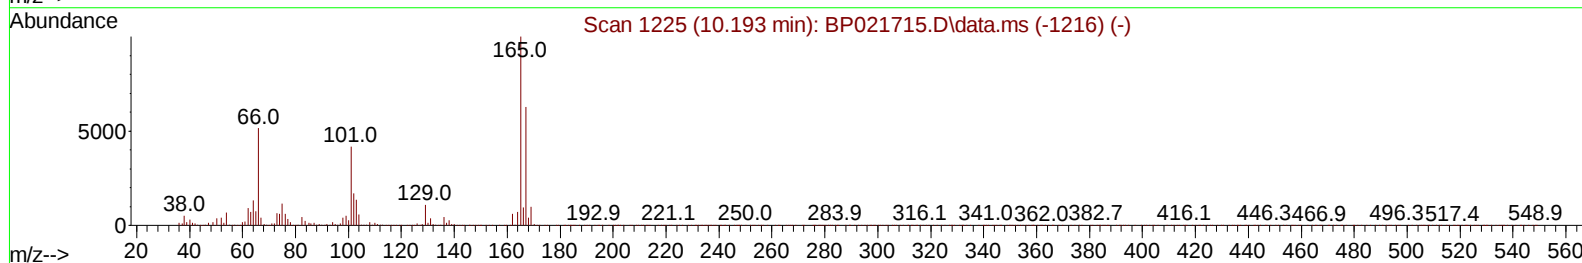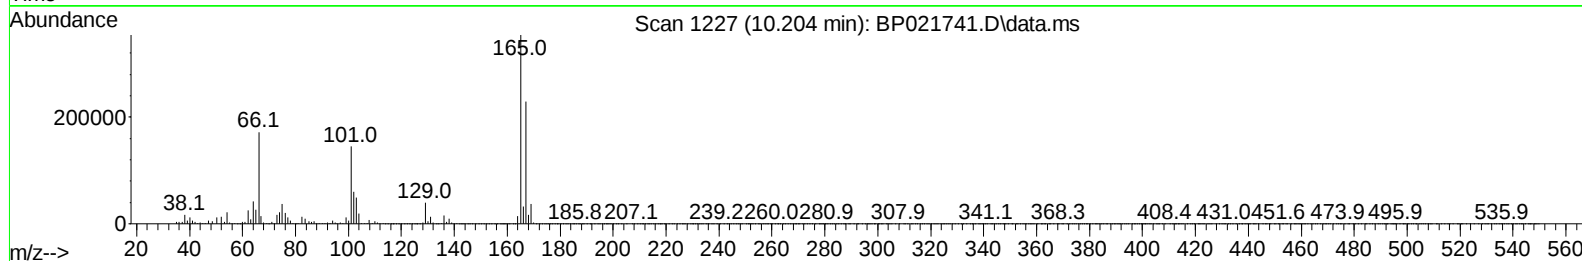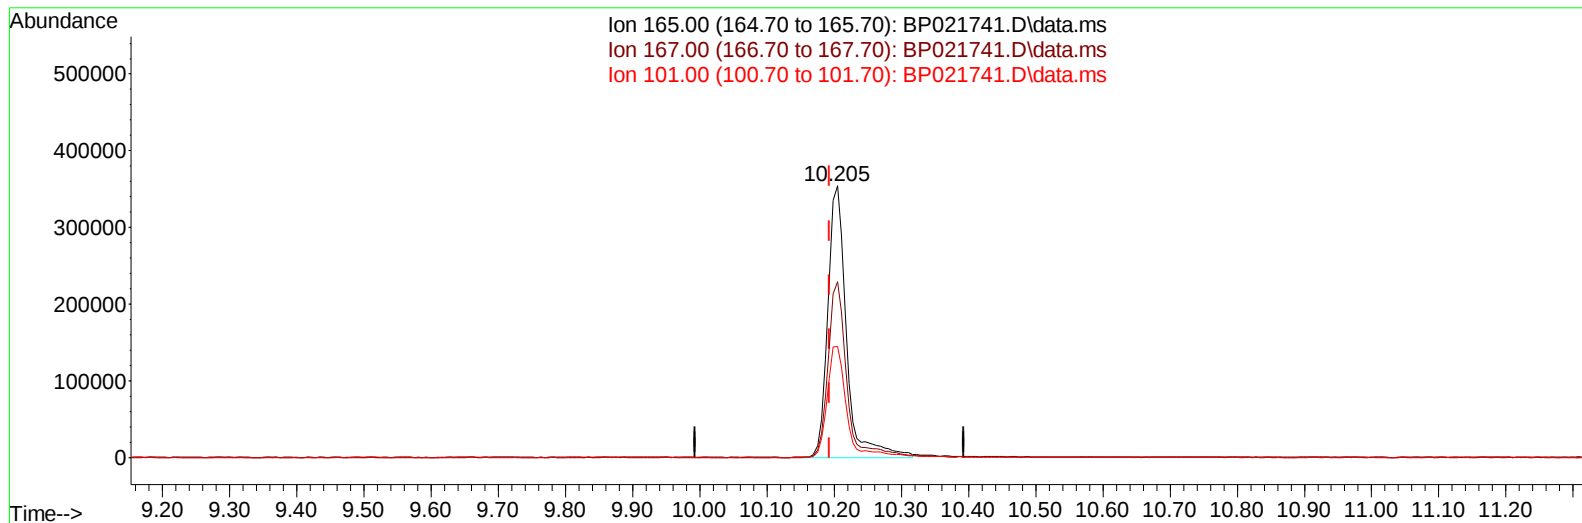

TIC: BP021741.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.204min (+ 0.012) 31.39 ng/ul m

response 683114

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	64.62
101.00	41.40	41.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021741.D
Acq On : 30 Aug 2024 05:02
Operator : RC/JU
Sample : P3711-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A7

Manual IntegrationsAPPROVED

Quant Time: Aug 30 05:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/30/2024
Supervised By :mohammad ahmed 09/02/2024

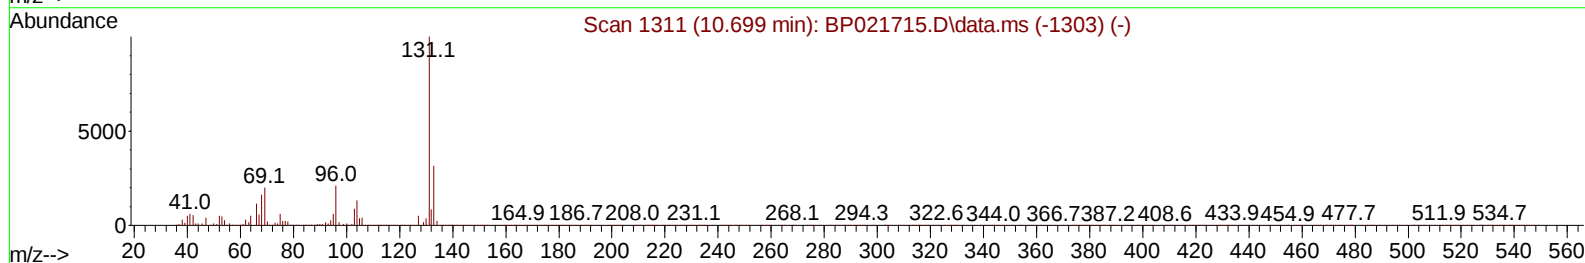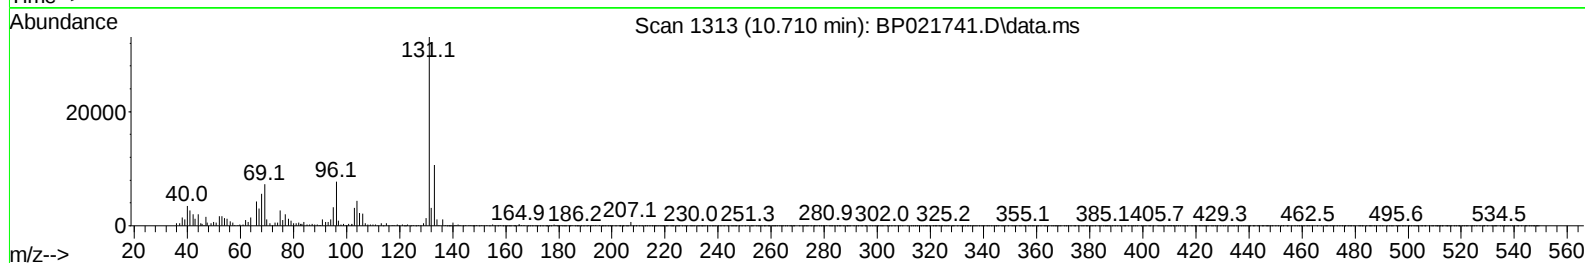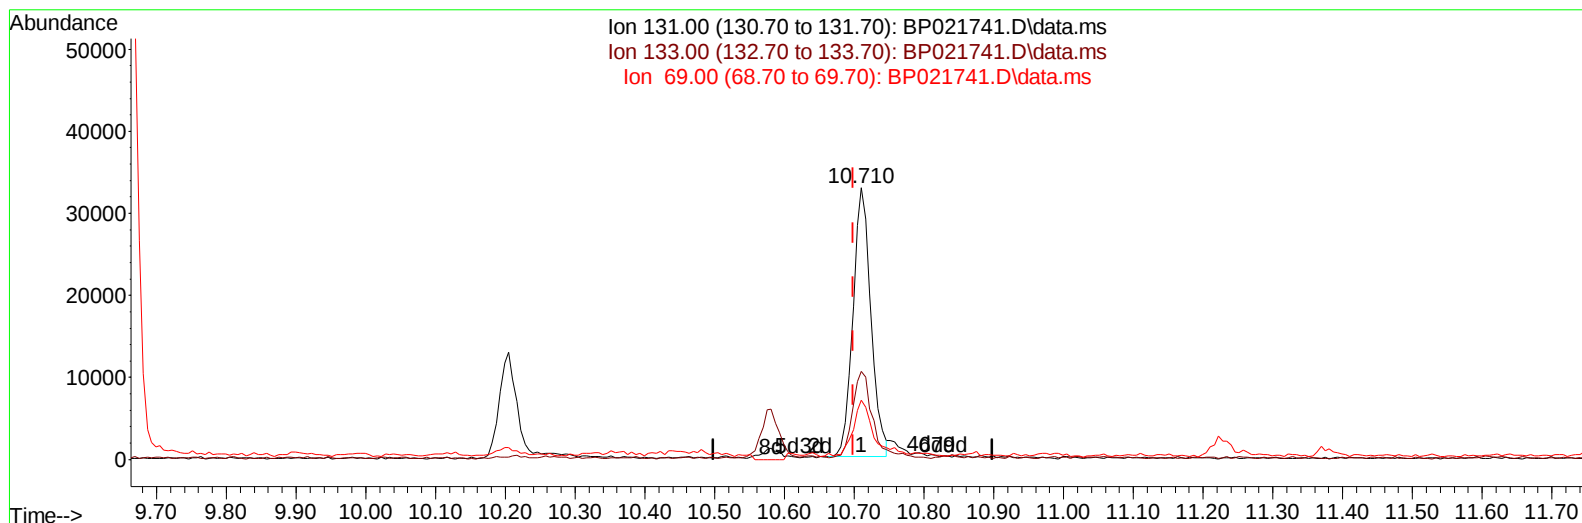

TIC: BP021741.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.710min (+ 0.012) 1.85 ng/u1

response 58598

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	32.35
69.00	19.80	21.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021741.D
Acq On : 30 Aug 2024 05:02
Operator : RC/JU
Sample : P3711-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A7

Manual IntegrationsAPPROVED

Quant Time: Aug 30 05:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/30/2024
Supervised By :mohammad ahmed 09/02/2024

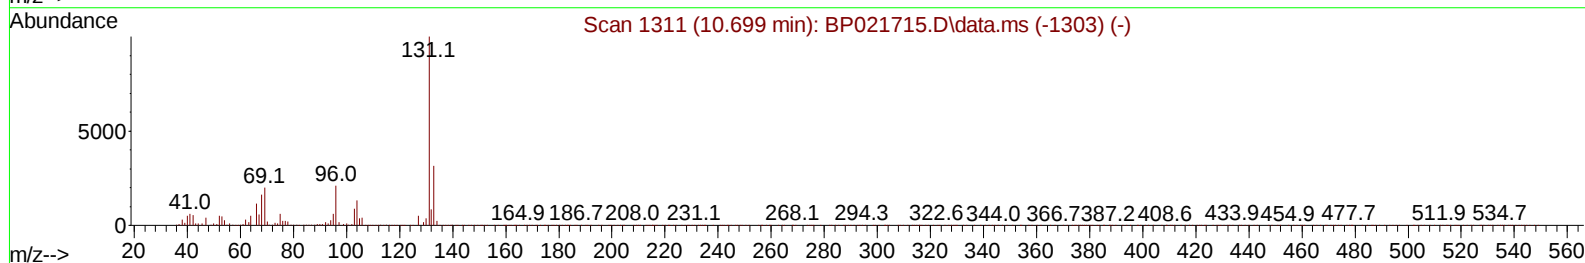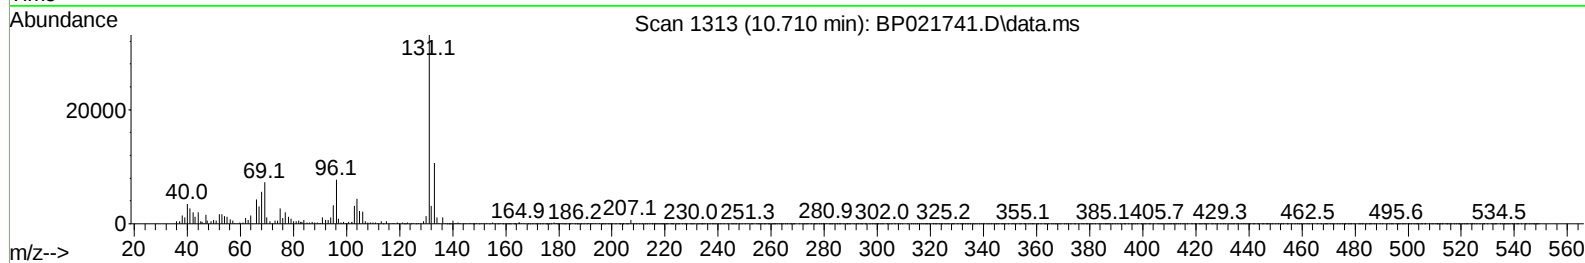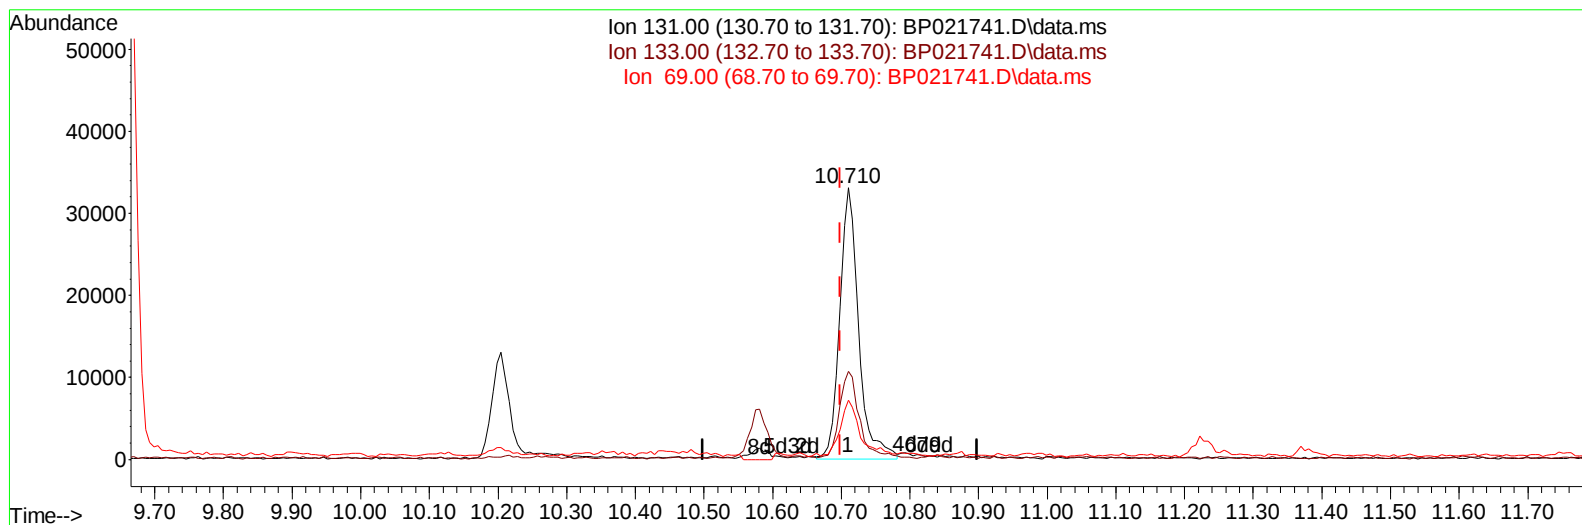

TIC: BP021741.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.710min (+ 0.012) 1.99 ng/ul m

response 63131

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	32.35
69.00	19.80	21.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
 Data File : BP021741.D
 Acq On : 30 Aug 2024 05:02
 Operator : RC/JU
 Sample : P3711-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E24A7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/30/2024
 Supervised By :mohammad ahmed 09/02/2024

Quant Time: Aug 30 05:39:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.787	152		320338	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136		1352355	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.434	164		942436	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.234	188		2091883	20.000	ng/ul	0.00
79) Chrysene-d12	21.680	240		1921869	20.000	ng/ul	0.01
88) Perylene-d12	25.098	264		2182217	20.000	ng/ul	0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.275	96		41061	4.255	ng/uL	0.00
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	6.963	99		445286	13.025	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67		550964	29.614	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132		679750	30.798	ng/ul	0.00
15) 4-Methylphenol-d8	8.493	113		651725	24.671	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128		348128	31.996	ng/ul	0.00
24) 2-Nitrophenol-d4	9.657	143		374472	33.907	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.204	165		683114m	31.388	ng/ul	0.01
31) 4-Chloroaniline-d4	10.710	131		63131m	1.994	ng/ul	0.01
46) Dimethylphthalate-d6	13.840	166		2309340	32.024	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160		2392372	29.549	ng/ul	0.00
54) 4-Nitrophenol-d4	14.645	143		184085	13.418	ng/ul	0.02
60) Fluorene-d10	15.440	176		2026239	33.422	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200		323979	28.159	ng/ul	0.00
73) Anthracene-d10	17.334	188		3462751	34.879	ng/ul	0.00
81) Pyrene-d10	19.698	212		4168314	37.941	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.857	264		4214906	36.222	ng/ul	0.02
Target Compounds							
						Qvalue	
16) Acetophenone	8.605	105		65321	1.542	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021741.D
Acq On : 30 Aug 2024 05:02
Operator : RC/JU
Sample : P3711-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A7

Manual IntegrationsAPPROVED

Quant Time: Aug 30 05:39:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/30/2024
Supervised By :mohammad ahmed 09/02/2024

