

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
 Data File : BP021720.D
 Acq On : 29 Aug 2024 13:14
 Operator : RC/JU
 Sample : P3711-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E24A6

Quant Time: Aug 29 14:24:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 27 05:11:38 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	301378	20.000	ng/u1	0.00
20) Naphthalene-d8	10.569	136	1272640	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.422	164	872044	20.000	ng/u1	-0.02
64) Phenanthrene-d10	17.228	188	1956283	20.000	ng/u1	-0.02
79) Chrysene-d12	21.686	240	1881087	20.000	ng/u1	0.00
88) Perylene-d12	25.104	264	2105575	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	39607	4.363	ng/uL	0.00
4) Pyridine-d5	3.693	84	221321	8.429	ng/u1	0.00
7) Phenol-d5	6.958	99	267773	8.325	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	493590	28.200	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.322	132	522339	25.155	ng/u1	0.00
15) 4-Methylphenol-d8	8.481	113	470420	18.928	ng/u1	-0.01
21) Nitrobenzene-d5	8.934	128	282727	27.613	ng/u1	0.00
24) 2-Nitrophenol-d4	9.652	143	283830	27.309	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	540226	26.377	ng/u1	0.00
31) 4-Chloroaniline-d4	10.699	131	751282	25.214	ng/u1	0.00
46) Dimethylphthalate-d6	13.828	166	1965553	29.457	ng/u1	-0.01
49) Acenaphthylene-d8	14.116	160	2070805	27.642	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.628	143	86444	6.809	ng/u1	0.00
60) Fluorene-d10	15.434	176	1691623	30.155	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.551	200	245812	22.846	ng/u1	-0.02
73) Anthracene-d10	17.328	188	3061334	32.973	ng/u1	-0.02
81) Pyrene-d10	19.704	212	3694489	34.358	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.868	264	3697991	32.936	ng/u1	0.00
Target Compounds						
16) Acetophenone	8.599	105	52879	1.327	ng/u1	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021720.D
Acq On : 29 Aug 2024 13:14
Operator : RC/JU
Sample : P3711-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A6

Quant Time: Aug 29 14:24:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 27 05:11:38 2024
Response via : Initial Calibration

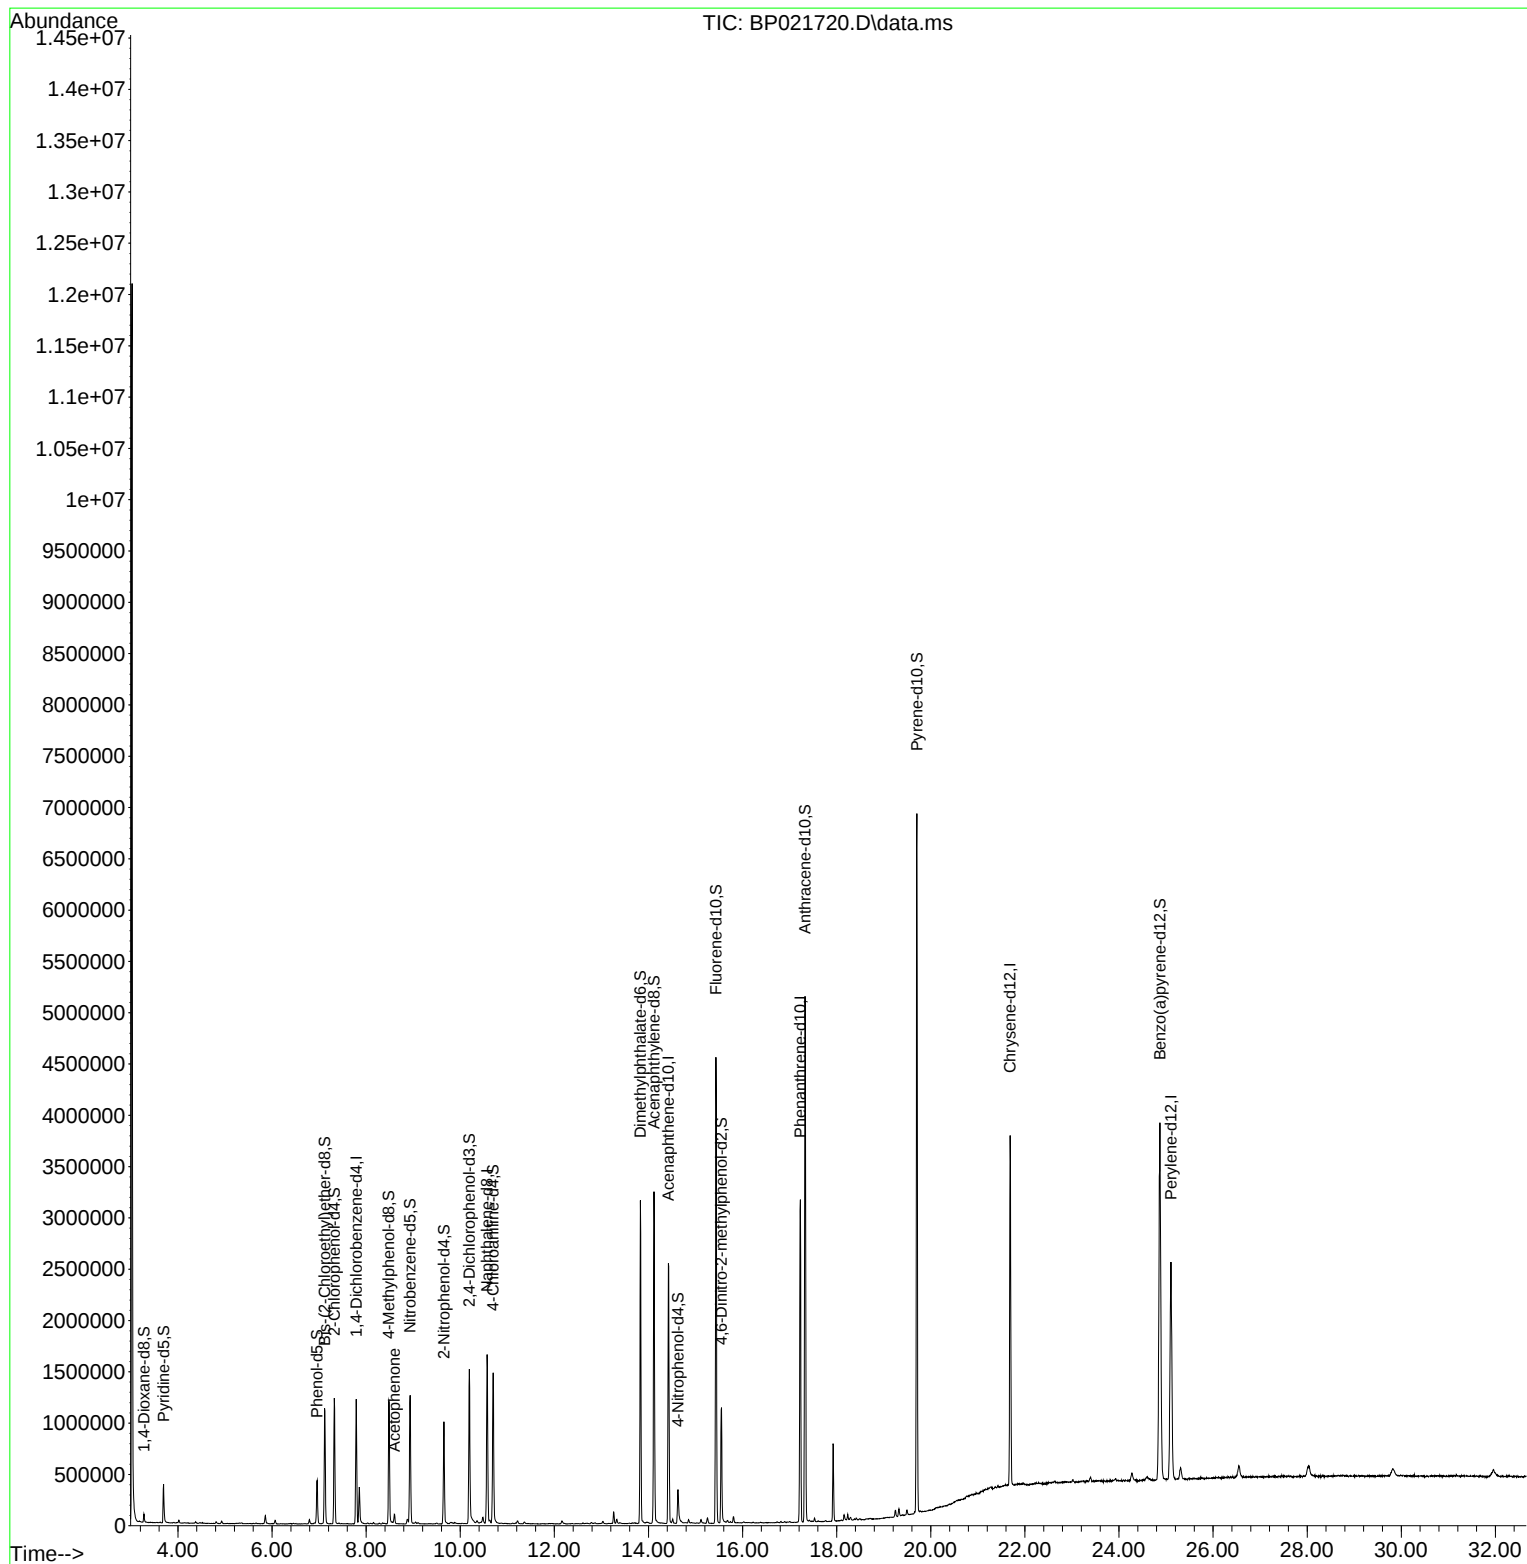

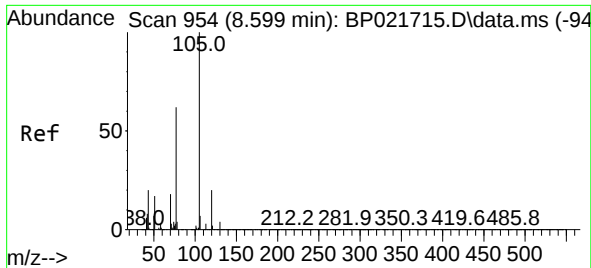

#16
Acetophenone
Concen: 1.327 ng/ul
RT: 8.599 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP021720.D
Acq: 29 Aug 2024 13:14

Instrument :
BNA_P
ClientSampleId :
E24A6

Tgt Ion:	105	Resp:	52879
Ion	Ratio	Lower	Upper
105	100		
77	78.9	59.4	89.2
51	23.2	16.4	24.6

