

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
 Data File : BP021743.D
 Acq On : 30 Aug 2024 06:28
 Operator : RC/JU
 Sample : P3711-18
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E24B0

Quant Time: Aug 30 07:11:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	400831	20.000	ng/u1	0.00
20) Naphthalene-d8	10.575	136	1779048	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.434	164	1210491	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.233	188	2640652	20.000	ng/u1	0.00
79) Chrysene-d12	21.686	240	2413469	20.000	ng/u1	0.02
88) Perylene-d12	25.086	264	2699892	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	54790	4.538	ng/uL	0.00
4) Pyridine-d5	3.705	84	15942	0.457	ng/u1	0.02
7) Phenol-d5	6.963	99	630015	14.728	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	714216	30.680	ng/u1	0.00
11) 2-Chlorophenol-d4	7.328	132	906695	32.831	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	928103	28.077	ng/u1	0.00
21) Nitrobenzene-d5	8.934	128	467386	32.654	ng/u1	0.00
24) 2-Nitrophenol-d4	9.657	143	513097	35.316	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.204	165	964309	33.681	ng/u1	0.01
31) 4-Chloroaniline-d4	10.704	131	1091422	26.203	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	3132365	33.818	ng/u1	0.00
49) Acenaphthylene-d8	14.122	160	3478275	33.448	ng/u1	0.00
54) 4-Nitrophenol-d4	14.639	143	262623	14.903	ng/u1	0.01
60) Fluorene-d10	15.439	176	2701880	34.697	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	377600	25.999	ng/u1	0.00
73) Anthracene-d10	17.339	188	4676019	37.312	ng/u1	0.00
81) Pyrene-d10	19.721	212	5454778	39.538	ng/u1	0.03
92) Benzo(a)pyrene-d12	24.862	264	5634143	39.135	ng/u1	0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.604	105	66539	1.256	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021743.D
Acq On : 30 Aug 2024 06:28
Operator : RC/JU
Sample : P3711-18
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24B0


Quant Time: Aug 30 07:11:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

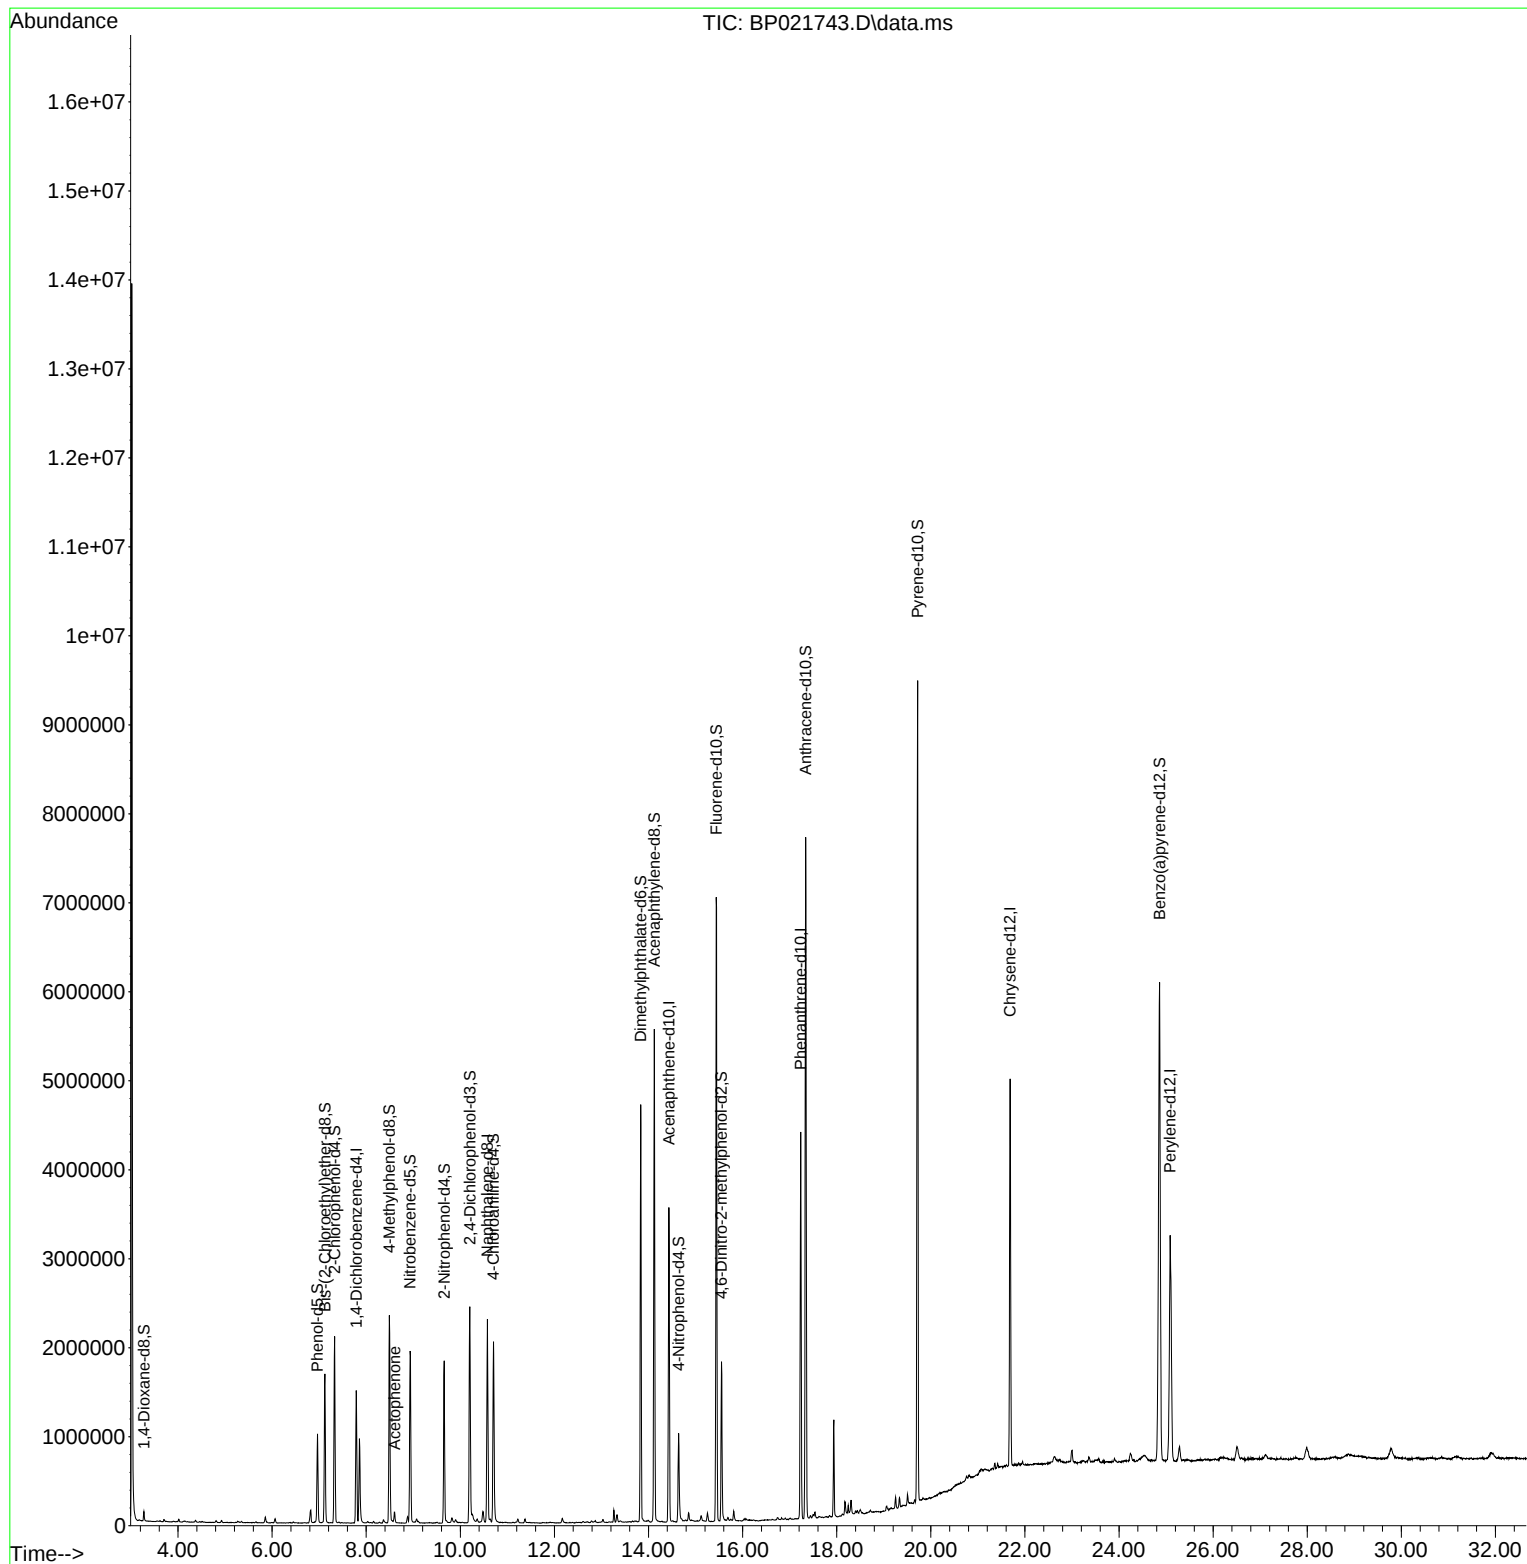

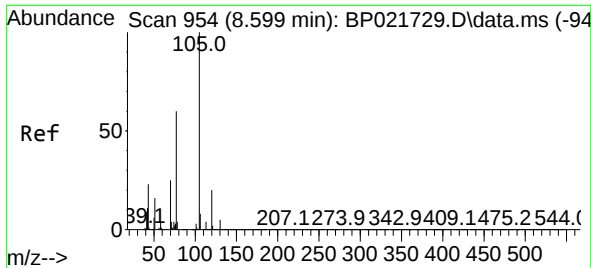

#16
 Acetophenone
 Concen: 1.256 ng/ul
 RT: 8.604 min Scan# 91
 Delta R.T. 0.006 min
 Lab File: BP021743.D
 Acq: 30 Aug 2024 06:28

Instrument :
 BNA_P
 ClientSampleId :
 E24B0

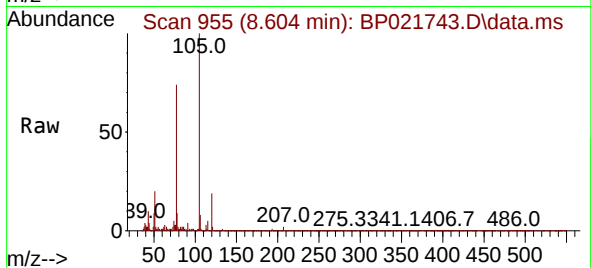

Tgt Ion:	105	Resp:	66539
Ion	Ratio	Lower	Upper
105	100		
77	74.0	59.4	89.2
51	20.3	16.4	24.6

