

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
 Data File : BP021719.D
 Acq On : 29 Aug 2024 12:32
 Operator : RC/JU
 Sample : P3711-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E24A3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021719.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.023	3	6	28	rVB	10715207	13386180	100.00%	14.867%
2	3.275	45	49	56	rVB	76463	97771	0.73%	0.109%
3	3.693	116	120	133	rBV	178162	264565	1.98%	0.294%
4	4.023	172	176	181	rVB	16959	23297	0.17%	0.026%
5	4.817	306	311	317	rVB3	13232	24670	0.18%	0.027%
6	4.928	324	330	336	rBV2	21637	34117	0.25%	0.038%
7	6.069	518	524	530	rBV	29791	49529	0.37%	0.055%
8	6.958	669	675	687	rBV	421958	671830	5.02%	0.746%
9	7.122	696	703	713	rVB	924216	1507671	11.26%	1.674%
10	7.322	729	737	748	rBV	1097997	1693197	12.65%	1.881%
11	7.787	808	816	824	rBV	987518	1648004	12.31%	1.830%
12	8.158	874	879	886	rVB9	9784	19129	0.14%	0.021%
13	8.487	926	935	944	rBV	1059749	1786221	13.34%	1.984%
14	8.552	944	946	953	rVB7	11855	17104	0.13%	0.019%
15	8.934	1001	1011	1026	rBV	1087202	1848025	13.81%	2.052%
16	9.658	1125	1134	1145	rBV	844541	1415165	10.57%	1.572%
17	10.193	1215	1225	1249	rBV	1254781	2362246	17.65%	2.624%
18	10.575	1282	1290	1301	rBV	1314771	2377404	17.76%	2.640%
19	10.705	1304	1312	1330	rVB	879785	1670627	12.48%	1.855%
20	12.169	1554	1561	1570	rBV2	19913	41892	0.31%	0.047%
21	13.834	1835	1844	1860	rBV	2700017	3813597	28.49%	4.236%
22	14.116	1883	1892	1911	rBV2	2596405	4112779	30.72%	4.568%
23	14.428	1935	1945	1967	rBV	2079880	3442230	25.71%	3.823%
24	14.622	1972	1978	1994	rBV	289780	687460	5.14%	0.764%
25	14.857	2015	2018	2025	rVB8	15563	22165	0.17%	0.025%
26	15.445	2109	2118	2131	rBV	3645517	5674268	42.39%	6.302%
27	15.551	2131	2136	2153	rVV	1122106	1604358	11.99%	1.782%
28	15.681	2154	2158	2162	rVB4	17635	26640	0.20%	0.030%
29	17.239	2416	2423	2432	rBV	3088828	4275079	31.94%	4.748%
30	17.345	2433	2441	2452	rBV	4830040	7068630	52.81%	7.851%
31	18.181	2578	2583	2592	rBV2	101002	160444	1.20%	0.178%
32	18.310	2601	2605	2611	rVB6	24301	40169	0.30%	0.045%
33	19.257	2761	2766	2772	rVB	65879	91715	0.69%	0.102%
34	19.333	2774	2779	2784	rVB2	53667	86335	0.64%	0.096%
35	19.504	2805	2808	2814	rBV3	64840	90591	0.68%	0.101%
36	19.710	2836	2843	2852	rBV	5016161	8553326	63.90%	9.500%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021719.D
Acq On : 29 Aug 2024 12:32
Operator : RC/JU
Sample : P3711-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Title : SVOA CALIBRATION

37	21.680	3172	3178	3191	rBV2	3007292	4965655	37.10%	5.515%
38	24.857	3707	3718	3733	rVB	3337072	9036475	67.51%	10.036%
39	25.086	3748	3757	3772	rVB	1832619	5347522	39.95%	5.939%




Sum of corrected areas: 90038082

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021719.D
Acq On : 29 Aug 2024 12:32
Operator : RC/JU
Sample : P3711-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

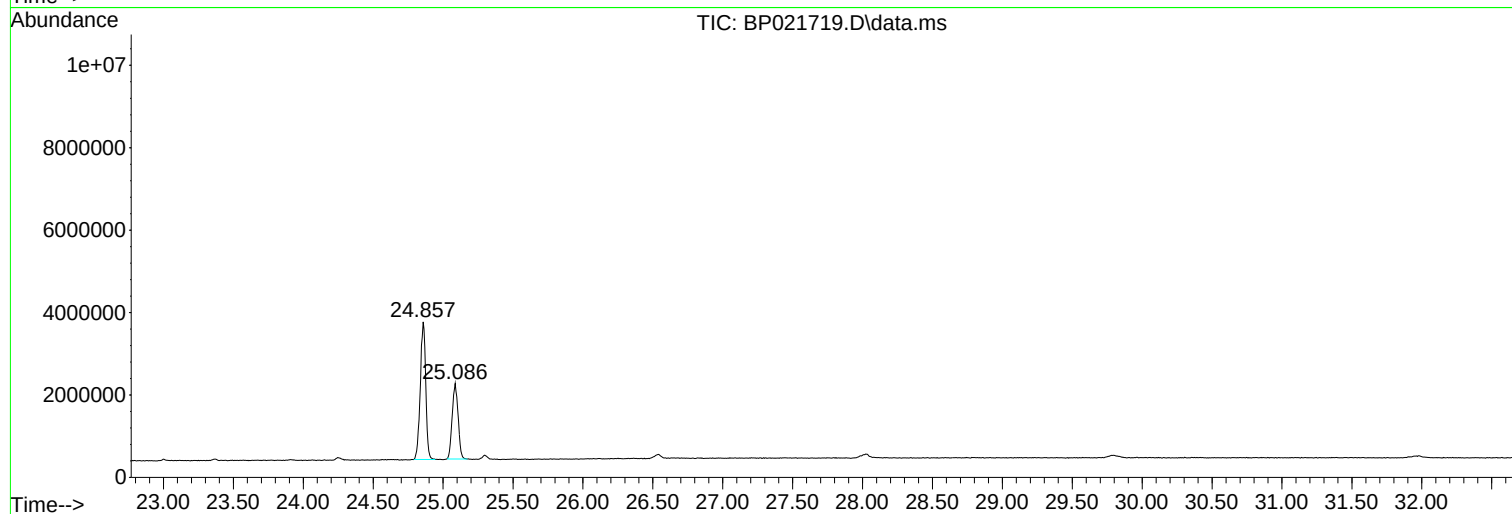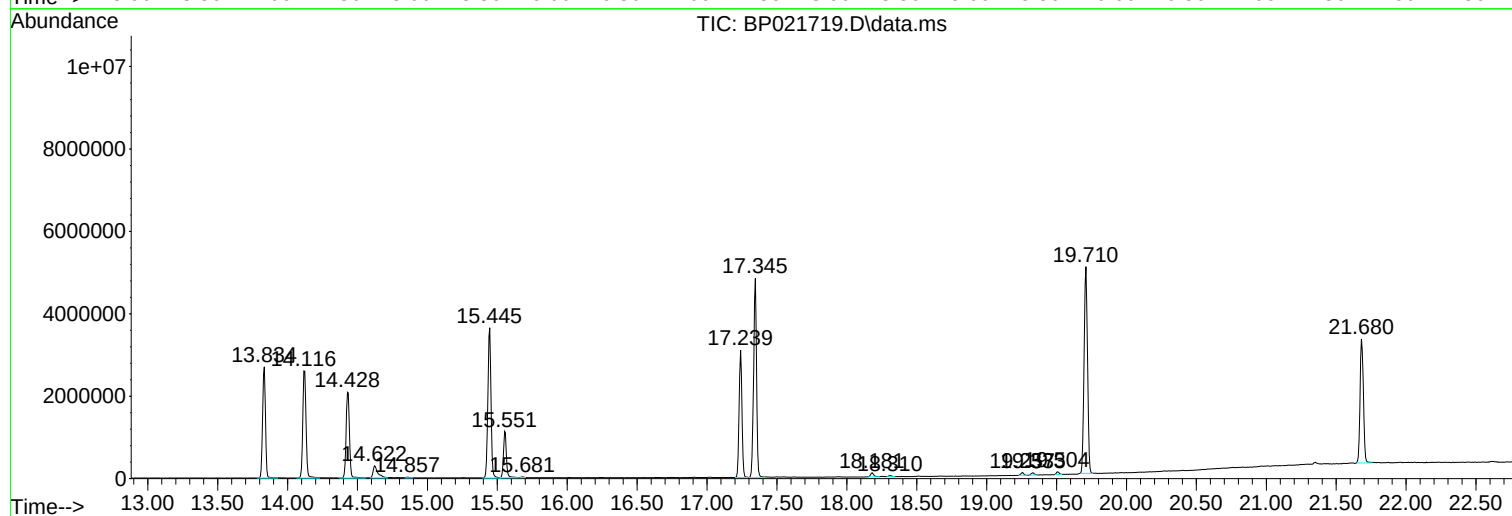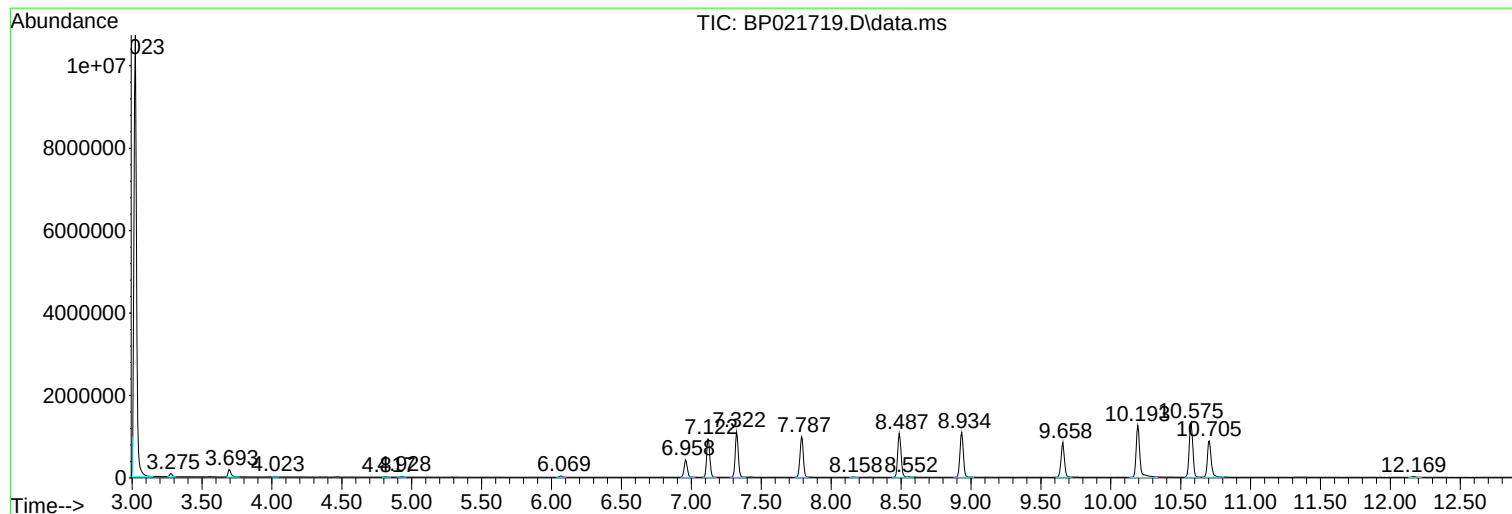

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021719.D
Acq On : 29 Aug 2024 12:32
Operator : RC/JU
Sample : P3711-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.023	162.45 ng/ul	13386200	1,4-Dichlorobenzene-d4	7.787

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	74
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

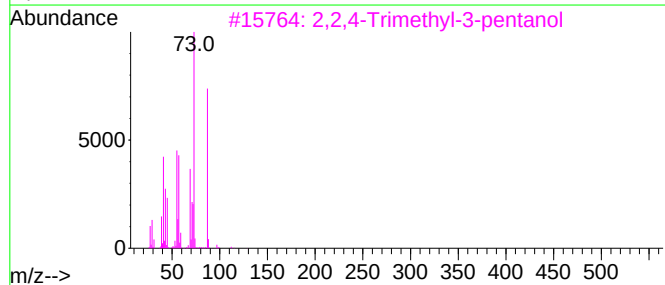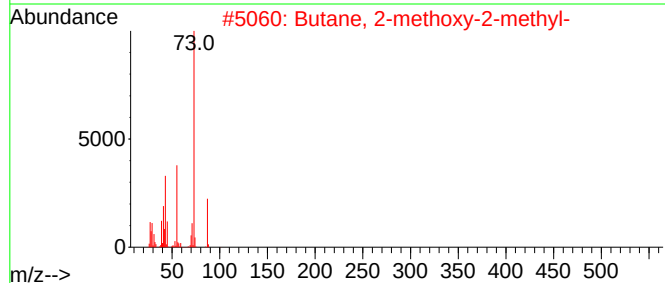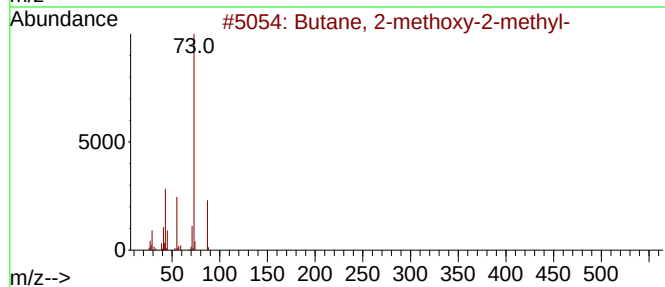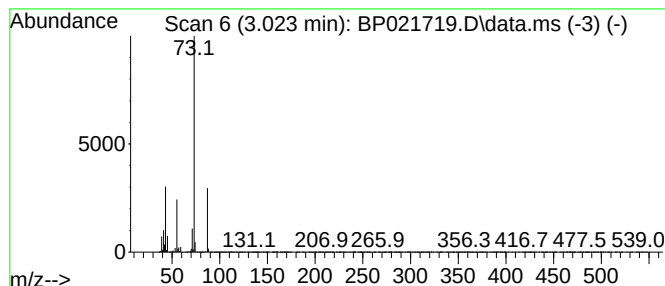

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021719.D
Acq On : 29 Aug 2024 12:32
Operator : RC/JU
Sample : P3711-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E24A3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.023	162.4	ng/ul	13386200	1	7.787	1648000	20.0