

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
 Data File : BP021746.D
 Acq On : 30 Aug 2024 08:37
 Operator : RC/JU
 Sample : SP6609
 Misc : SFAM SPIKE
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SP6609

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	51	rVV	98777	126482	0.44%	0.017%
2	3.334	51	59	68	rVV	298811	667027	2.31%	0.092%
3	3.734	122	127	143	rVB	3656265	4826206	16.75%	0.664%
4	4.017	170	175	184	rVB	34688	66409	0.23%	0.009%
5	4.540	258	264	276	rVB2	70409	153224	0.53%	0.021%
6	4.946	327	333	341	rBV	197927	272296	0.94%	0.037%
7	6.940	664	672	676	rBV	3505113	5343096	18.54%	0.735%
8	6.999	676	682	696	rVB	3904147	6441809	22.35%	0.886%
9	7.216	712	719	732	rVB	3108093	4907966	17.03%	0.675%
10	7.363	736	744	754	rBV	4045468	6456758	22.40%	0.888%
11	7.793	810	817	830	rVB	1167369	1913882	6.64%	0.263%
12	8.240	885	893	899	rBV	4979851	8370960	29.05%	1.152%
13	8.310	899	905	913	rVV	3267353	5298811	18.39%	0.729%
14	8.569	938	949	951	rBV	4797535	8754695	30.38%	1.204%
15	8.605	951	955	969	rVB2	6587168	12777364	44.34%	1.758%
16	8.875	993	1001	1009	rVB	3430195	5880891	20.41%	0.809%
17	8.981	1011	1019	1030	rBV	3392130	5631728	19.54%	0.775%
18	9.252	1059	1065	1073	rVB	828913	1290112	4.48%	0.177%
19	9.516	1101	1110	1123	rBV	4836550	8256242	28.65%	1.136%
20	9.687	1131	1139	1145	rBV	2805361	4753555	16.49%	0.654%
21	9.757	1145	1151	1160	rVV	5387294	8921455	30.96%	1.227%
22	9.987	1177	1190	1204	rVB	4047896	6358955	22.07%	0.875%
23	10.234	1222	1232	1250	rBV	4730472	7843272	27.22%	1.079%
24	10.581	1281	1291	1294	rBV	1527587	2709029	9.40%	0.373%
25	10.634	1294	1300	1308	rVV	5981701	10474951	36.35%	1.441%
26	10.728	1308	1316	1325	rVV	3100754	5783516	20.07%	0.796%
27	10.810	1325	1330	1339	rVV3	67547	185097	0.64%	0.025%
28	10.922	1341	1349	1365	rVB	4591769	7772950	26.97%	1.069%
29	11.546	1444	1455	1470	rBV	2077381	5006582	17.37%	0.689%
30	11.710	1479	1483	1491	rVB6	14612	31396	0.11%	0.004%
31	11.875	1503	1511	1526	rBV	4681730	8432744	29.26%	1.160%
32	12.134	1548	1555	1565	rVB	1715410	2726711	9.46%	0.375%
33	12.246	1565	1574	1581	rBV	7330407	11592533	40.23%	1.595%
34	12.369	1587	1595	1602	rBV	475960	807431	2.80%	0.111%
35	12.463	1603	1611	1622	rVB	6904866	11575942	40.17%	1.593%
36	12.610	1622	1636	1643	rBV2	7061229	14117591	48.99%	1.942%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
 Data File : BP021746.D
 Acq On : 30 Aug 2024 08:37
 Operator : RC/JU
 Sample : SP6609
 Misc : SFAM SPIKE
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SP6609

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

37	12.857	1669	1678	1684	rBV	5520646	8775406	30.45%	1.207%
38	12.934	1684	1691	1709	rVB	5203665	8689916	30.15%	1.196%
39	13.222	1727	1740	1743	rBV	5988413	9736728	33.79%	1.340%
40	13.257	1743	1746	1750	rVV	8536461	12898061	44.76%	1.775%
41	13.298	1750	1753	1769	rVB	6929382	10175941	35.31%	1.400%
42	13.504	1776	1788	1799	rBV	3848714	6443292	22.36%	0.886%
43	13.734	1821	1827	1835	rVB	120266	179696	0.62%	0.025%
44	13.893	1846	1854	1866	rBV	6362032	9834958	34.13%	1.353%
45	13.998	1866	1872	1883	rVB	5199935	6761896	23.46%	0.930%
46	14.157	1891	1899	1908	rVB	6810951	11415693	39.61%	1.571%
47	14.263	1913	1917	1921	rBV2	22682	30608	0.11%	0.004%
48	14.334	1921	1929	1938	rBV	4093057	6160133	21.38%	0.848%
49	14.434	1938	1946	1951	rVV	2140453	3477358	12.07%	0.478%
50	14.498	1951	1957	1962	rVV	8623469	13777748	47.81%	1.896%
51	14.545	1962	1965	1975	rVV	2386292	3350043	11.62%	0.461%
52	14.663	1976	1985	1992	rVV	3262231	5485695	19.04%	0.755%
53	14.757	1992	2001	2005	rVV	6819513	10857826	37.68%	1.494%
54	14.804	2005	2009	2012	rVV	4605749	7357299	25.53%	1.012%
55	14.845	2012	2016	2027	rVB	7182301	11131702	38.63%	1.532%
56	15.069	2047	2054	2070	rBV	5304676	8687148	30.14%	1.195%
57	15.275	2077	2089	2104	rVB	7823521	10930077	37.93%	1.504%
58	15.498	2120	2127	2135	rBV3	15144098	28818561	100.00%	3.965%
59	15.575	2135	2140	2154	rVV	3412689	4744851	16.46%	0.653%
60	15.710	2156	2163	2169	rVV	9325686	12886953	44.72%	1.773%
61	15.751	2169	2170	2179	rVV2	67929	88619	0.31%	0.012%
62	15.839	2182	2185	2196	rVB3	17003	32065	0.11%	0.004%
63	16.104	2224	2230	2235	rVB2	80647	118005	0.41%	0.016%
64	16.187	2239	2244	2248	rBV6	17665	29407	0.10%	0.004%
65	16.404	2274	2281	2291	rBV	6854082	9684879	33.61%	1.332%
66	16.528	2295	2302	2309	rBV	8294698	10552829	36.62%	1.452%
67	16.692	2322	2330	2347	rVB	7460029	10613220	36.83%	1.460%
68	16.881	2355	2362	2379	rBV	6302138	8986693	31.18%	1.236%
69	17.022	2381	2386	2388	rBV2	93516	144741	0.50%	0.020%
70	17.234	2415	2422	2425	rBV	2454743	4215423	14.63%	0.580%
71	17.275	2425	2429	2438	rVV	10221299	15473378	53.69%	2.129%
72	17.369	2438	2445	2458	rVB	10026212	15419919	53.51%	2.121%
73	17.516	2467	2470	2475	rVB	25192	33096	0.11%	0.005%
74	17.645	2485	2492	2509	rBV	9442162	13540251	46.98%	1.863%
75	18.181	2579	2583	2588	rBV7	19541	45660	0.16%	0.006%
76	18.251	2589	2595	2600	rVV	11044142	13077873	45.38%	1.799%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
 Data File : BP021746.D
 Acq On : 30 Aug 2024 08:37
 Operator : RC/JU
 Sample : SP6609
 Misc : SFAM SPIKE
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SP6609

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

77	18.292	2600	2602	2611	rVB2	142413	220666	0.77%	0.030%
78	18.510	2634	2639	2644	rBV2	134289	211215	0.73%	0.029%
79	18.692	2666	2670	2676	rBV2	33811	53784	0.19%	0.007%
80	19.098	2736	2739	2745	rVB5	47701	73770	0.26%	0.010%
81	19.298	2770	2773	2776	rBV	62616	73264	0.25%	0.010%
82	19.357	2776	2783	2790	rVV	11086191	17143265	59.49%	2.359%
83	19.616	2823	2827	2832	rBV2	227841	320965	1.11%	0.044%
84	19.733	2840	2847	2859	rVB	11499695	18049134	62.63%	2.483%
85	19.869	2866	2870	2876	rVB	127281	189634	0.66%	0.026%
86	20.122	2909	2913	2917	rVB	113158	144223	0.50%	0.020%
87	20.686	3003	3009	3015	rBV	10608801	14126675	49.02%	1.944%
88	21.586	3156	3162	3163	rBV	7075099	8386572	29.10%	1.154%
89	21.610	3163	3166	3171	rVV	12473797	17361556	60.24%	2.389%
90	21.674	3171	3177	3183	rVV2	11315488	22164392	76.91%	3.049%
91	21.739	3183	3188	3196	rVB	10974697	17805934	61.79%	2.450%
92	22.063	3239	3243	3250	rVB	438104	694246	2.41%	0.096%
93	22.774	3360	3364	3372	rVB	379805	607538	2.11%	0.084%
94	22.916	3380	3388	3399	rVB	8393643	15690825	54.45%	2.159%
95	24.021	3566	3576	3582	rBV	7075108	19247383	66.79%	2.648%
96	24.092	3582	3588	3601	rVB	7636522	18710273	64.92%	2.574%
97	24.939	3721	3732	3745	rVB	6545104	18824880	65.32%	2.590%
98	25.086	3749	3757	3768	rVB	1736156	4407485	15.29%	0.606%
99	28.980	4405	4419	4420	rBV	4403568	10433919	36.21%	1.436%
100	30.192	4608	4625	4626	rBV	3534230	10707811	37.16%	1.473%




Sum of corrected areas: 726842724

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021746.D
Acq On : 30 Aug 2024 08:37
Operator : RC/JU
Sample : SP6609
Misc : SFAM SPIKE
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SP6609

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

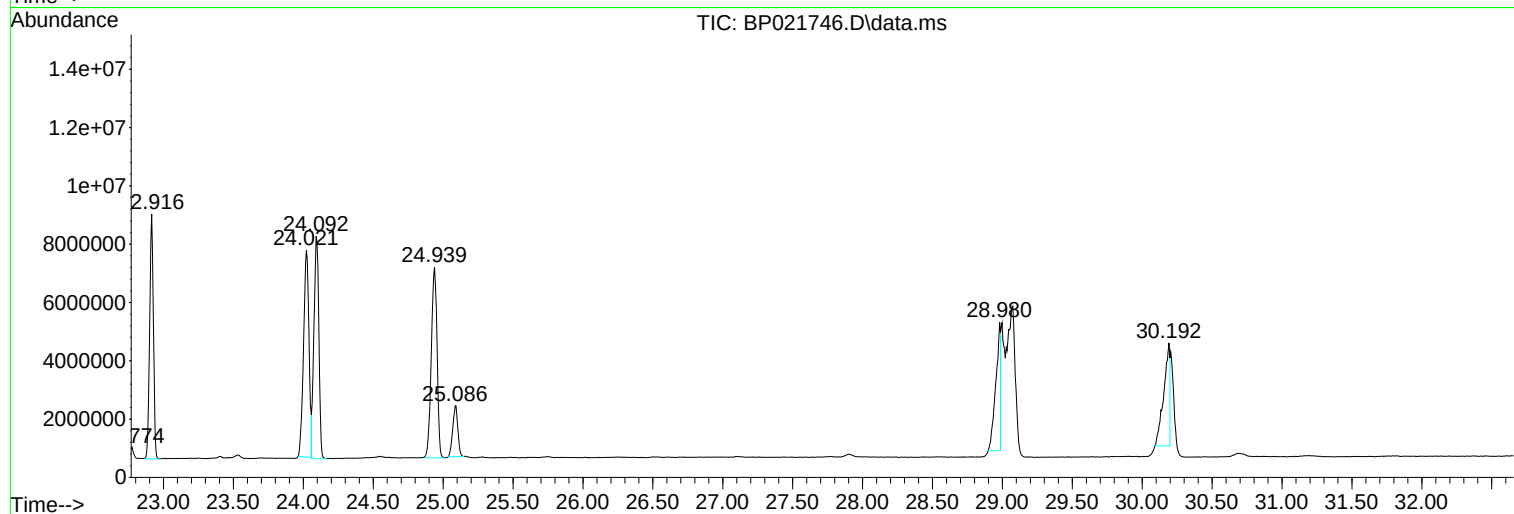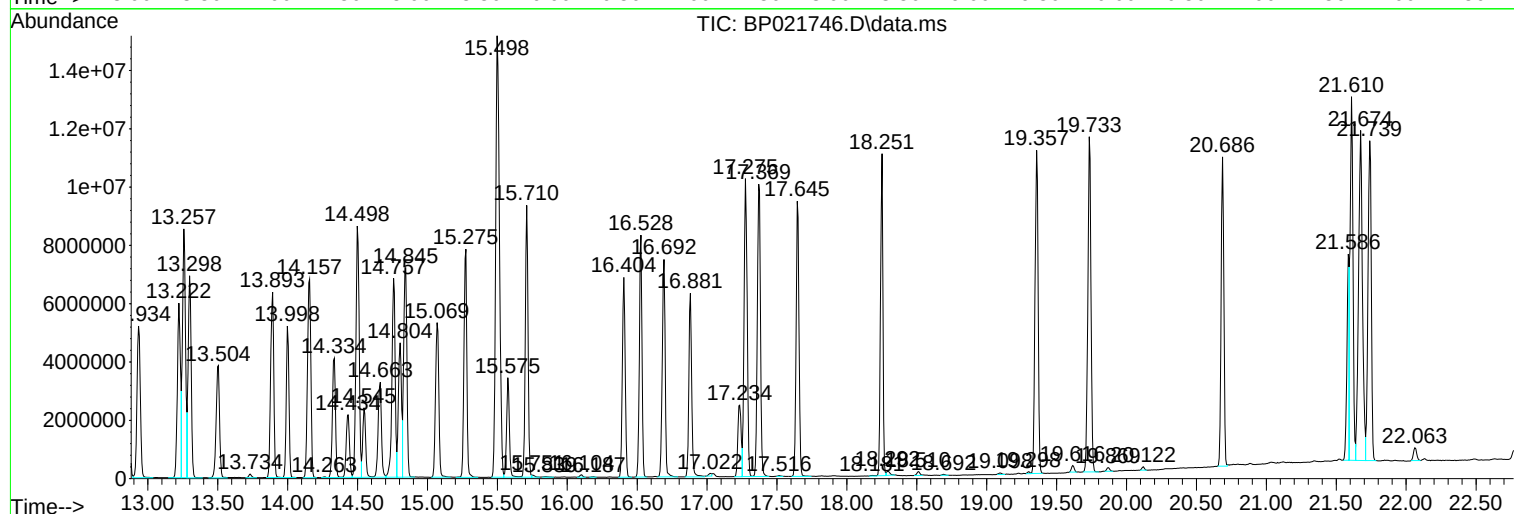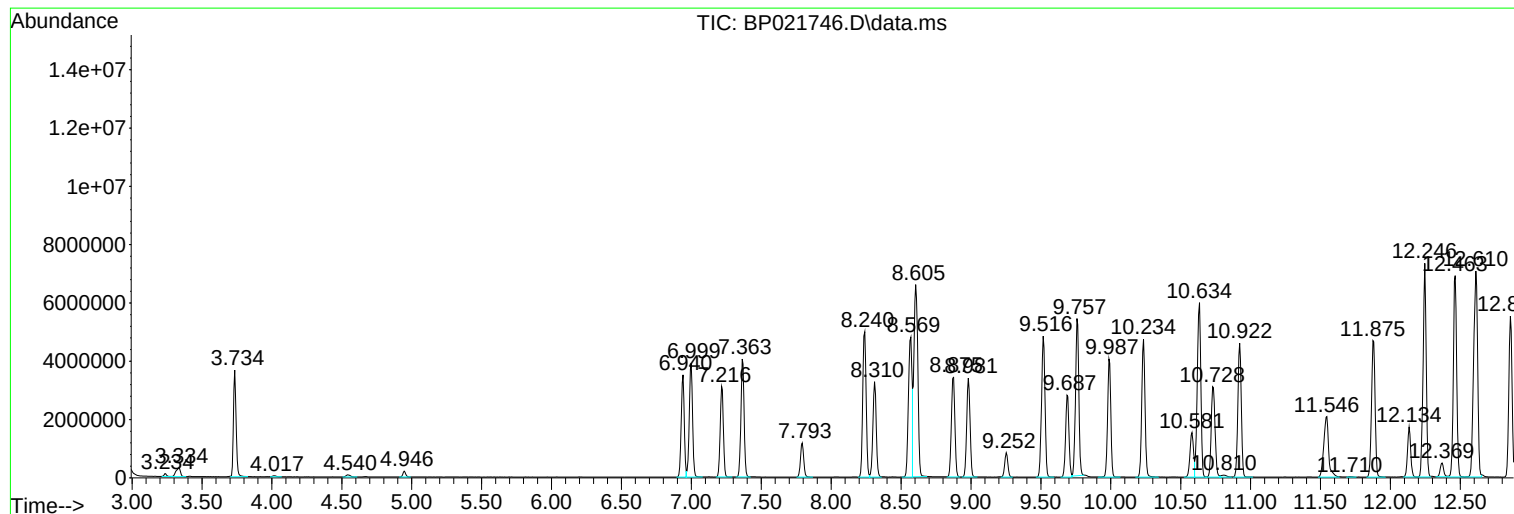

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021746.D
Acq On : 30 Aug 2024 08:37
Operator : RC/JU
Sample : SP6609
Misc : SFAM SPIKE
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SP6609

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082924\
Data File : BP021746.D
Acq On : 30 Aug 2024 08:37
Operator : RC/JU
Sample : SP6609
Misc : SFAM SPIKE
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SP6609

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------