
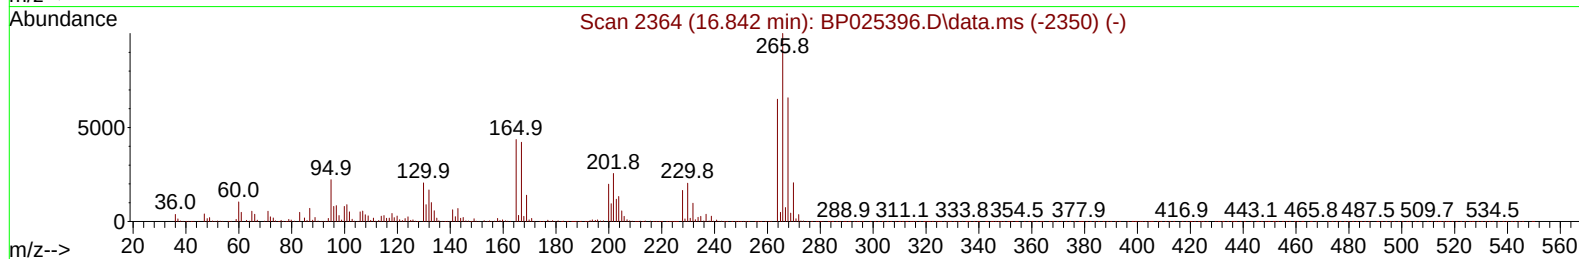
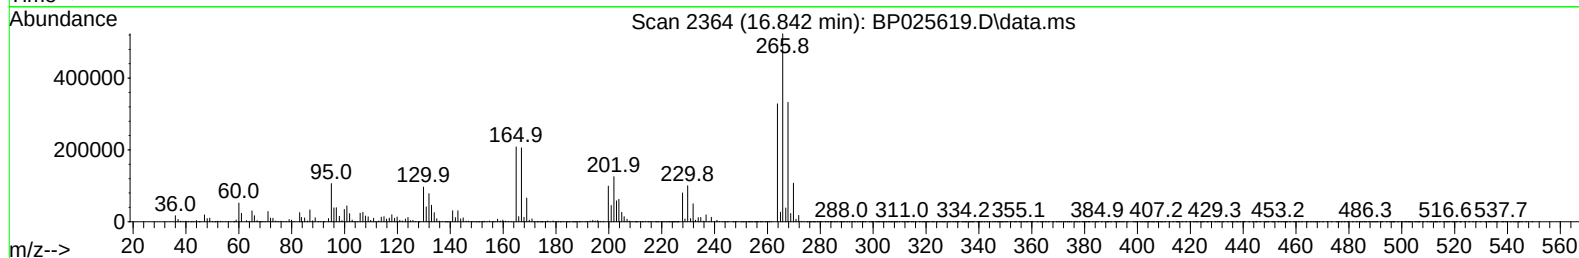


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082925\
Data File : BP025619.D
Acq On : 29 Aug 2025 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 12:15:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

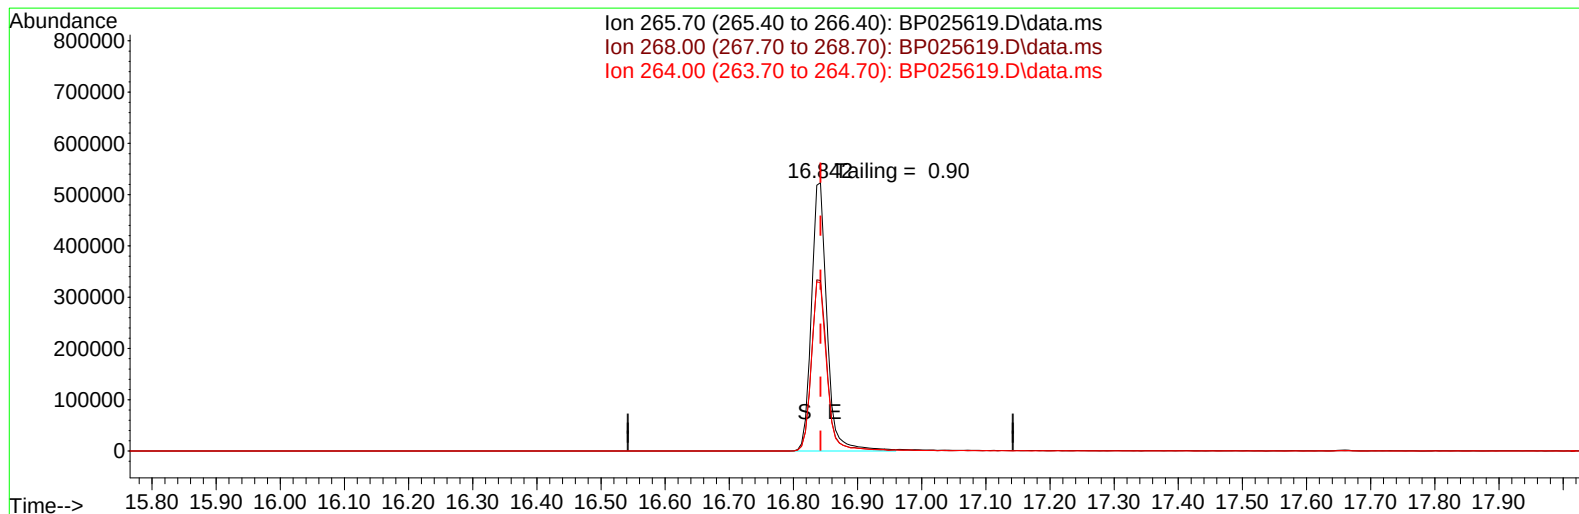

TIC: BP025619.D\data.ms

(70) Pentachlorophenol (C)




16.842min (-0.000) 584297.48 ng

response 893451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	63.49
264.00	65.00	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082925\
Data File : BP025619.D
Acq On : 29 Aug 2025 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 12:15:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

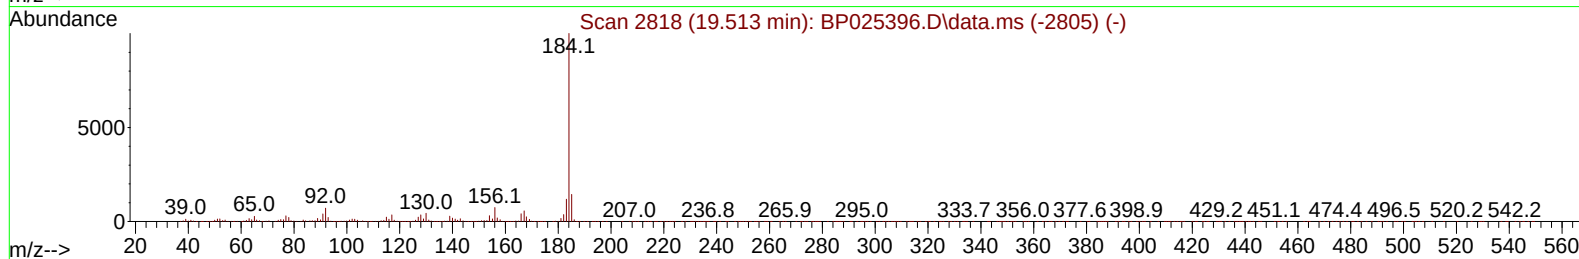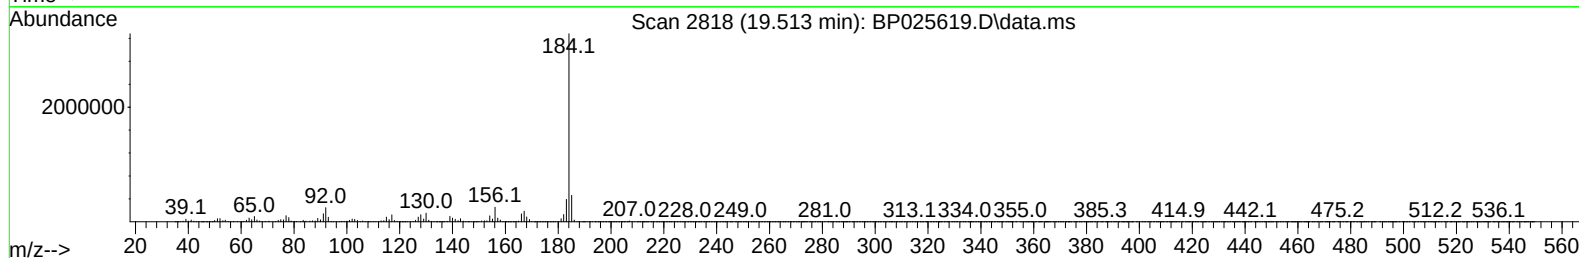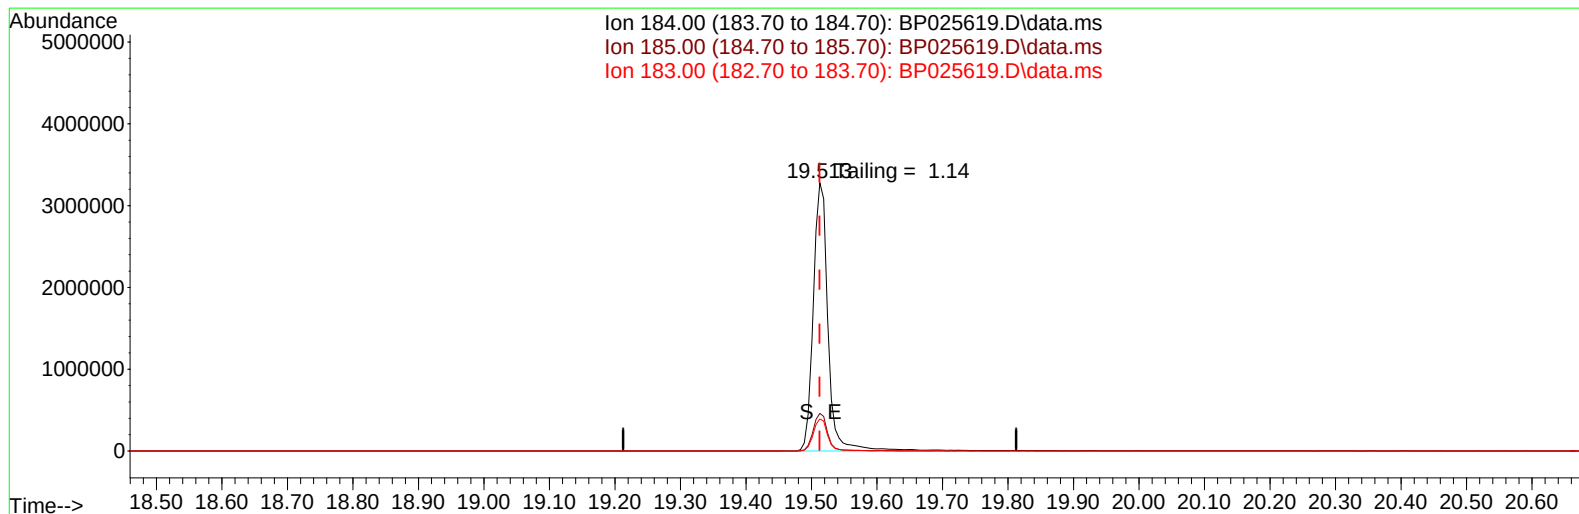

TIC: BP025619.D\data.ms

(77) Benzidine**19.513min (-0.000) 276434.71 ng****response 5103867**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.01
183.00	11.80	11.95
0.00	0.00	0.00