
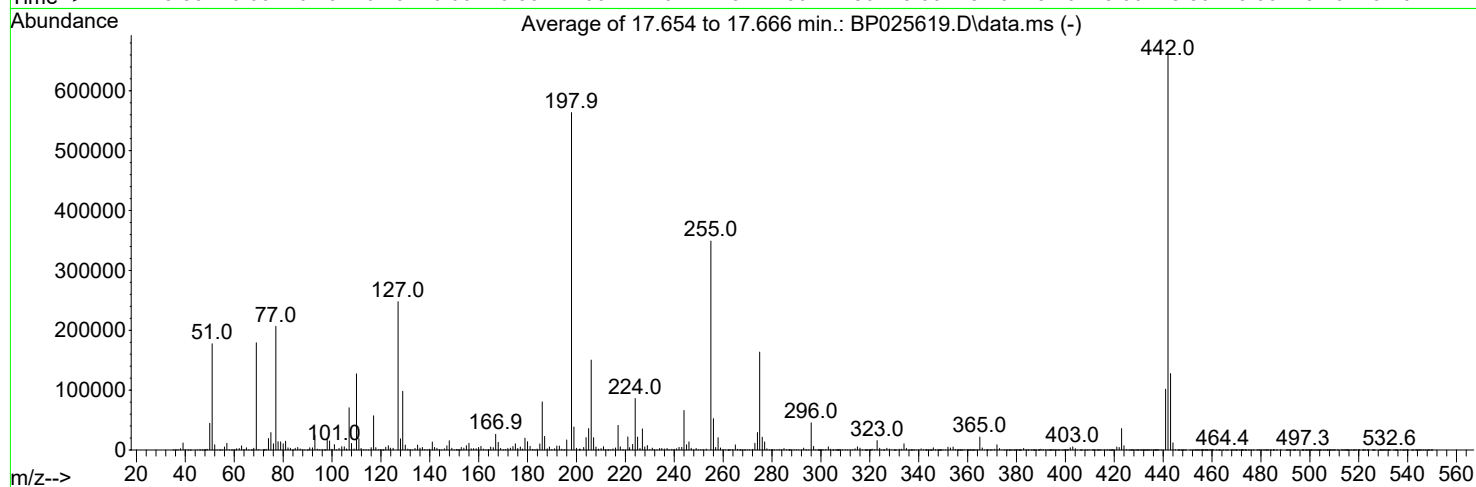


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082925\
Data File : BP025619.D
Acq On : 29 Aug 2025 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

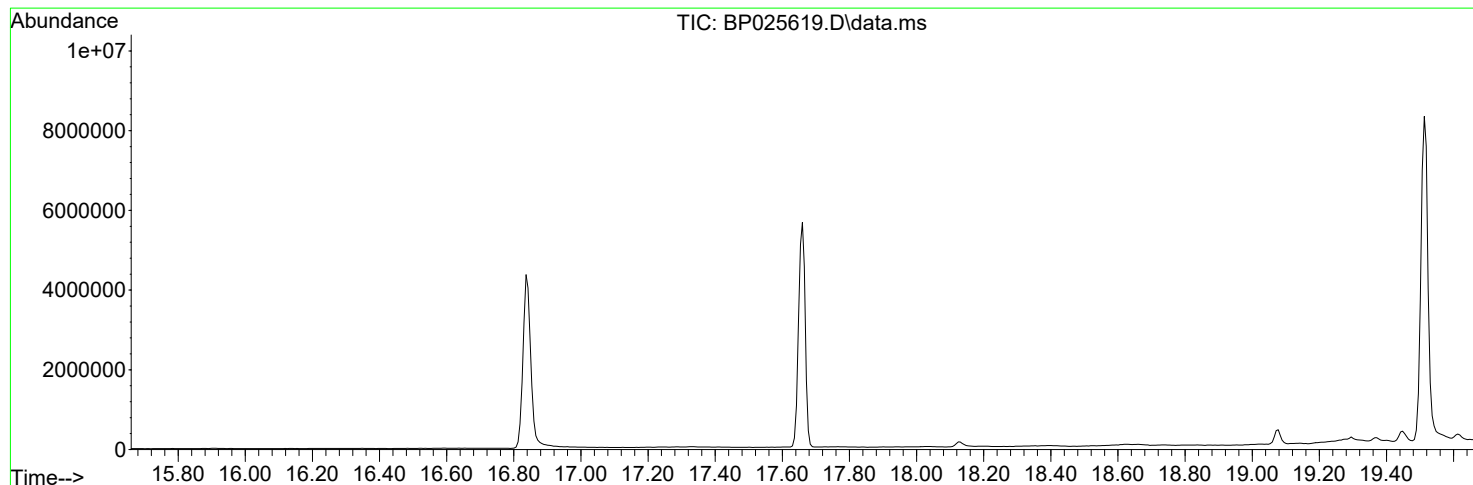

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2492

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2872	PASS
69	69	100	100	100.0	179112	PASS
70	69	0.00	2	0.5	879	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	563738	PASS
199	198	5	9	6.9	38651	PASS
365	198	1	100	3.8	21659	PASS
441	443	0.01	150	79.5	101685	PASS
442	442	100	100	100.0	659541	PASS
443	442	15	24	19.4	127855	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/29/2025	BNA_P	<u>BP025619.D</u>
Compound Name	Response	Retention Time
DDT	2426769	20.807
DDD	68299	20.354
DDE	6997	19.813
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
75296	2502065	3.01

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082925\
Data File : BP025619.D
Acq On : 29 Aug 2025 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 29 12:15:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

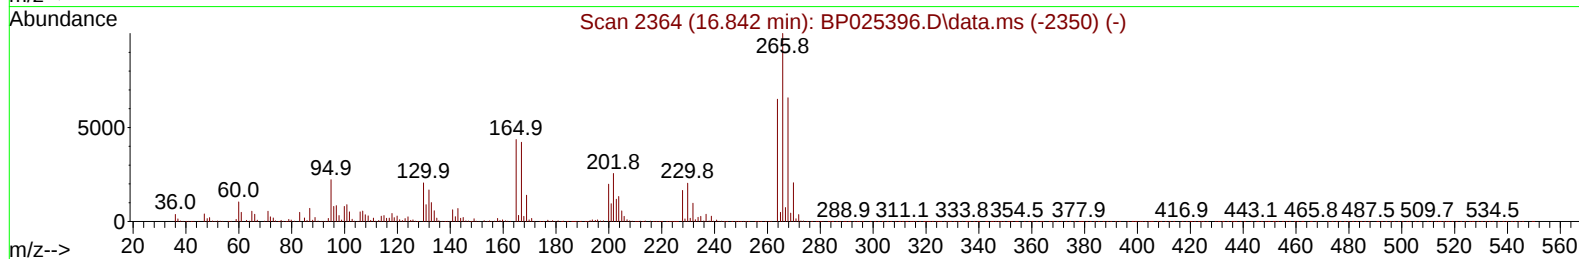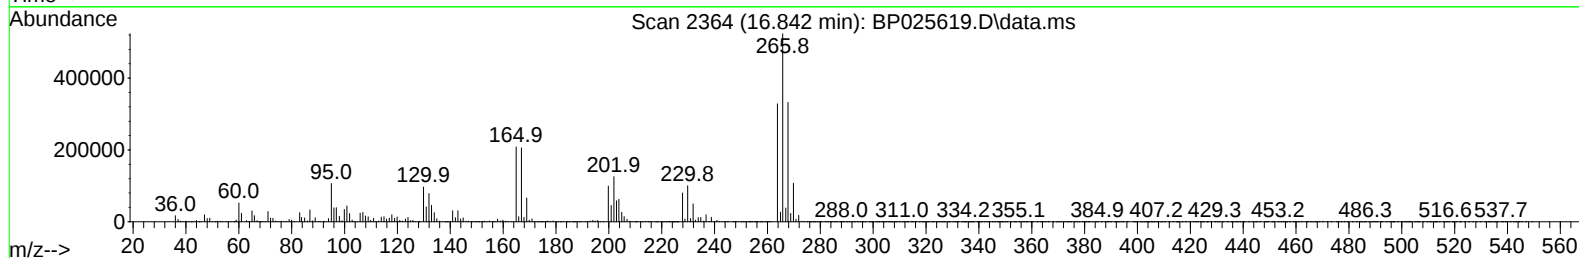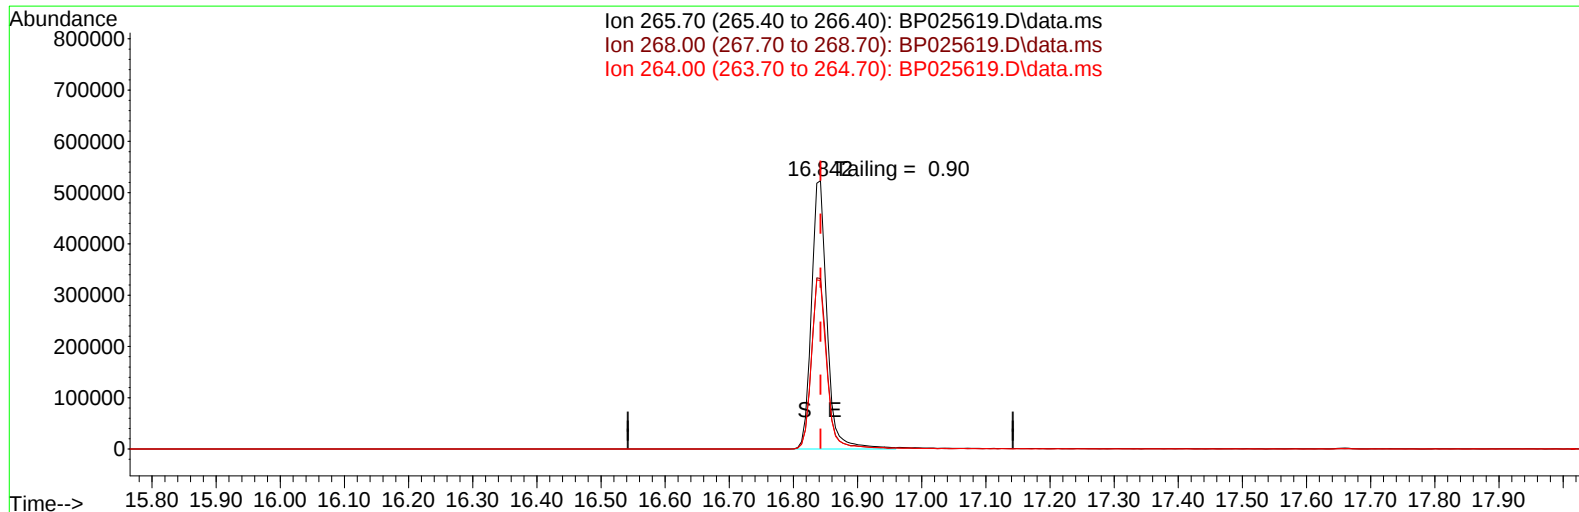

TIC: BP025619.D\data.ms

(70) Pentachlorophenol (C)

16.842min (-0.000) 584297.48 ng




response 893451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	63.49
264.00	65.00	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082925\
Data File : BP025619.D
Acq On : 29 Aug 2025 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 29 12:15:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

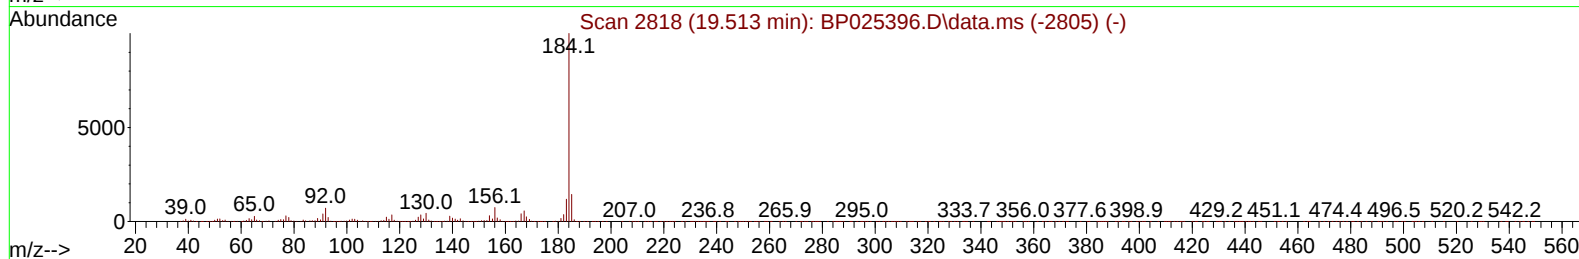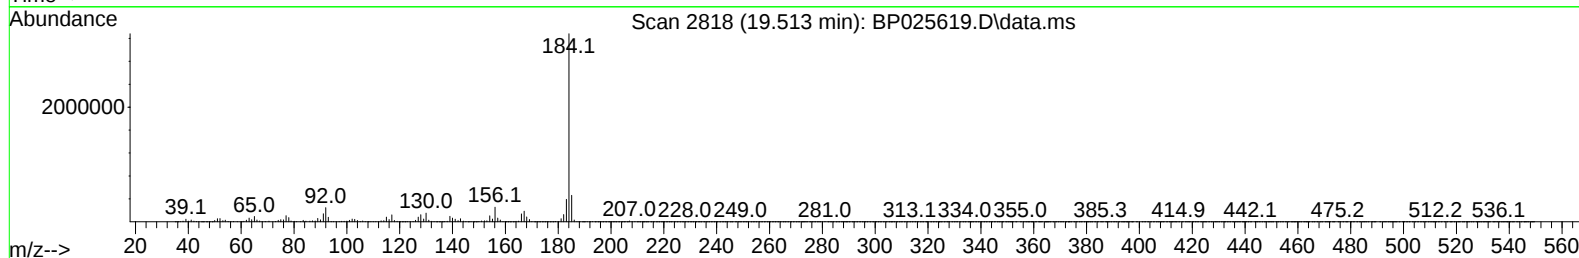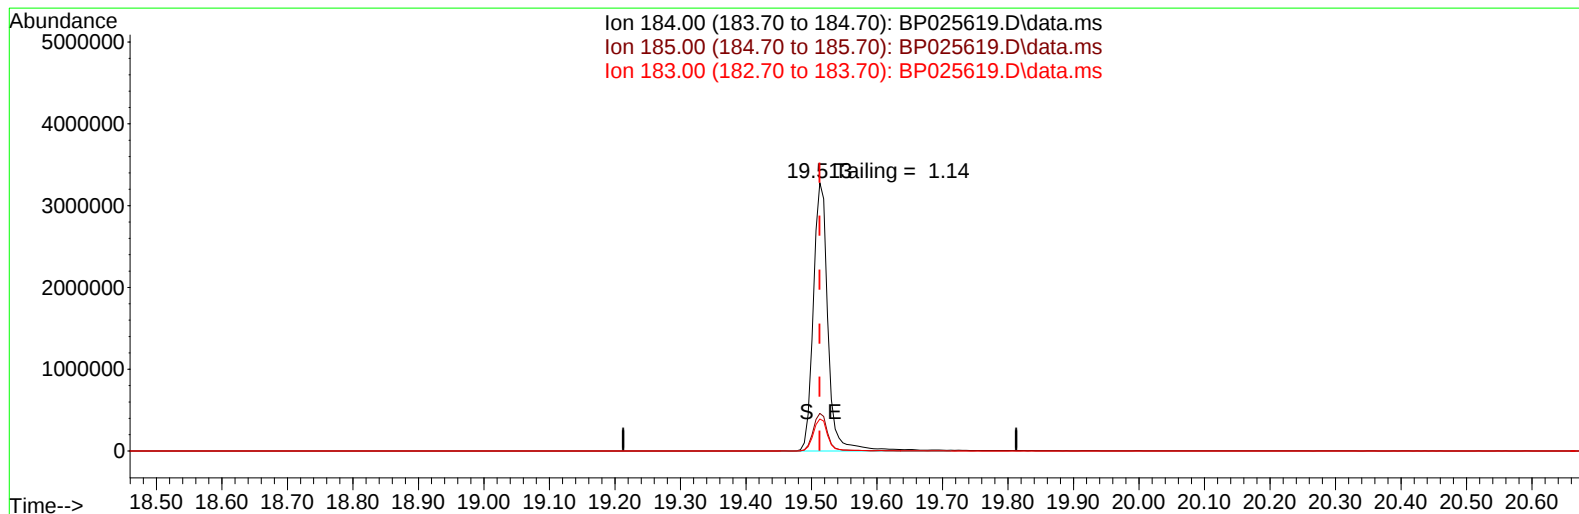

TIC: BP025619.D\data.ms

(77) Benzidine

19.513min (-0.000) 276434.71 ng

response 5103867

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.01
183.00	11.80	11.95
0.00	0.00	0.00