




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
 Data File : BP021774.D
 Acq On : 31 Aug 2024 06:49
 Operator : RC/JU
 Sample : P3733-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44A1

Manual IntegrationsAPPROVED

Quant Time: Aug 31 07:15:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/02/2024
 Supervised By :mohammad ahmed 09/03/2024

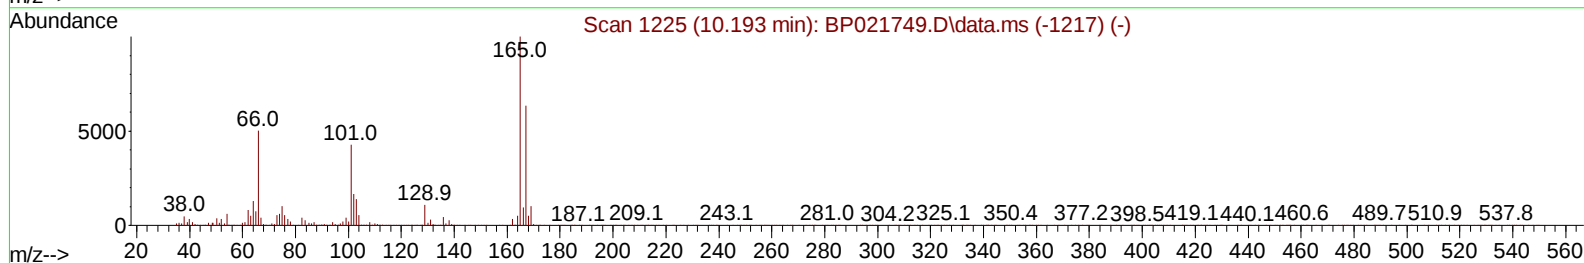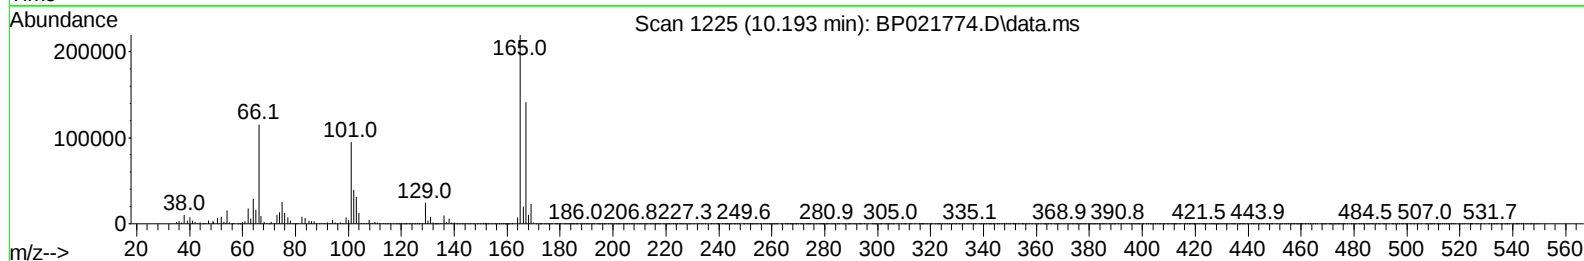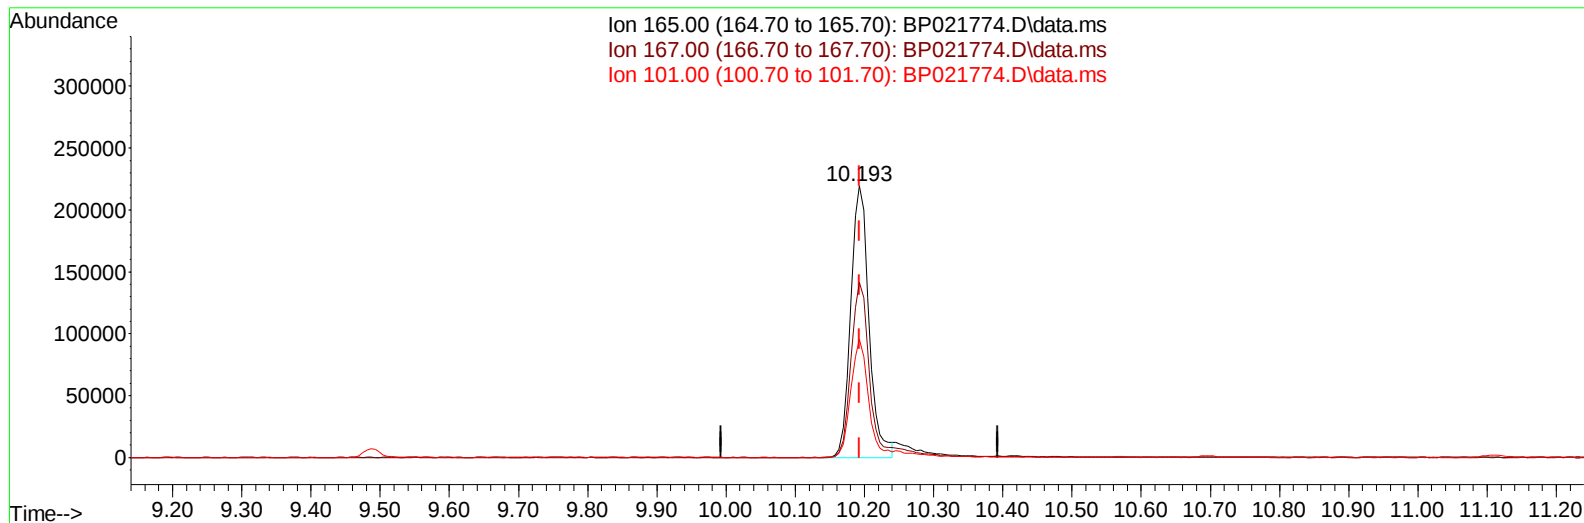

TIC: BP021774.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.193min (0.000) 23.29 ng/u1

response 398905

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	64.50
101.00	41.40	43.44
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021774.D
Acq On : 31 Aug 2024 06:49
Operator : RC/JU
Sample : P3733-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44A1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/03/2024

Quant Time: Aug 31 07:15:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

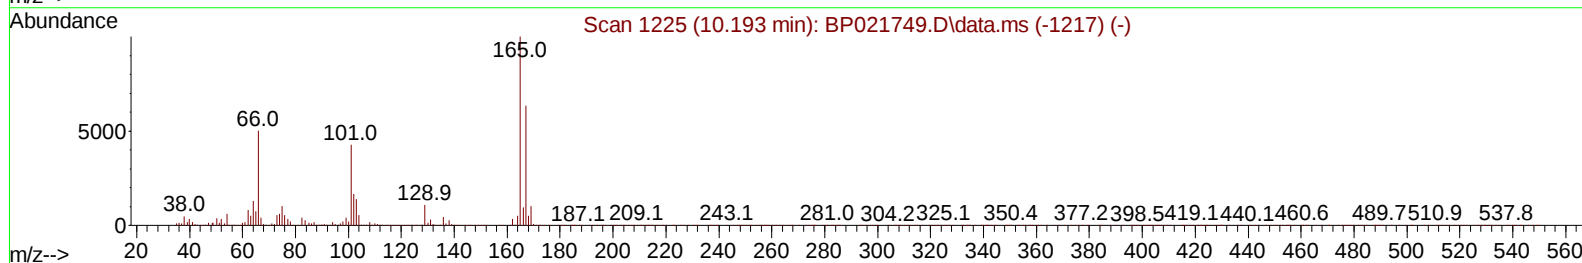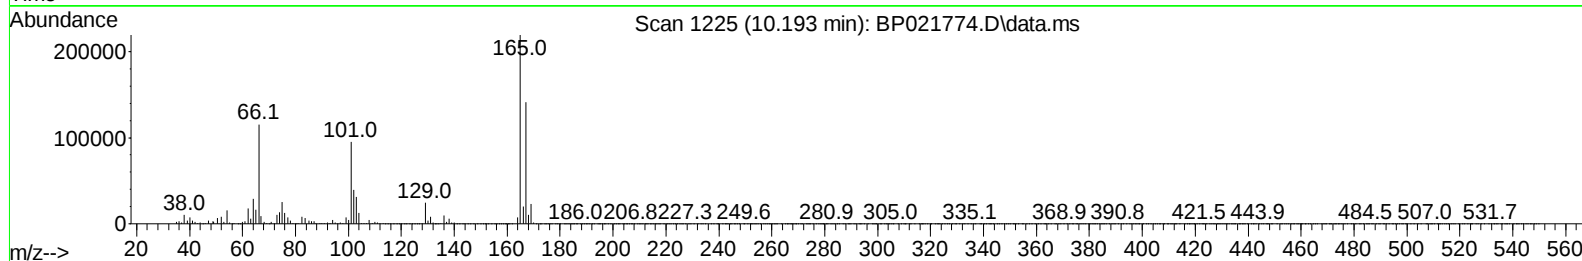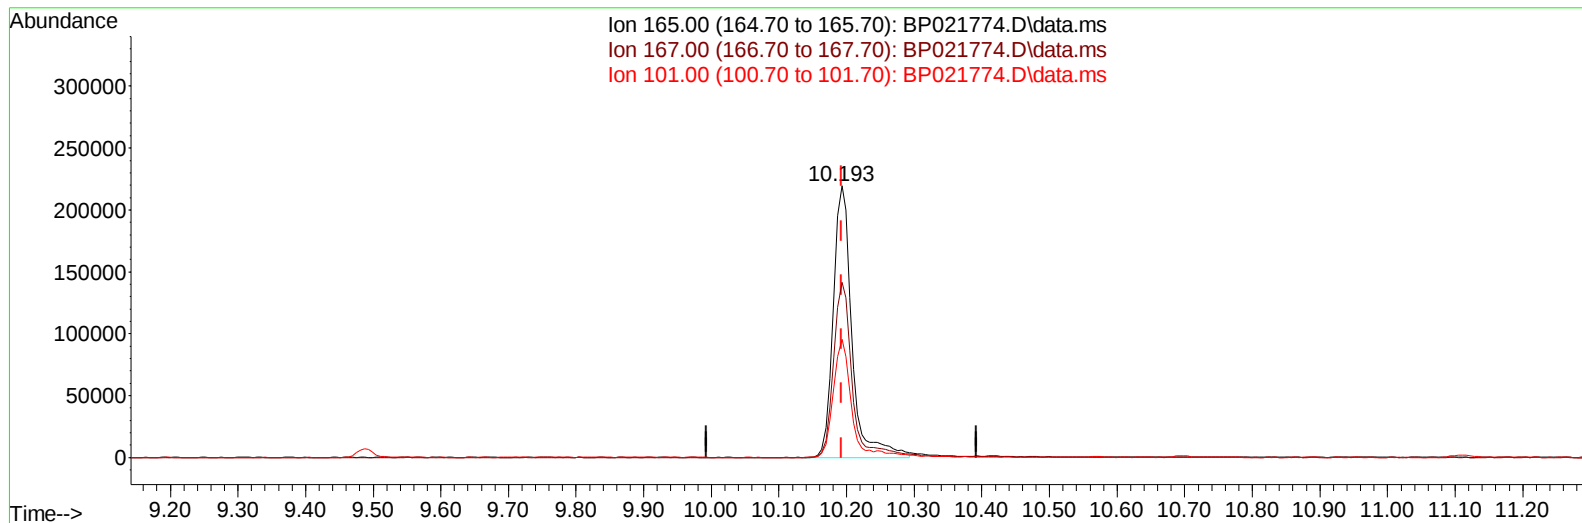

TIC: BP021774.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.193min (0.000) 24.71 ng/ul m

response 423263

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	64.50
101.00	41.40	43.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
 Data File : BP021774.D
 Acq On : 31 Aug 2024 06:49
 Operator : RC/JU
 Sample : P3733-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44A1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/02/2024
 Supervised By :mohammad ahmed 09/03/2024

Quant Time: Aug 31 07:15:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	265835	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	1064269	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	676768	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.239	188	1450345	20.000	ng/ul	0.01
79) Chrysene-d12	21.675	240	1467902	20.000	ng/ul	0.00
88) Perylene-d12	25.080	264	1677414	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	38213	4.772	ng/uL	0.00
4) Pyridine-d5	3.681	84	550217	23.757	ng/ul	0.00
7) Phenol-d5	6.952	99	711890	25.093	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.116	67	390651	25.303	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	472544	25.800	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	542788	24.759	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	224329	26.199	ng/ul	0.00
24) 2-Nitrophenol-d4	9.646	143	231449	26.630	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	423263m	24.713	ng/ul	0.00
31) 4-Chloroaniline-d4	10.699	131	639199	25.652	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1431835	27.650	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	1609491	27.683	ng/ul	0.00
54) 4-Nitrophenol-d4	14.640	143	223665	22.702	ng/ul	0.01
60) Fluorene-d10	15.445	176	1233109	28.324	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	146977	18.425	ng/ul	0.00
73) Anthracene-d10	17.328	188	1971818	28.647	ng/ul	-0.01
81) Pyrene-d10	19.698	212	2439689	29.075	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.845	264	2612857	29.212	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021774.D
Acq On : 31 Aug 2024 06:49
Operator : RC/JU
Sample : P3733-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44A1

Manual IntegrationsAPPROVED

Quant Time: Aug 31 07:15:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/02/2024
Supervised By :mohammad ahmed 09/03/2024

