




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021775.D
Acq On : 31 Aug 2024 07:32
Operator : RC/JU
Sample : P3733-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44A2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/03/2024
Supervised By :mohammad ahmed 09/03/2024

Quant Time: Sep 02 01:08:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

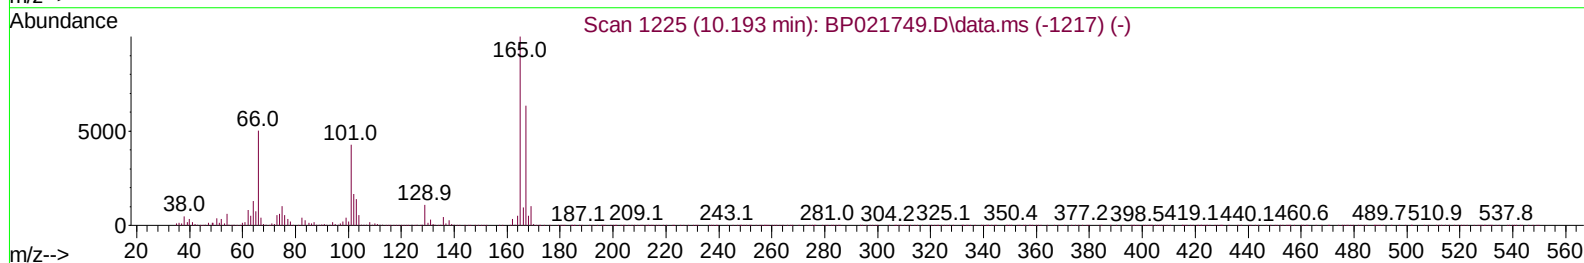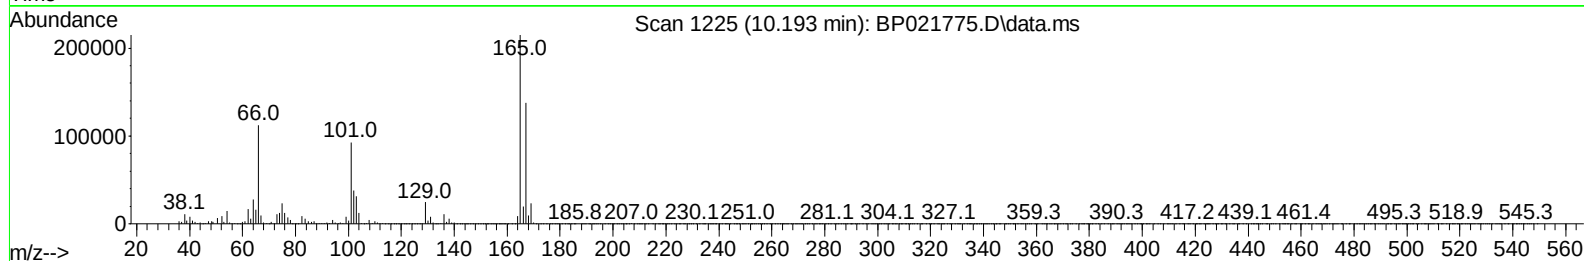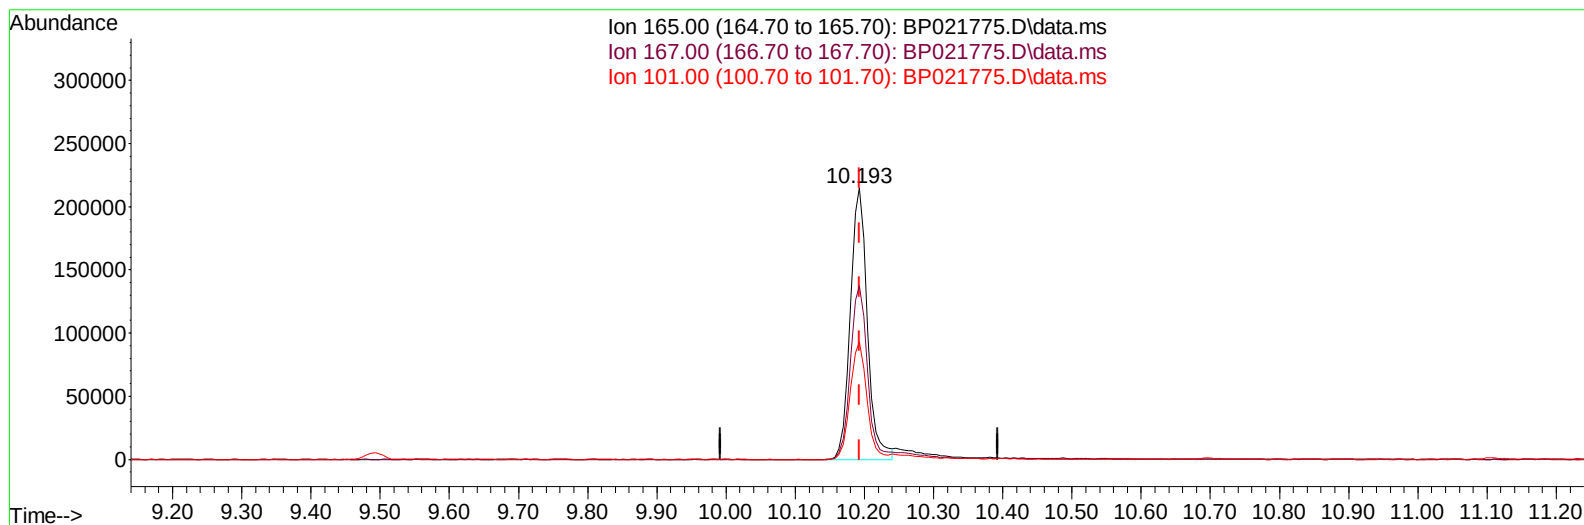

TIC: BP021775.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.193min (+ 0.000) 22.31 ng/ul

response 364098

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	64.09
101.00	41.40	43.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021775.D
Acq On : 31 Aug 2024 07:32
Operator : RC/JU
Sample : P3733-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44A2

Manual IntegrationsAPPROVED

Quant Time: Sep 02 01:08:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/03/2024
Supervised By :mohammad ahmed 09/03/2024

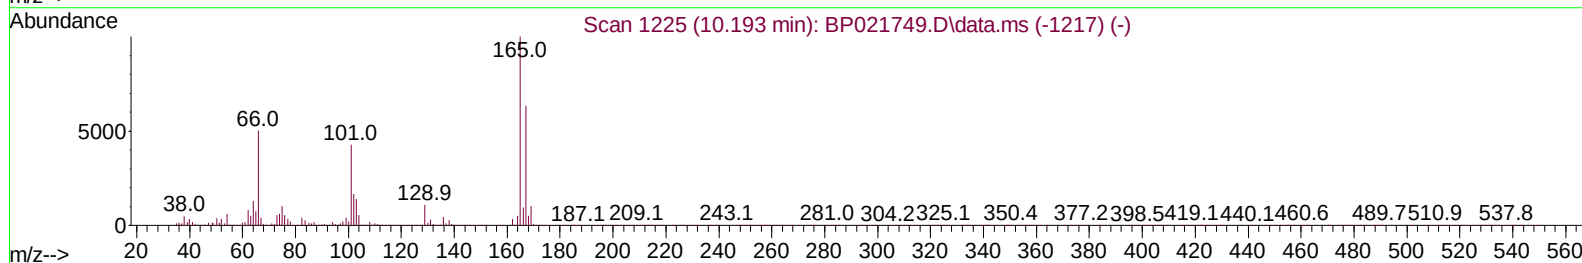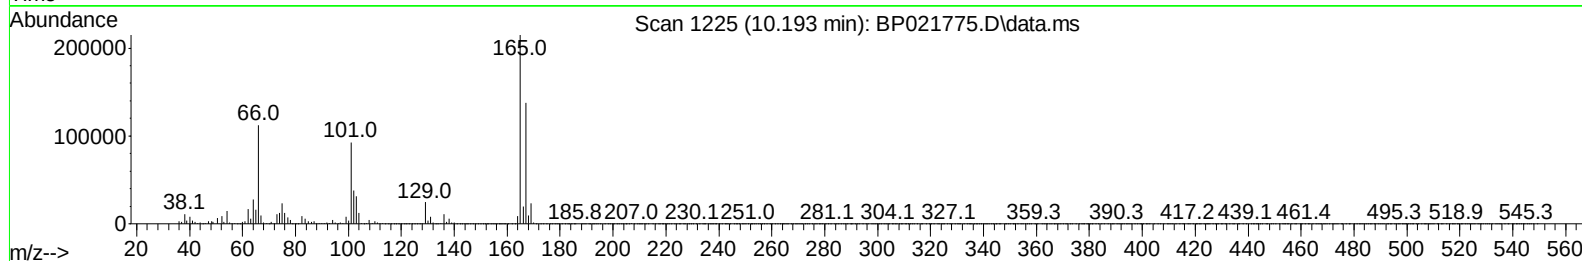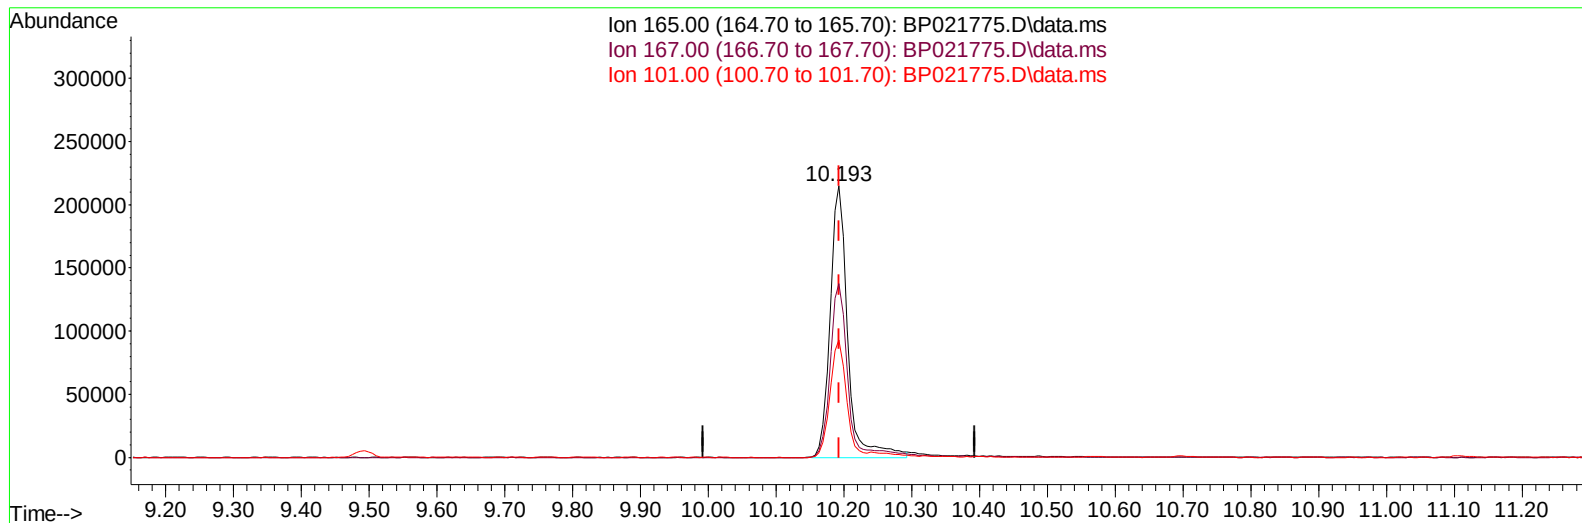

TIC: BP021775.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.193min (+ 0.000) 23.56 ng/ul m

response 384367

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	64.09
101.00	41.40	43.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
 Data File : BP021775.D
 Acq On : 31 Aug 2024 07:32
 Operator : RC/JU
 Sample : P3733-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44A2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/03/2024
 Supervised By :mohammad ahmed 09/03/2024

Quant Time: Sep 02 01:15:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	262103	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	1013897	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.434	164	610877	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	1280879	20.000	ng/ul	0.00
79) Chrysene-d12	21.669	240	1272549	20.000	ng/ul	0.00
88) Perylene-d12	25.069	264	1545779	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	36583	4.634	ng/uL	0.00
4) Pyridine-d5	3.687	84	513835	22.502	ng/ul	0.00
7) Phenol-d5	6.958	99	670042	23.954	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.111	67	370855	24.362	ng/ul	0.00
11) 2-Chlorophenol-d4	7.322	132	453923	25.136	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	501270	23.191	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	213062	26.119	ng/ul	0.00
24) 2-Nitrophenol-d4	9.646	143	211544	25.549	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	384367m	23.556	ng/ul	0.00
31) 4-Chloroaniline-d4	10.693	131	594921	25.061	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1274294	27.262	ng/ul	0.00
49) Acenaphthylene-d8	14.122	160	1430349	27.255	ng/ul	0.00
54) 4-Nitrophenol-d4	14.640	143	197657	22.226	ng/ul	0.01
60) Fluorene-d10	15.445	176	1080078	27.485	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	128153	18.191	ng/ul	0.00
73) Anthracene-d10	17.328	188	1720213	28.298	ng/ul	-0.01
81) Pyrene-d10	19.698	212	2118356	29.121	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.845	264	2389287	28.987	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021775.D
Acq On : 31 Aug 2024 07:32
Operator : RC/JU
Sample : P3733-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44A2

Manual IntegrationsAPPROVED

Quant Time: Sep 02 01:15:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/03/2024
Supervised By :mohammad ahmed 09/03/2024

