




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021779.D
Acq On : 31 Aug 2024 10:25
Operator : RC/JU
Sample : P3733-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44A6

Manual IntegrationsAPPROVED

Quant Time: Sep 02 01:09:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/03/2024
Supervised By :mohammad ahmed 09/03/2024

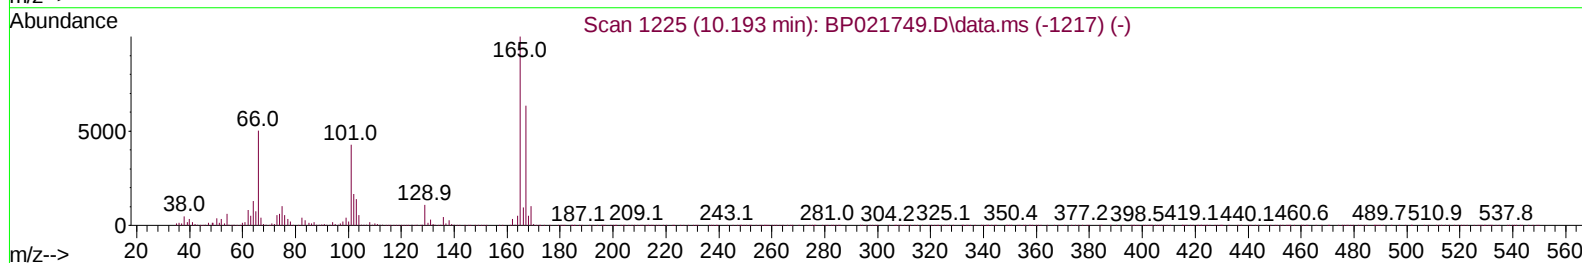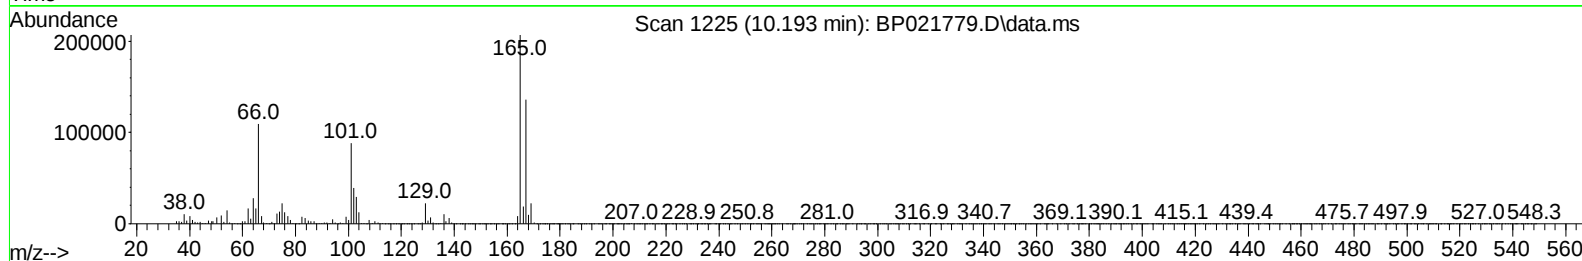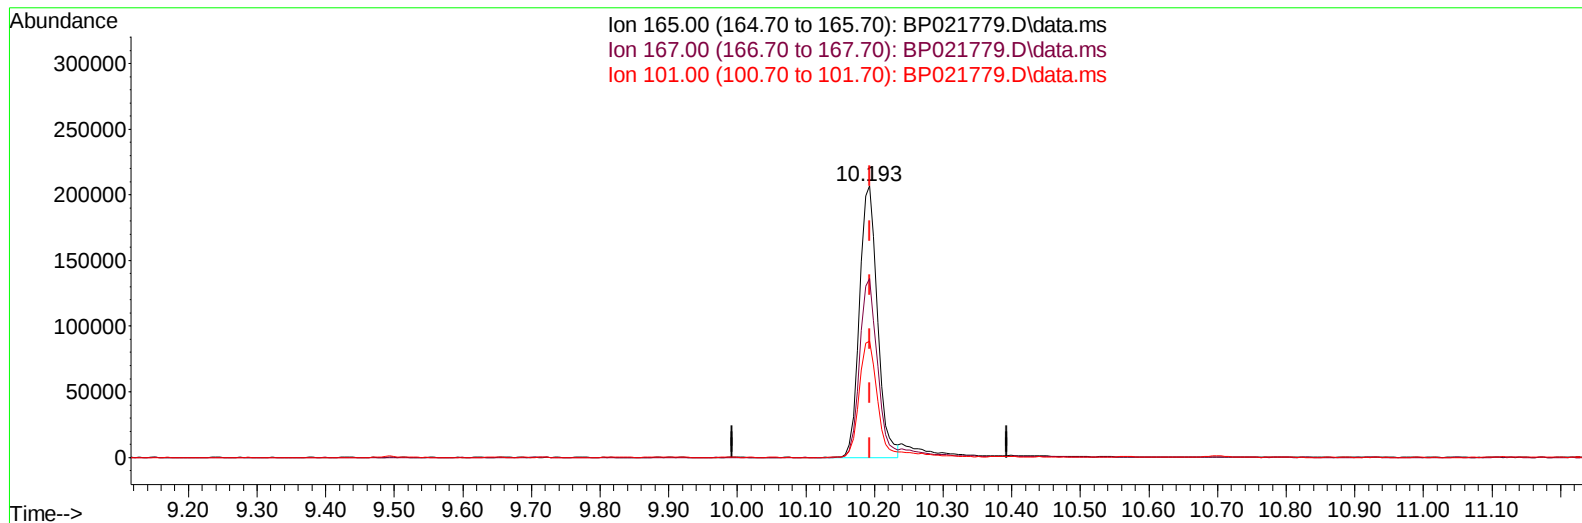

TIC: BP021779.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.193min (-0.000) 21.57 ng/u1

response 375453

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	65.86
101.00	41.40	42.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021779.D
Acq On : 31 Aug 2024 10:25
Operator : RC/JU
Sample : P3733-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44A6

Manual IntegrationsAPPROVED

Quant Time: Sep 02 01:09:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/03/2024
Supervised By :mohammad ahmed 09/03/2024

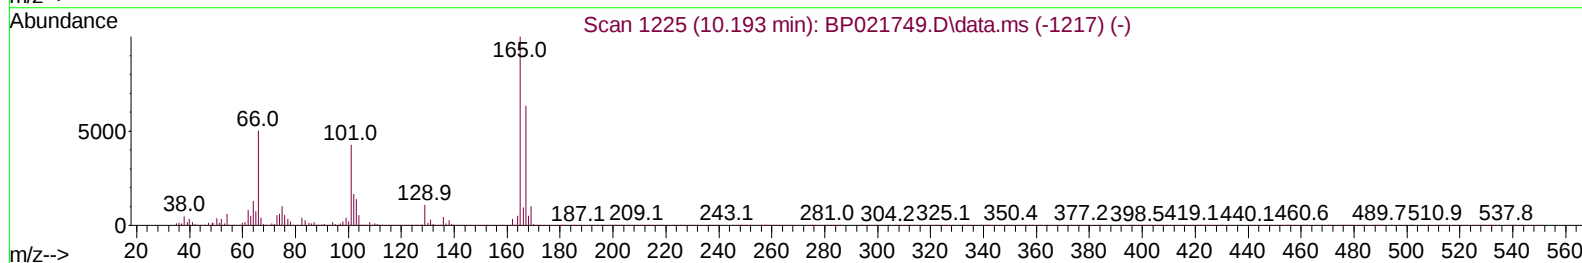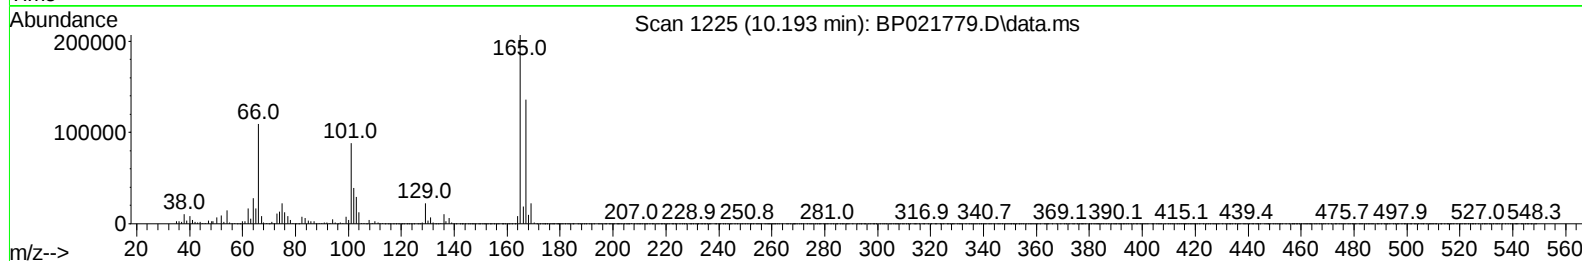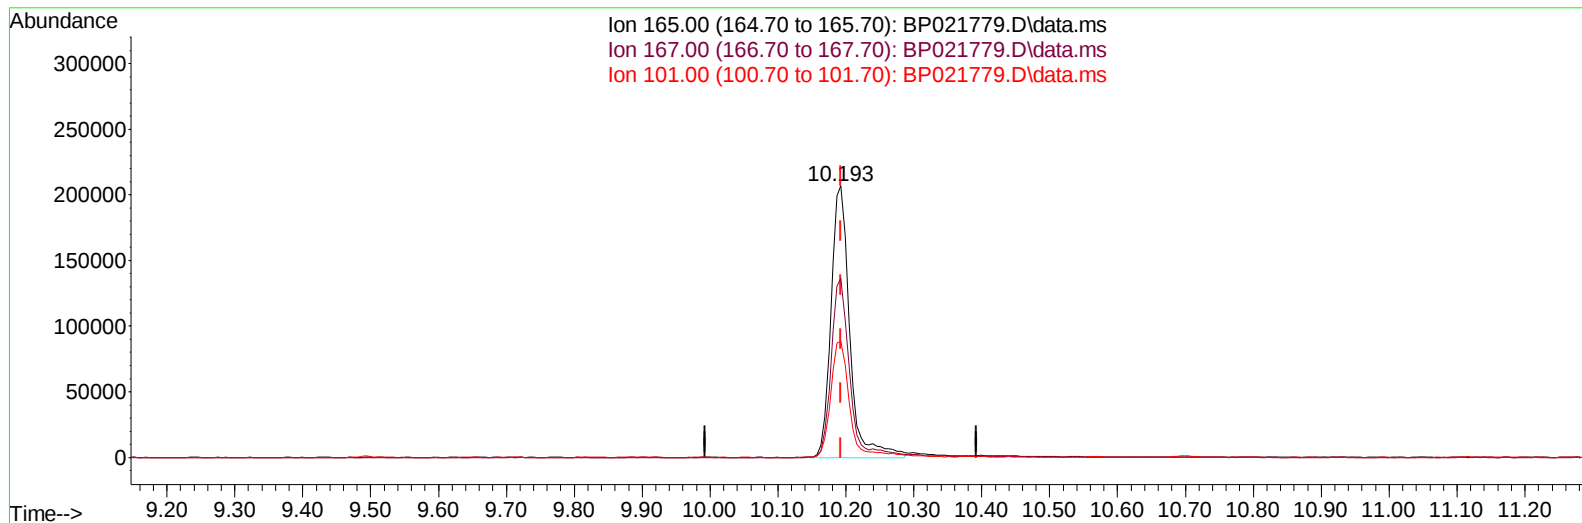

TIC: BP021779.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.193min (-0.000) 22.77 ng/ul m

response 396342

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	65.86
101.00	41.40	42.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
 Data File : BP021779.D
 Acq On : 31 Aug 2024 10:25
 Operator : RC/JU
 Sample : P3733-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44A6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/03/2024
 Supervised By :mohammad ahmed 09/03/2024

Quant Time: Sep 02 01:43:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 29 23:56:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	273709	20.000	ng/ul	0.00
20) Naphthalene-d8	10.563	136	1081385	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	676661	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.239	188	1443302	20.000	ng/ul	0.01
79) Chrysene-d12	21.692	240	1463319	20.000	ng/ul	0.02
88) Perylene-d12	25.092	264	1658508	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	34127	4.139	ng/uL	0.00
4) Pyridine-d5	3.687	84	498843	20.919	ng/ul	0.00
7) Phenol-d5	6.952	99	657614	22.513	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	373249	23.480	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	444630	23.577	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	516692	22.891	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	214140	24.613	ng/ul	0.00
24) 2-Nitrophenol-d4	9.646	143	216535	24.519	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	396342m	22.774	ng/ul	0.00
31) 4-Chloroaniline-d4	10.698	131	610611	24.117	ng/ul	0.00
46) Dimethylphthalate-d6	13.828	166	1472783	28.445	ng/ul	-0.01
49) Acenaphthylene-d8	14.116	160	1591180	27.372	ng/ul	0.00
54) 4-Nitrophenol-d4	14.628	143	205929	20.905	ng/ul	0.00
60) Fluorene-d10	15.439	176	1228554	28.224	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	149835	18.875	ng/ul	0.00
73) Anthracene-d10	17.339	188	1934781	28.246	ng/ul	0.00
81) Pyrene-d10	19.710	212	2342271	28.001	ng/ul	0.02
92) Benzo(a)pyrene-d12	24.857	264	2543337	28.759	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021779.D
Acq On : 31 Aug 2024 10:25
Operator : RC/JU
Sample : P3733-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44A6

Manual IntegrationsAPPROVED

Quant Time: Sep 02 01:43:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 29 23:56:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/03/2024
Supervised By :mohammad ahmed 09/03/2024

