

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
 Data File : BP021756.D
 Acq On : 30 Aug 2024 17:00
 Operator : RC/JU
 Sample : PB163016BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK016

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	11	rVB	136717	144071	2.06%	0.213%
2	3.117	18	22	26	rVB	20081	25429	0.36%	0.038%
3	3.269	44	48	54	rVB	80648	103035	1.47%	0.152%
4	3.687	114	119	133	rBV	1012514	1435797	20.55%	2.119%
5	4.016	171	175	179	rVB	19997	25351	0.36%	0.037%
6	6.957	667	675	685	rBV	1149898	1828642	26.17%	2.699%
7	7.116	695	702	711	rVB	941260	1453739	20.81%	2.146%
8	7.322	730	737	746	rBV	1080563	1722296	24.65%	2.542%
9	7.787	807	816	824	rBV	907165	1419788	20.32%	2.096%
10	8.487	927	935	945	rBV	1319647	2211678	31.66%	3.265%
11	8.934	1000	1011	1022	rBV	975132	1696122	24.28%	2.504%
12	9.369	1080	1085	1090	rBV9	3650	7258	0.10%	0.011%
13	9.651	1123	1133	1145	rBV	814222	1334571	19.10%	1.970%
14	10.193	1217	1225	1252	rBV	1014892	2071698	29.65%	3.058%
15	10.575	1282	1290	1298	rBV	1128831	1934928	27.69%	2.856%
16	10.704	1304	1312	1332	rVB	1030896	1990732	28.49%	2.938%
17	11.369	1421	1425	1429	rBV7	5064	8376	0.12%	0.012%
18	12.163	1553	1560	1569	rBV3	17451	38849	0.56%	0.057%
19	12.375	1588	1596	1600	rBV10	3096	8291	0.12%	0.012%
20	13.828	1836	1843	1856	rBV	2000114	3186412	45.61%	4.703%
21	14.122	1883	1893	1911	rBV2	2114863	3667235	52.49%	5.413%
22	14.434	1938	1946	1957	rBV	1743531	2662776	38.11%	3.930%
23	14.516	1957	1960	1968	rVB10	6052	12052	0.17%	0.018%
24	14.639	1974	1981	2001	rBV	809421	1725891	24.70%	2.548%
25	14.851	2014	2017	2022	rVB7	7337	11987	0.17%	0.018%
26	15.257	2082	2086	2093	rBV10	3478	7810	0.11%	0.012%
27	15.439	2110	2117	2131	rBV	3157907	4692921	67.17%	6.927%
28	15.557	2131	2137	2154	rVV	894537	1404506	20.10%	2.073%
29	15.686	2155	2159	2165	rVB5	13203	29441	0.42%	0.043%
30	16.251	2250	2255	2261	rVB10	8316	14283	0.20%	0.021%
31	17.239	2416	2423	2432	rBV	2365884	3447939	49.35%	5.089%
32	17.333	2432	2439	2452	rVV2	3662234	5334124	76.35%	7.874%
33	17.933	2539	2541	2545	rVB5	9714	7785	0.11%	0.011%
34	18.180	2579	2583	2589	rBV9	21368	41253	0.59%	0.061%
35	18.298	2600	2603	2608	rVB7	15350	20101	0.29%	0.030%
36	19.251	2762	2765	2771	rBV	42995	61708	0.88%	0.091%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021756.D
Acq On : 30 Aug 2024 17:00
Operator : RC/JU
Sample : PB163016BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK016

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Title : SVOA CALIBRATION

37	19.327	2775	2778	2782	rVB	37963	54108	0.77%	0.080%
38	19.704	2836	2842	2850	rBV	4730854	6696187	95.84%	9.884%
39	21.680	3172	3178	3188	rBV	2595572	4062427	58.15%	5.996%
40	24.857	3709	3718	3734	rVB2	2331161	6986700	100.00%	10.313%
41	25.092	3750	3758	3771	rVB	1497497	4158591	59.52%	6.138%




Sum of corrected areas: 67746888

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021756.D
Acq On : 30 Aug 2024 17:00
Operator : RC/JU
Sample : PB163016BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK016

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

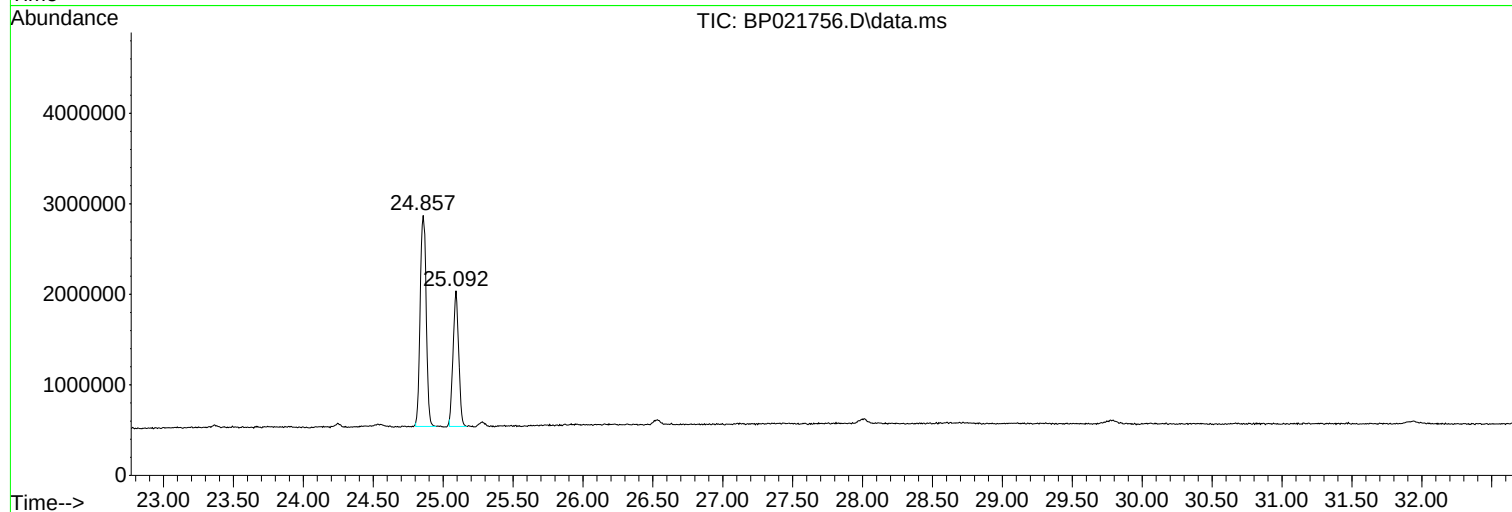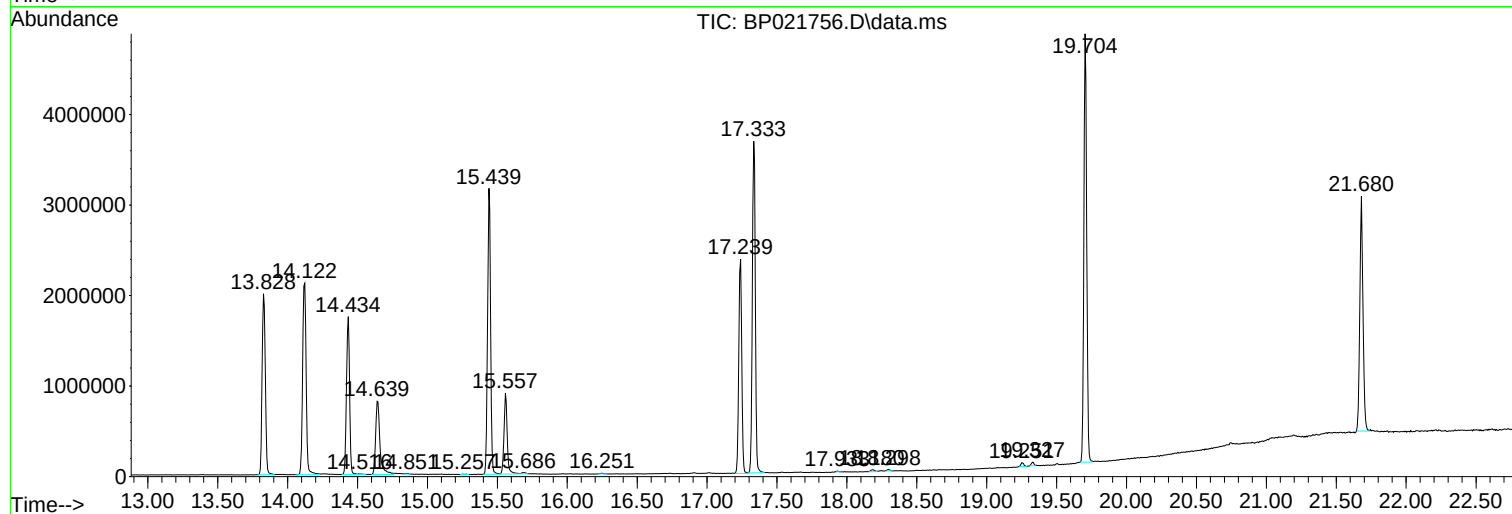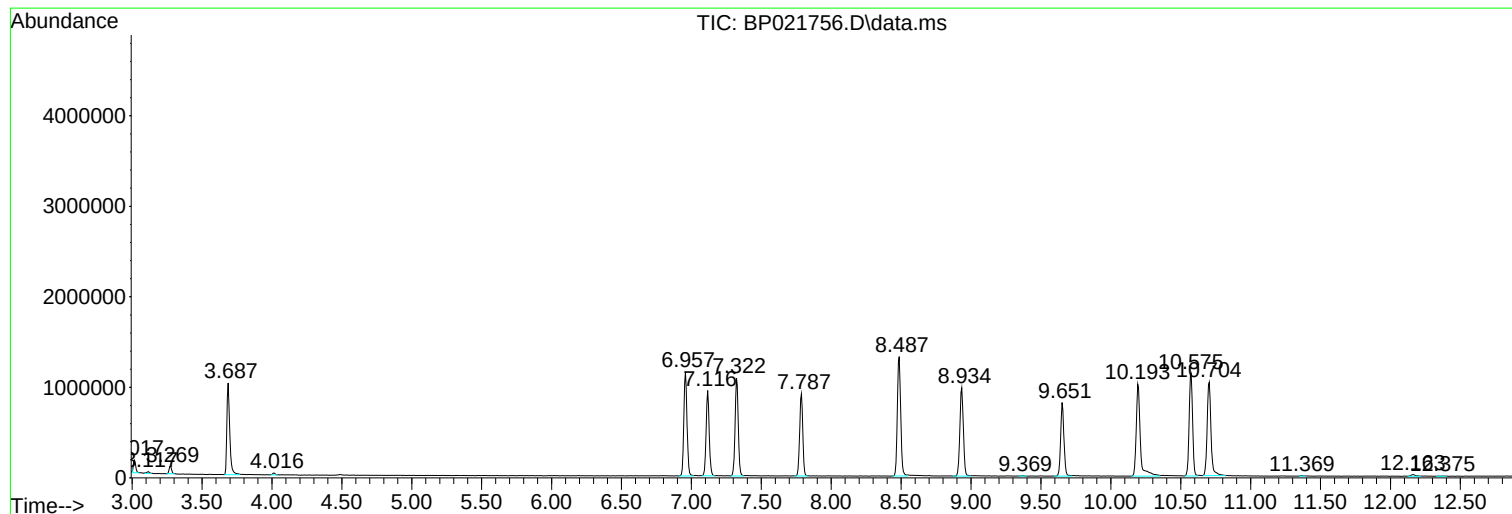

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021756.D
Acq On : 30 Aug 2024 17:00
Operator : RC/JU
Sample : PB163016BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK016










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.017	2.03 ng/ul	144071	1,4-Dichlorobenzene-d4	7.787

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

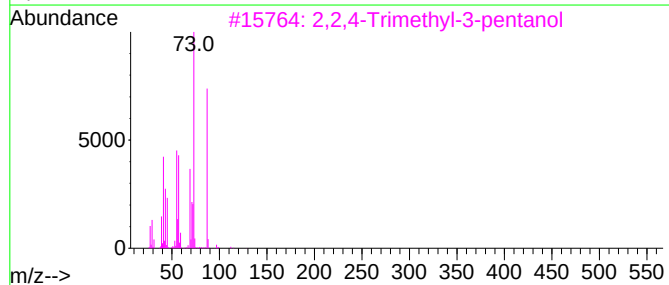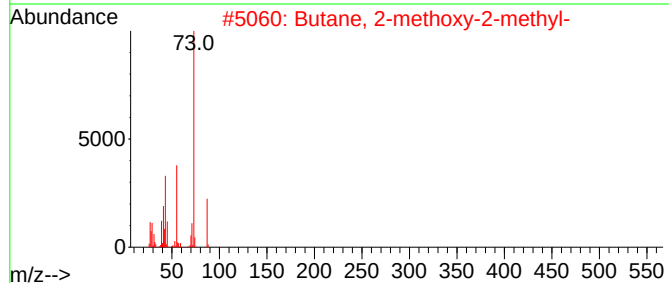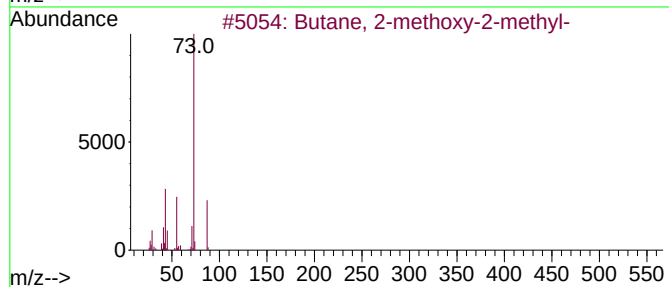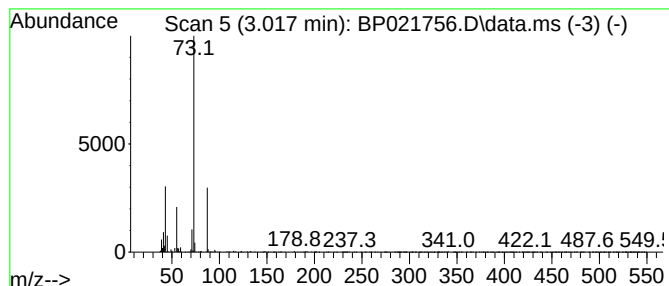

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP083024\
Data File : BP021756.D
Acq On : 30 Aug 2024 17:00
Operator : RC/JU
Sample : PB163016BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK016

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP082324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.017	2.0	ng/ul	144071	1	7.787	1419790	20.0